
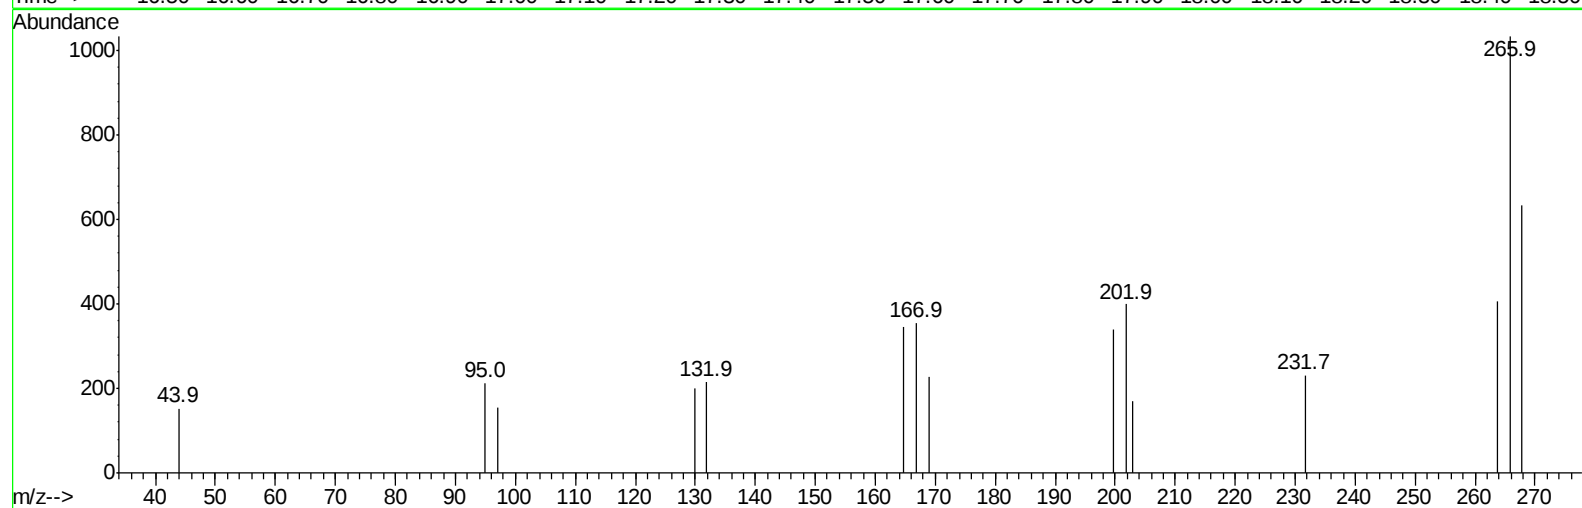


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062717\
 Data File : BG027700.D
 Acq On : 27 Jun 2017 15:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 02:58:12 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 21 18:52:15 2017
 Response via : Initial Calibration

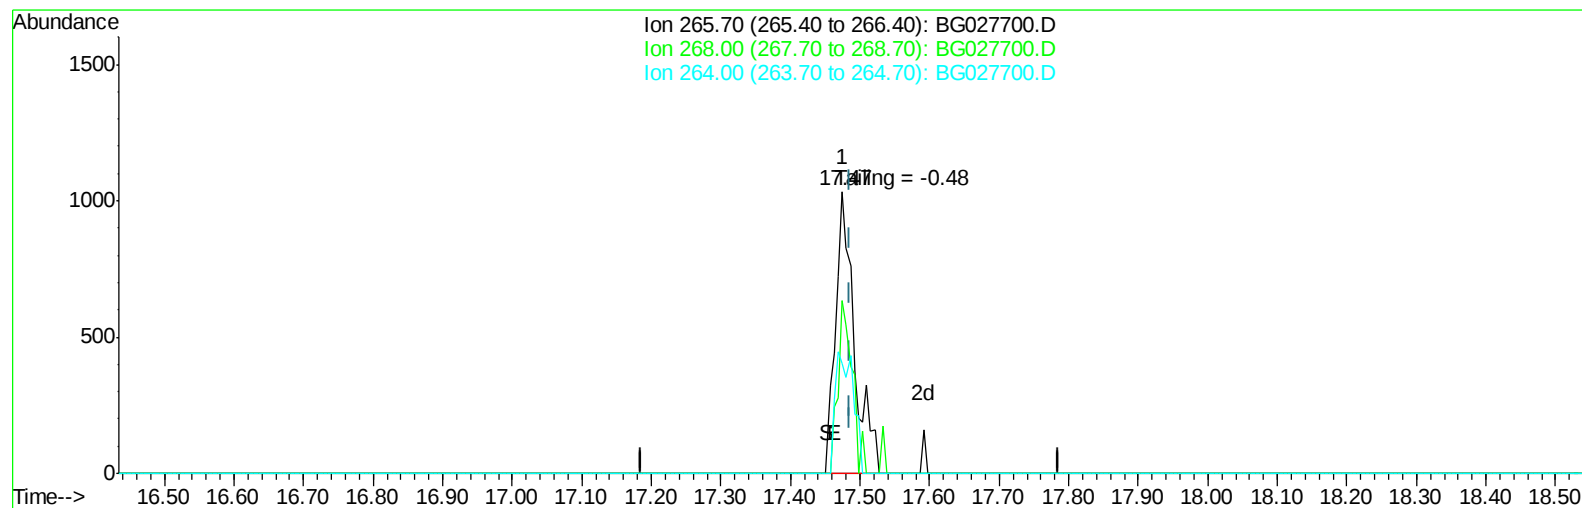

TIC: BG027700.D

(69) Pentachlorophenol (C)



17.474min (-0.011) 0.00ng m

response 1943

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	61.28
264.00	62.60	39.30#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062717\
Data File : BG027700.D
Acq On : 27 Jun 2017 15:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 02:58:12 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 21 18:52:15 2017
Response via : Initial Calibration

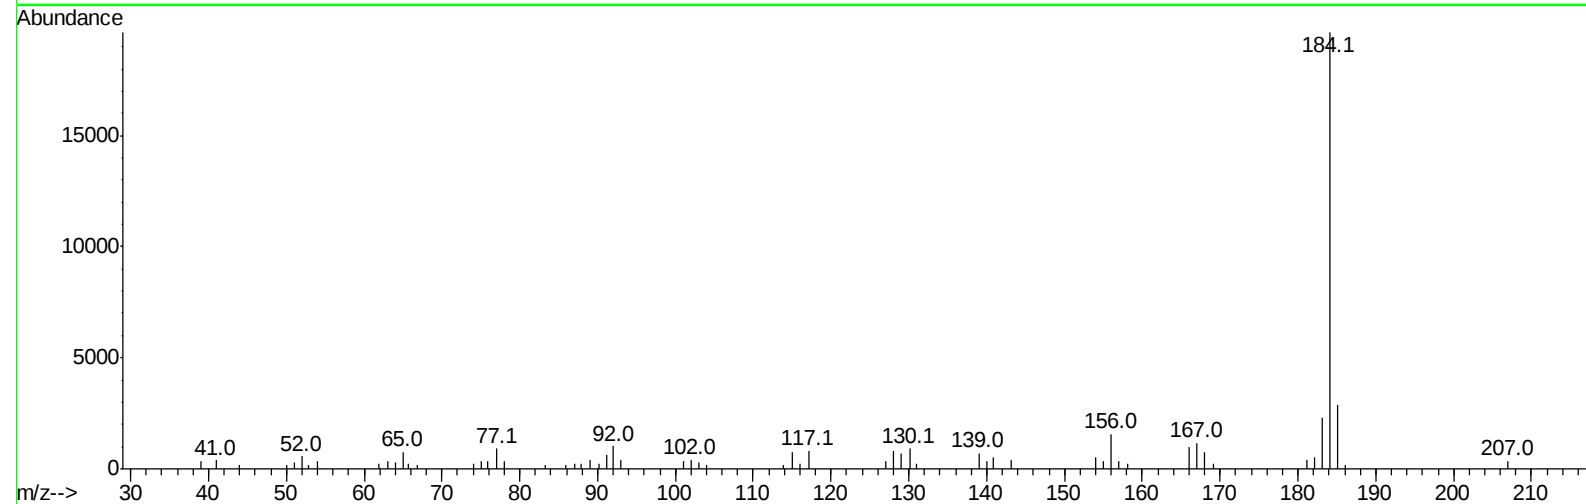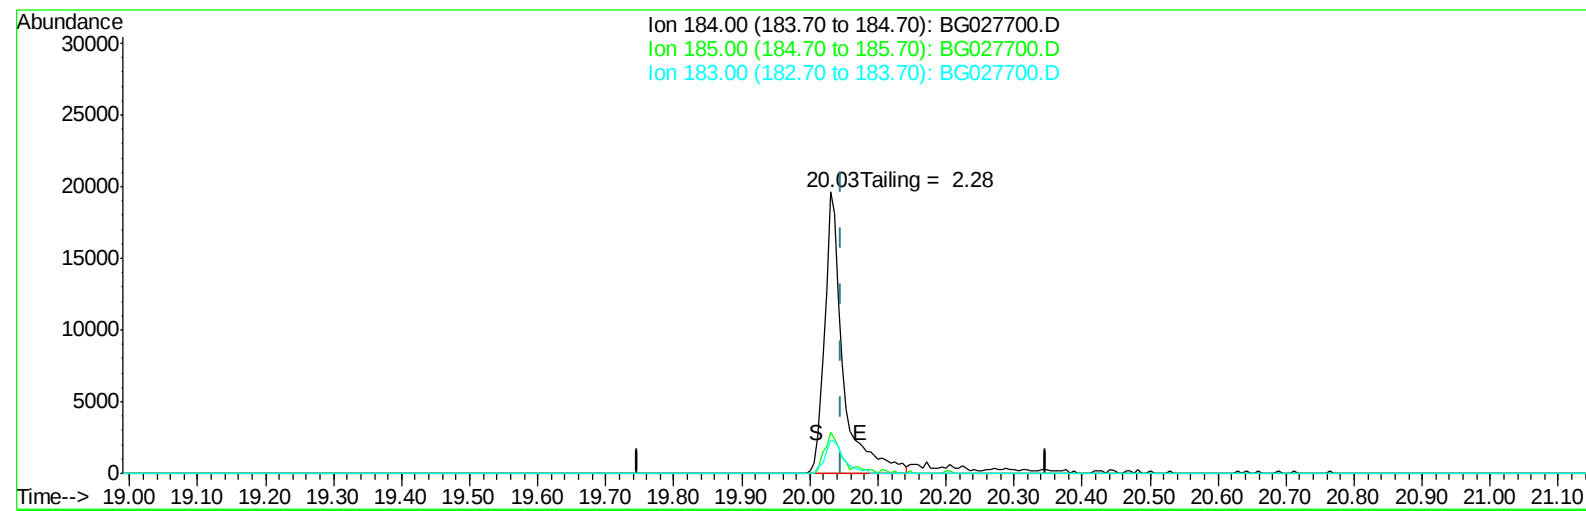

TIC: BG027700.D

(76) Benzidine

20.030min (-0.017) 0.00ng

response 37409

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.53
183.00	13.80	11.80
0.00	0.00	0.00