


Data Path : Z:\HPCHEM1\BNA G\Data\BG062717\
 Data File : BG027700.D
 Acq On : 27 Jun 2017 15:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 21 18:52:15 2017

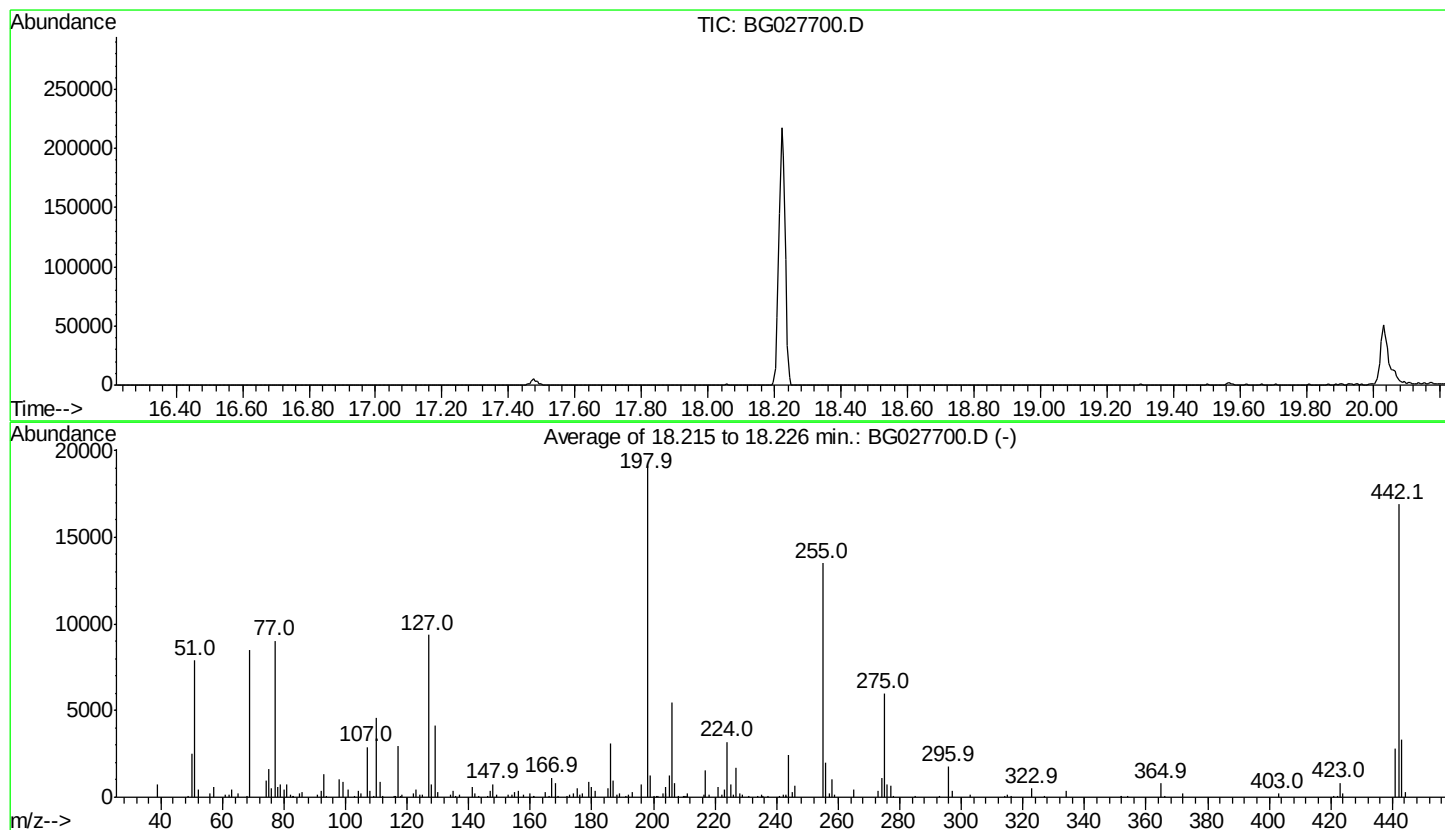

AutoFind: Scans 2438, 2439, 2440; Background Corrected with Scan 2432

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	7869	PASS
68	69	0.00	2	1.1	92	PASS
69	198	0.00	100	44.6	8528	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	9367	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19126	PASS
199	198	5	9	6.4	1226	PASS
275	198	10	60	31.1	5946	PASS
365	198	1	100	4.1	790	PASS
441	442	0.01	24	16.8	2834	PASS
442	198	50	100	88.4	16898	PASS
443	442	15	24	19.8	3343	PASS