

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062719\
 Data File : BG041499.D
 Acq On : 27 Jun 2019 22:07
 Operator : HP/JU
 Sample : K3552-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 M-6

Quant Time: Jun 28 05:53:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 27 13:25:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	26701	20.00	ng	0.00
21) Naphthalene-d8	10.85	136	96912	20.00	ng	0.00
39) Acenaphthene-d10	14.68	164	71440	20.00	ng	0.00
64) Phenanthrene-d10	17.43	188	191229	20.00	ng	0.00
76) Chrysene-d12	21.70	240	205965	20.00	ng	0.00
87) Perylene-d12	24.98	264	221361	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	188505	125.87	ng	0.00
7) Phenol-d6	7.19	99	272084	129.05	ng	0.00
23) Nitrobenzene-d5	9.21	82	192137	82.69	ng	0.00
42) 2,4,6-Tribromophenol	16.17	330	152909	125.36	ng	0.00
45) 2-Fluorobiphenyl	13.30	172	423598	76.09	ng	0.00
79) Terphenyl-d14	20.02	244	829871	85.62	ng	0.00
Target Compounds						
15) Benzyl Alcohol	8.35	79	3391	2.020	ng	# 45
19) n-Nitroso-di-n-propylamine	9.21	70	27802	17.679	ng	# 74
50) Dimethylphthalate	14.12	163	65043	10.005	ng	100
57) 2,4-Dinitrotoluene	14.68	165	9699	4.846	ng	# 22
67) 4-Bromophenyl-phenylether	16.17	248	10745	4.112	ng	# 1
77) Benzidine	20.02	184	13673	2.992	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG062719\
Data File : BG041499.D
Acq On : 27 Jun 2019 22:07
Operator : HP/JU
Sample : K3552-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
M-6

Quant Time: Jun 28 05:53:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

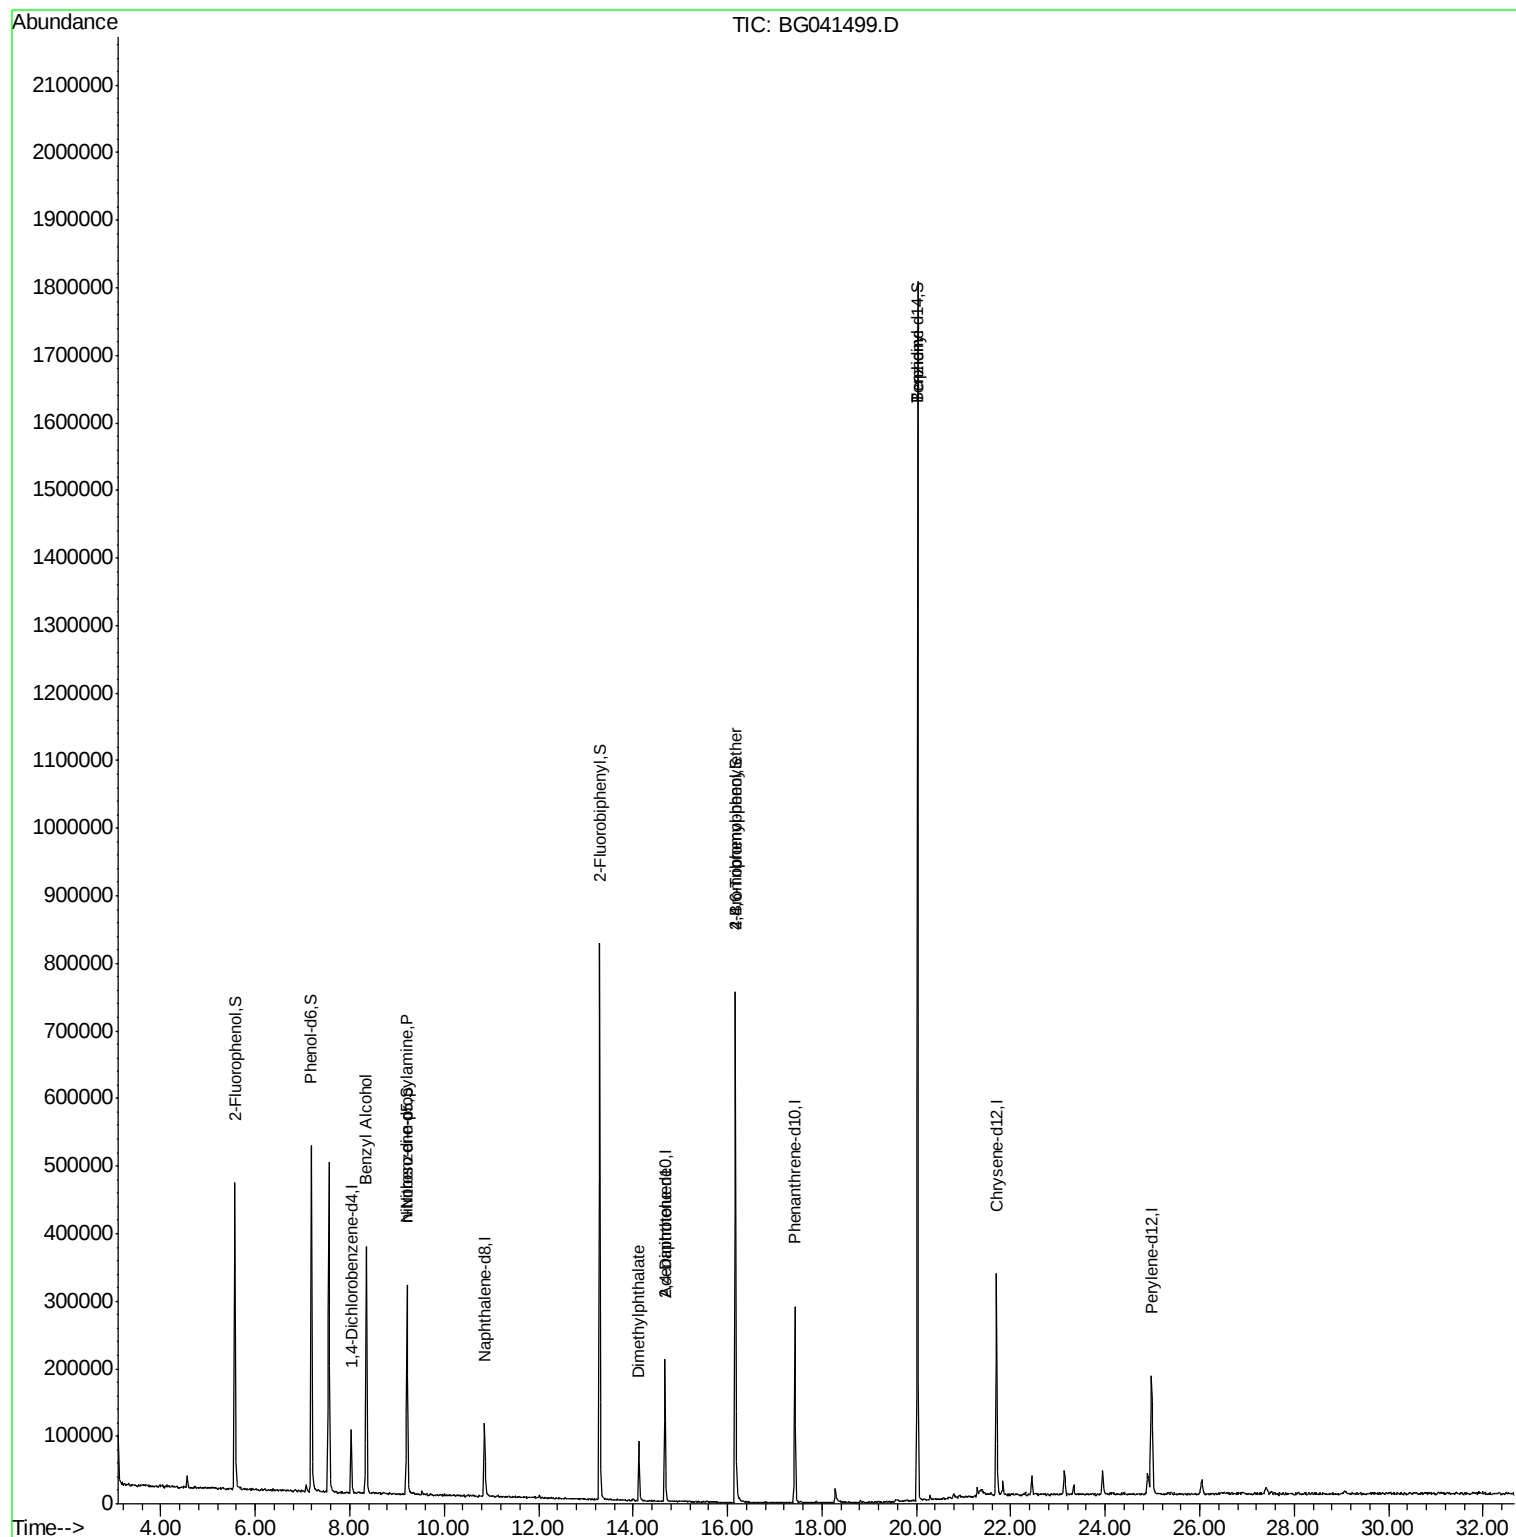

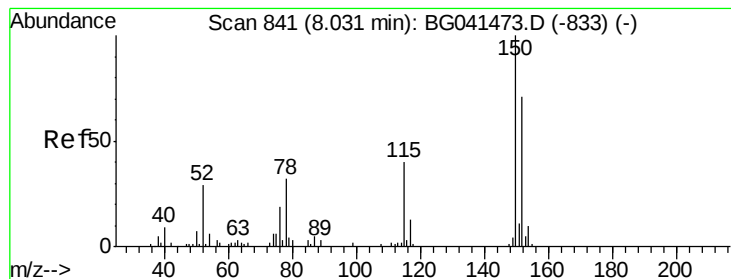

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 8.03 min Scan# 840

Delta R.T. -0.01 min

Lab File: BG041499.D

Acq: 27 Jun 2019 22:07

Instrument :

BNA_G

ClientSampleId :

M-6


Tgt Ion:152 Resp: 26701

Ion Ratio Lower Upper

152 100

150 142.0 112.4 168.6

115 57.9 44.6 66.8






Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

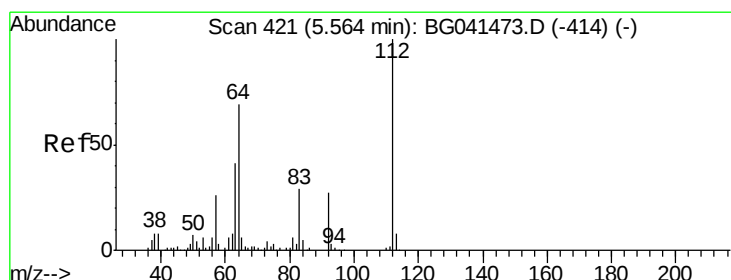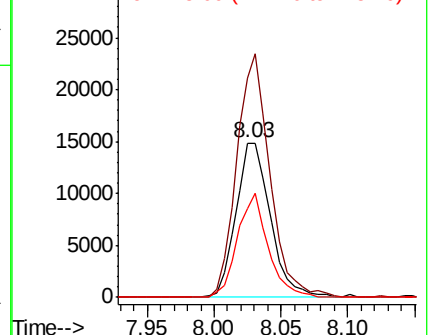

#5

2-Fluorophenol

Concen: 125.867 ng

RT: 5.57 min Scan# 422

Delta R.T. 0.01 min

Lab File: BG041499.D

Acq: 27 Jun 2019 22:07


Tgt Ion:112 Resp: 188505

Ion Ratio Lower Upper

112 100

64 65.4 55.1 82.7

63 38.1 32.4 48.6






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

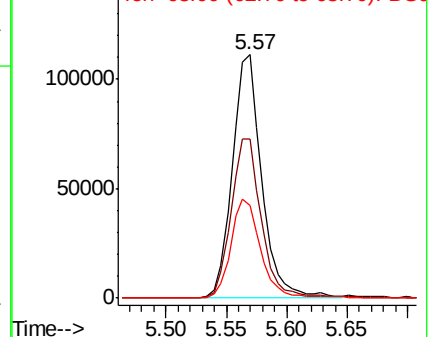

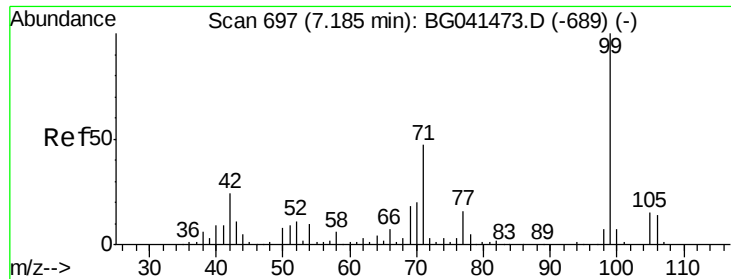

#7

Phenol-d6

Concen: 129.053 ng

RT: 7.19 min Scan# 698

Delta R.T. 0.01 min

Lab File: BG041499.D

Acq: 27 Jun 2019 22:07

Instrument :

BNA_G

ClientSampleId :

M-6


Tgt Ion: 99 Resp: 272084

Ion Ratio Lower Upper




99 100

42 22.4 19.0 28.6

71 44.6 37.4 56.2

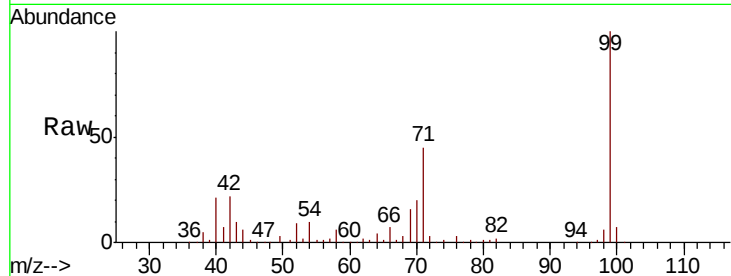

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

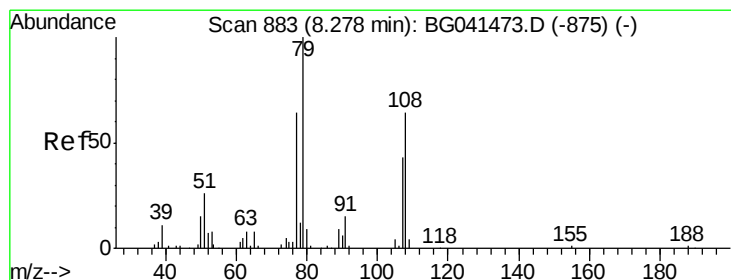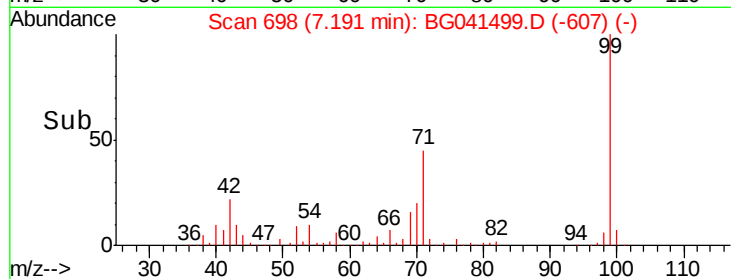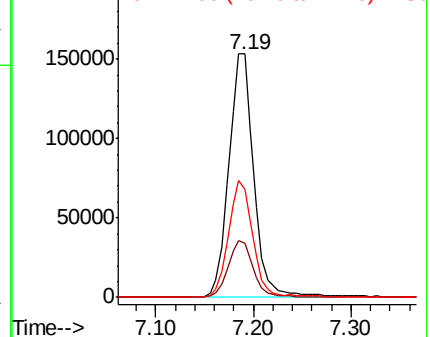

#15

Benzyl Alcohol

Concen: 2.020 ng

RT: 8.35 min Scan# 895

Delta R.T. 0.07 min

Lab File: BG041499.D

Acq: 27 Jun 2019 22:07


Tgt Ion: 79 Resp: 3391

Ion Ratio Lower Upper



79 100


108 42.3 51.4 77.0#

77 127.9 50.8 76.2#



Abundance Ion 79.00 (78.70 to 79.70): BGC
Ion 108.00 (107.70 to 108.70): BGC
Ion 77.00 (76.70 to 77.70): BGC




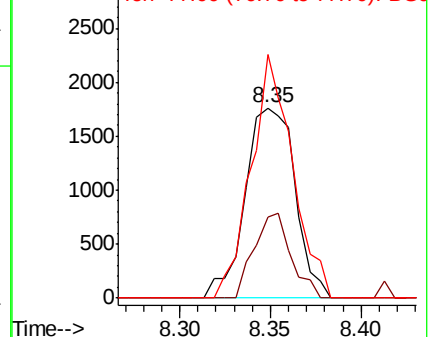




#19
n-Nitroso-di-n-propylamine
Concen: 17.679 ng
RT: 9.21 min Scan# 1042
Delta R.T. 0.38 min
Lab File: BG041499.D
Acq: 27 Jun 2019 22:07




Instrument :
BNA_G
ClientSampleId :
M-6


Tgt Ion: 70 Resp: 27802
Ion Ratio Lower Upper
70 100
42 48.2 52.6 78.8#
101 0.0 8.6 13.0#
130 2.7 16.6 25.0#

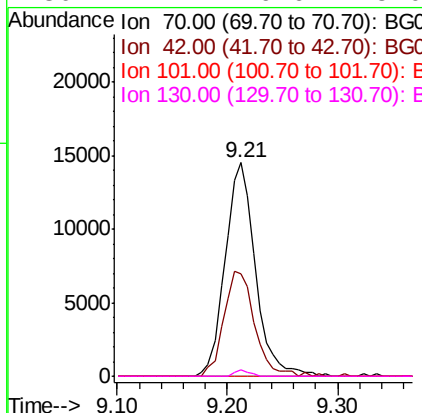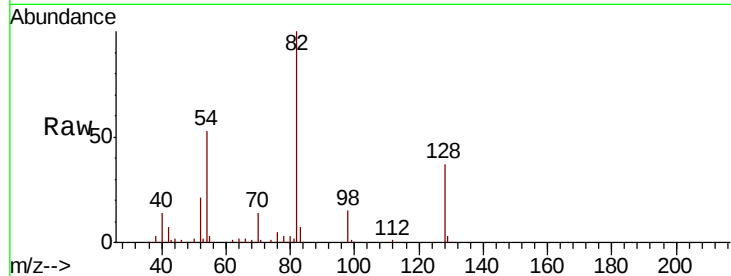

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.85 min Scan# 1321
Delta R.T. -0.01 min
Lab File: BG041499.D
Acq: 27 Jun 2019 22:07

Tgt Ion: 136 Resp: 96912
Ion Ratio Lower Upper
136 100
137 11.4 9.3 13.9
54 8.2 7.1 10.7
68 4.3 3.3 4.9


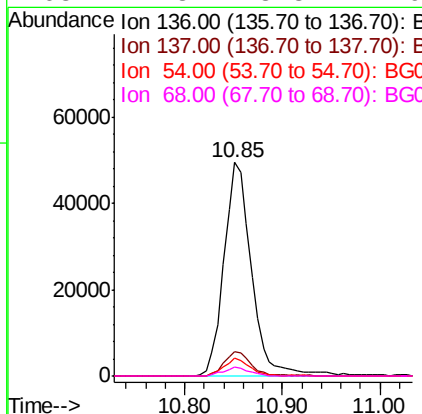

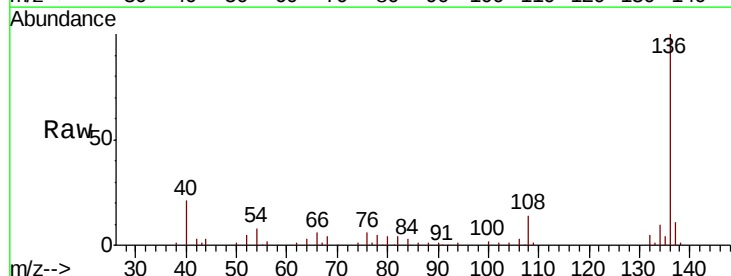




#23
Nitrobenzene-d5
Concen: 82.688 ng
RT: 9.21 min Scan# 1042
Delta R.T. -0.00 min
Lab File: BG041499.D
Acq: 27 Jun 2019 22:07




Instrument :
BNA_G
ClientSampleId :
M-6


Tgt Ion	Ratio	Lower	Upper
82	100		
128	37.2	30.9	46.3
54	52.8	42.2	63.2

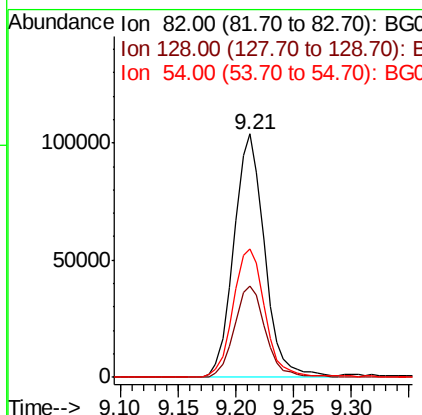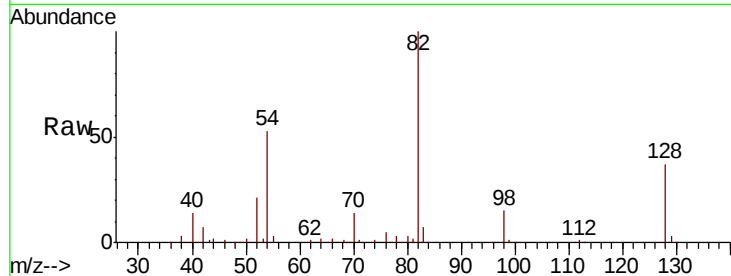

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.68 min Scan# 1972
Delta R.T. -0.00 min
Lab File: BG041499.D
Acq: 27 Jun 2019 22:07

Tgt Ion	Ratio	Lower	Upper
164	100		
162	110.5	84.4	126.6
160	47.0	38.8	58.2

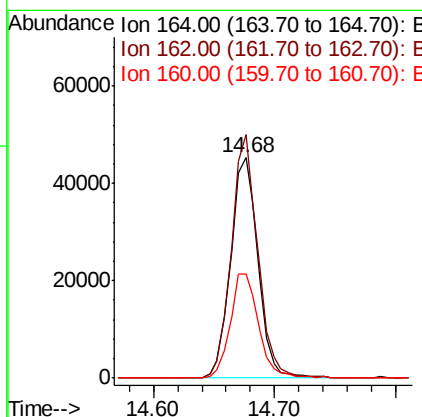


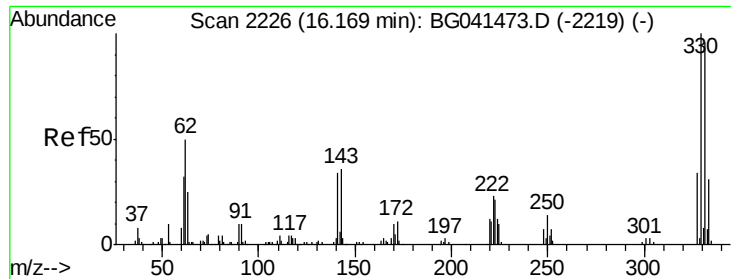




#42
 2,4,6-Tribromophenol
 Concen: 125.357 ng
 RT: 16.17 min Scan# 2226
 Delta R.T. -0.00 min
 Lab File: BG041499.D
 Acq: 27 Jun 2019 22:07

Instrument :
 BNA_G
 ClientSampleId :
 M-6

Tgt Ion:330 Resp: 152909
 Ion Ratio Lower Upper
 330 100
 332 95.0 75.5 113.3
 141 34.5 27.8 41.6




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

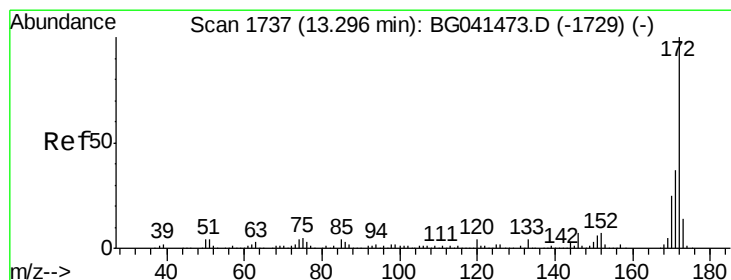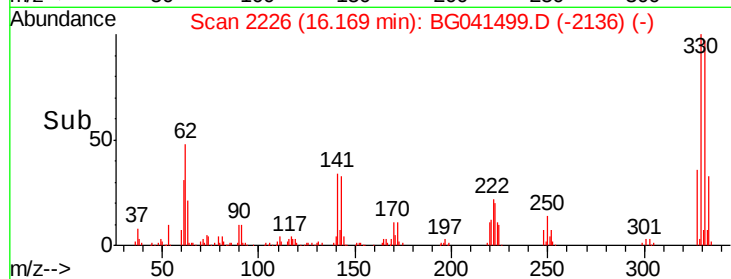
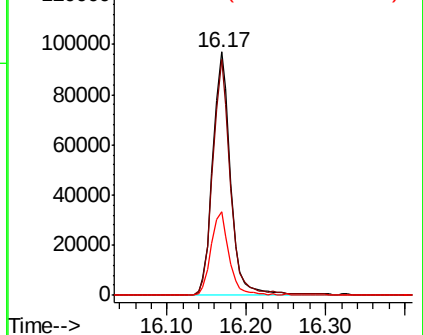



#45
 2-Fluorobiphenyl
 Concen: 76.090 ng
 RT: 13.30 min Scan# 1737
 Delta R.T. -0.00 min
 Lab File: BG041499.D
 Acq: 27 Jun 2019 22:07

Tgt Ion:172 Resp: 423598
 Ion Ratio Lower Upper
 172 100
 171 37.7 29.6 44.4
 170 25.1 20.0 30.0

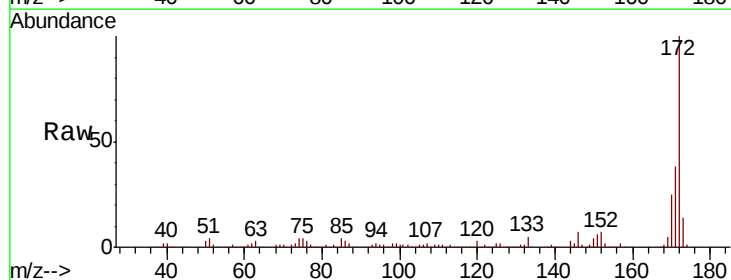

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

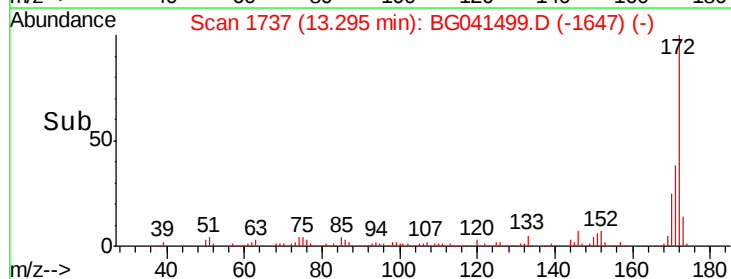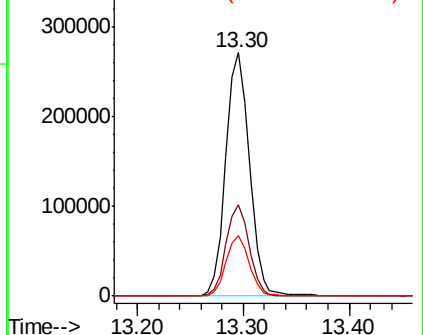

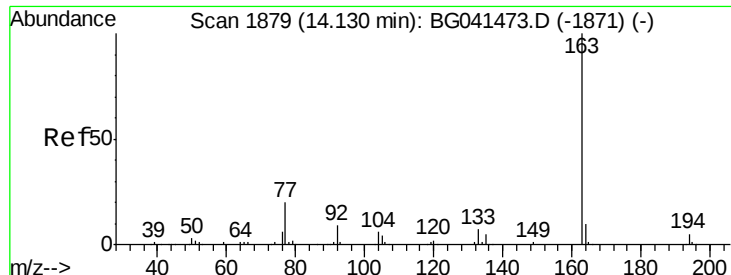

#50

Dimethylphthalate

Concen: 10.005 ng

RT: 14.12 min Scan# 1878

Delta R.T. -0.01 min

Lab File: BG041499.D

Acq: 27 Jun 2019 22:07

Instrument :

BNA_G

ClientSampleId :

M-6


Tgt Ion:163 Resp: 65043

Ion Ratio Lower Upper

163 100

194 4.9 3.7 5.5




164 9.6 7.8 11.6

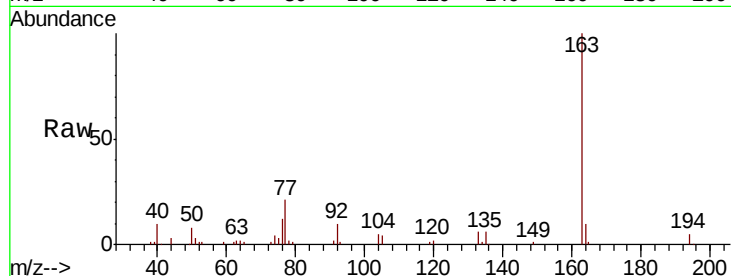

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

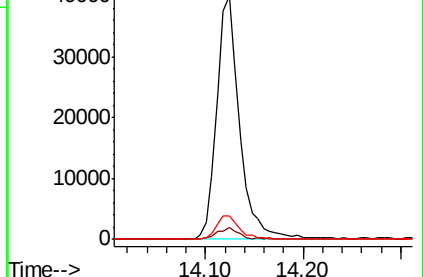

#57

2,4-Dinitrotoluene

Concen: 4.846 ng

RT: 14.68 min Scan# 1972

Delta R.T. -0.38 min

Lab File: BG041499.D

Acq: 27 Jun 2019 22:07

Tgt Ion:165 Resp: 9699


Ion Ratio Lower Upper

165 100

63 3.0 38.8 58.2#

89 0.0 60.1 90.1#

182 0.0 2.2 3.2#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

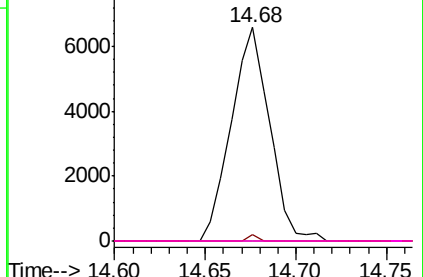

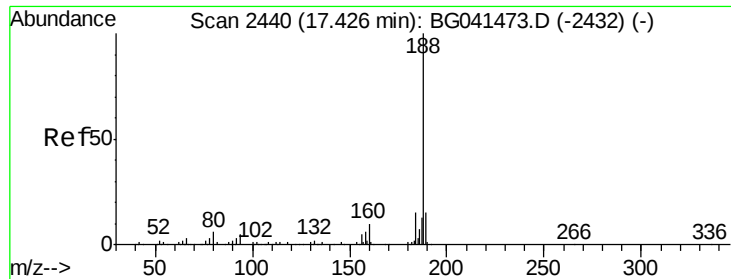

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.43 min Scan# 2440

Delta R.T. -0.00 min

Lab File: BG041499.D

Acq: 27 Jun 2019 22:07

Instrument :

BNA_G

ClientSampleId :

M-6


Tgt Ion:188 Resp: 191229

Ion Ratio Lower Upper

188 100

94 4.6 3.8 5.8

80 5.7 4.8 7.2

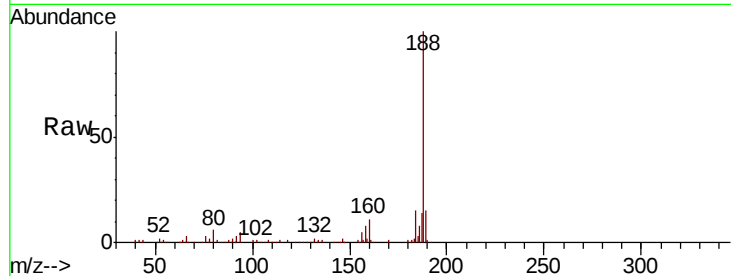

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

150000

100000

50000



0

17.43

17.40

17.50

Time-->



#67

4-Bromophenyl-phenylether

Concen: 4.112 ng

RT: 16.17 min Scan# 2226

Delta R.T. -0.44 min

Lab File: BG041499.D

Acq: 27 Jun 2019 22:07


Tgt Ion:248 Resp: 10745

Ion Ratio Lower Upper

248 100

250 193.2 78.1 117.1#

141 477.3 54.1 81.1#



Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

40000

30000

20000

10000

0


16.17


16.10

16.20

16.25

Time-->







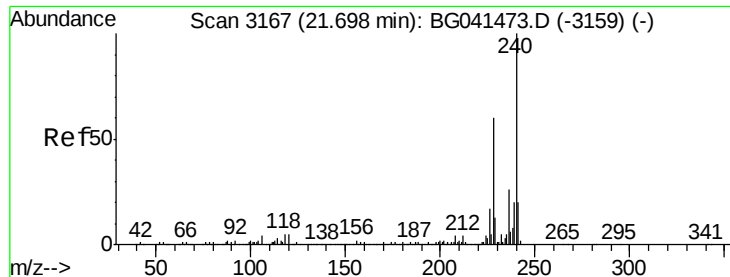

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.70 min Scan# 3167
Delta R.T. -0.00 min
Lab File: BG041499.D
Acq: 27 Jun 2019 22:07




Instrument :
BNA_G
ClientSampleId :
M-6


Tgt Ion:240 Resp: 205965
Ion Ratio Lower Upper
240 100
120 3.7 3.7 5.5#
236 25.0 20.8 31.2

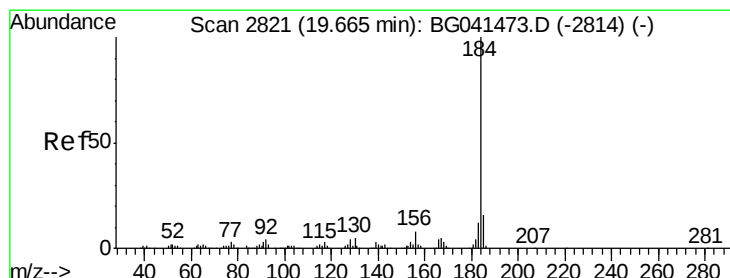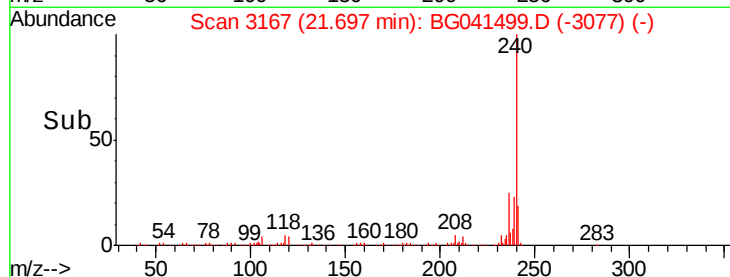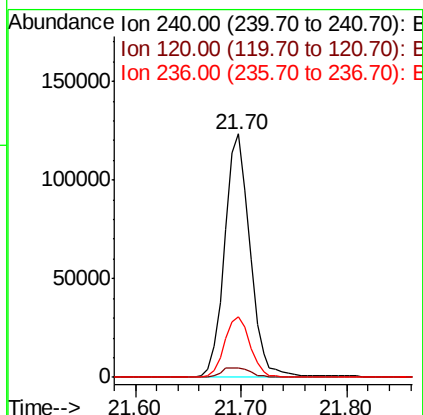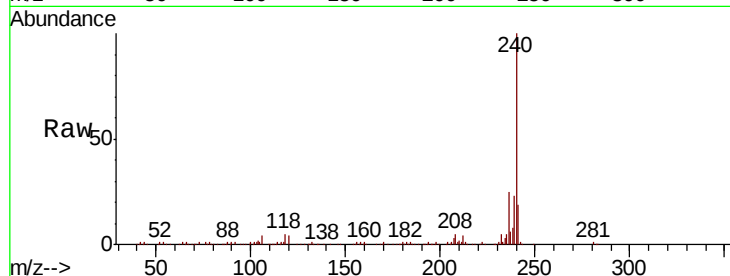

#77
Benzidine
Concen: 2.992 ng
RT: 20.02 min Scan# 2882
Delta R.T. 0.36 min
Lab File: BG041499.D
Acq: 27 Jun 2019 22:07

Tgt Ion:184 Resp: 13673
Ion Ratio Lower Upper
184 100
185 15.6 12.7 19.1
183 9.4 9.4 14.2#

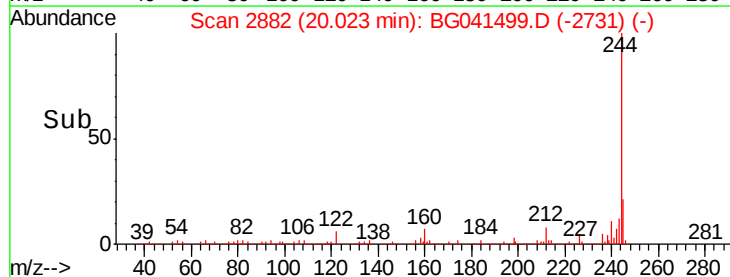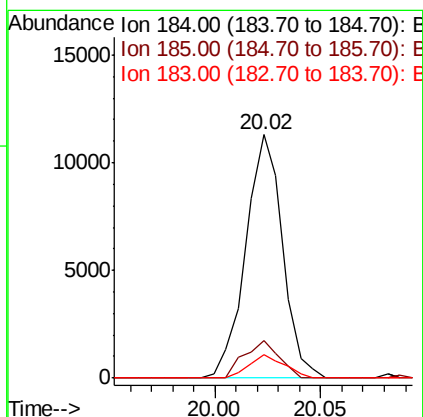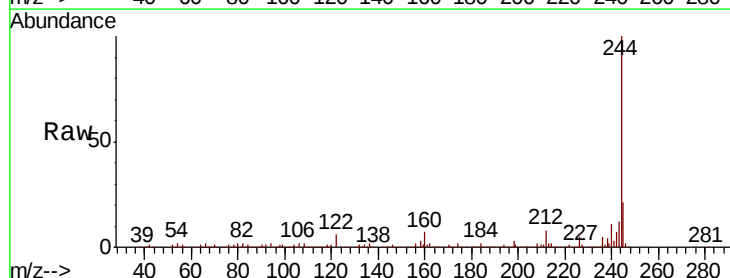

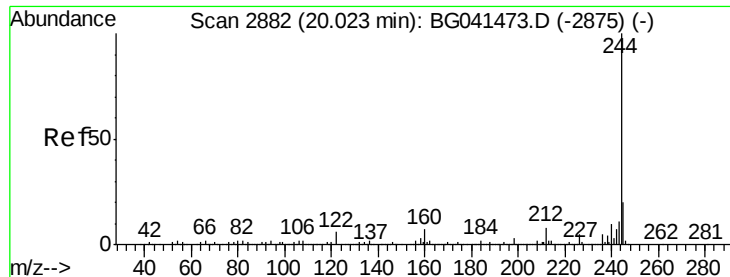

#79

Terphenyl-d14

Concen: 85.623 ng

RT: 20.02 min Scan# 2882

Delta R.T. -0.00 min

Lab File: BG041499.D

Acq: 27 Jun 2019 22:07

Instrument :

BNA_G

ClientSampled :

M-6


Tgt Ion:244 Resp: 829871

Ion Ratio Lower Upper

244 100

212 8.0 6.2 9.4




122 6.2 4.8 7.2

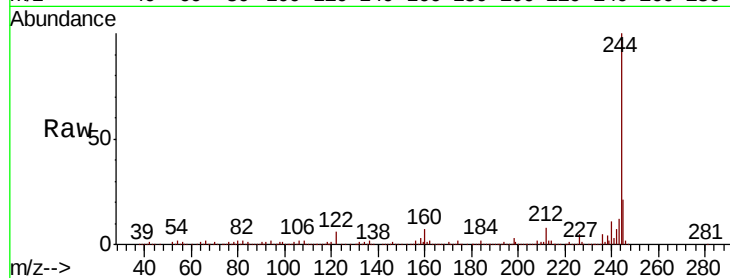

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

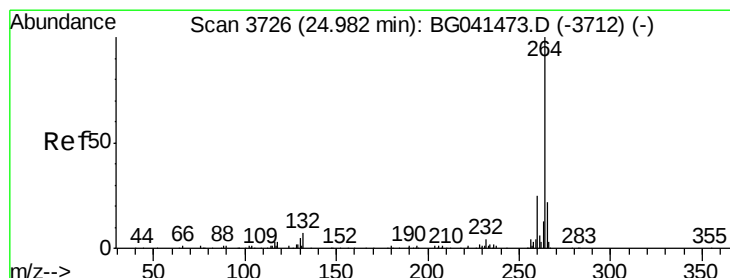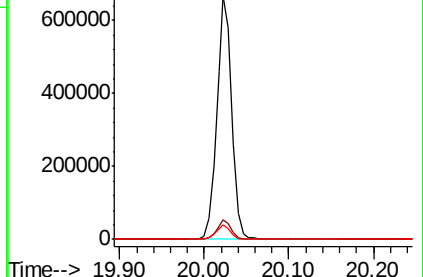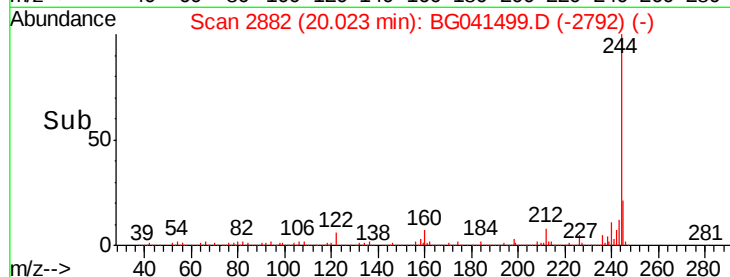

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.98 min Scan# 3726

Delta R.T. -0.00 min

Lab File: BG041499.D

Acq: 27 Jun 2019 22:07


Tgt Ion:264 Resp: 221361

Ion Ratio Lower Upper

264 100

260 22.4 19.7 29.5

265 22.2 17.4 26.2

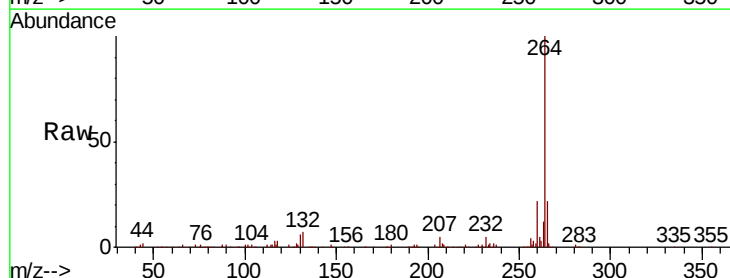

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

