
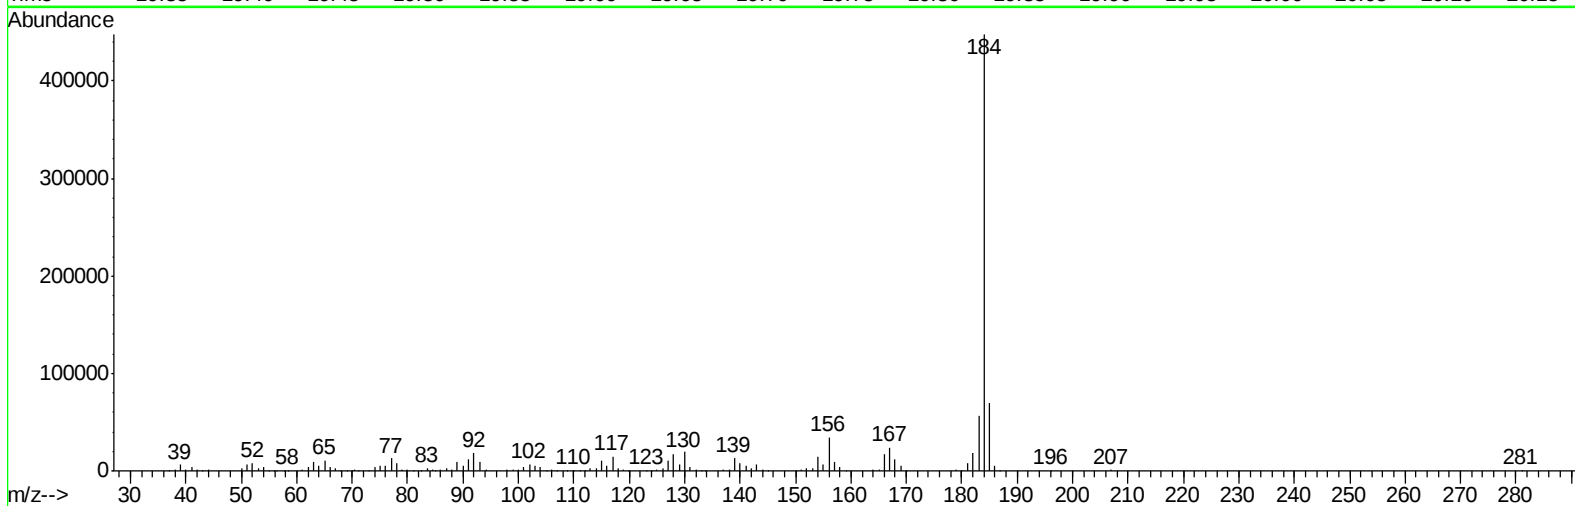


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062719\
Data File : BG041479.D
Acq On : 27 Jun 2019 7:24
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 08:11:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

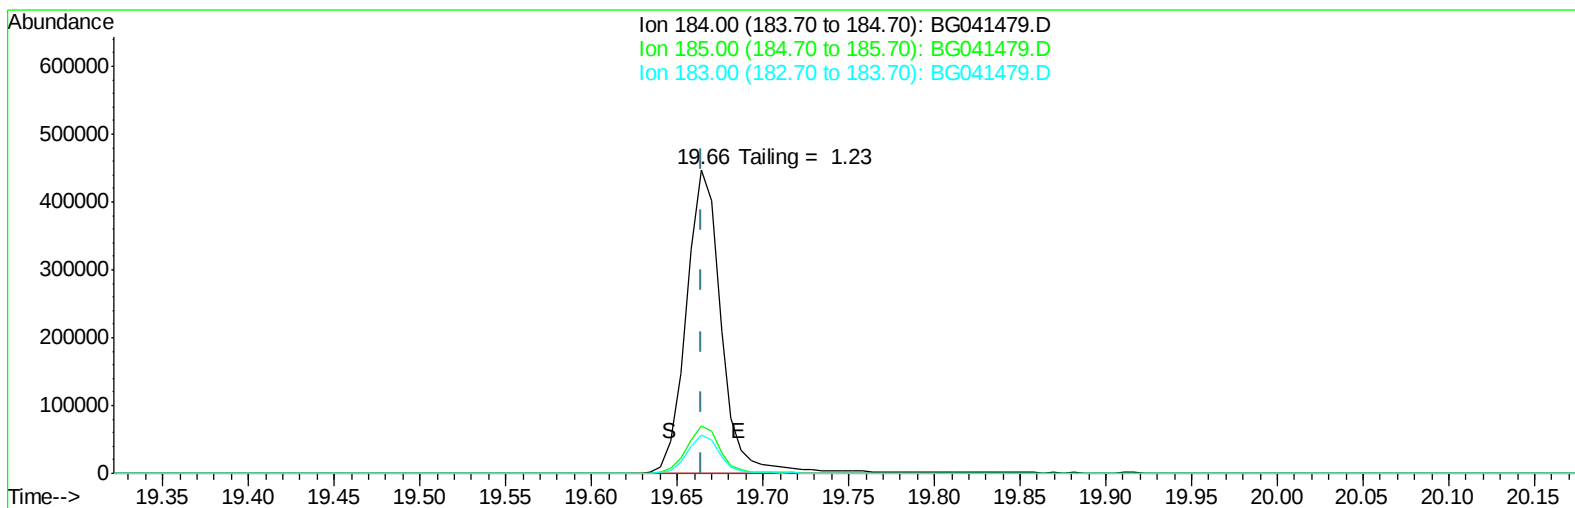

TIC: BG041479.D

(77) Benzidine



19.664min (-0.001) 9262.27ng

response 640987

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	15.50
183.00	11.80	12.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062719\
Data File : BG041479.D
Acq On : 27 Jun 2019 7:24
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 08:11:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG062619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 27 13:25:55 2019
Response via : Initial Calibration

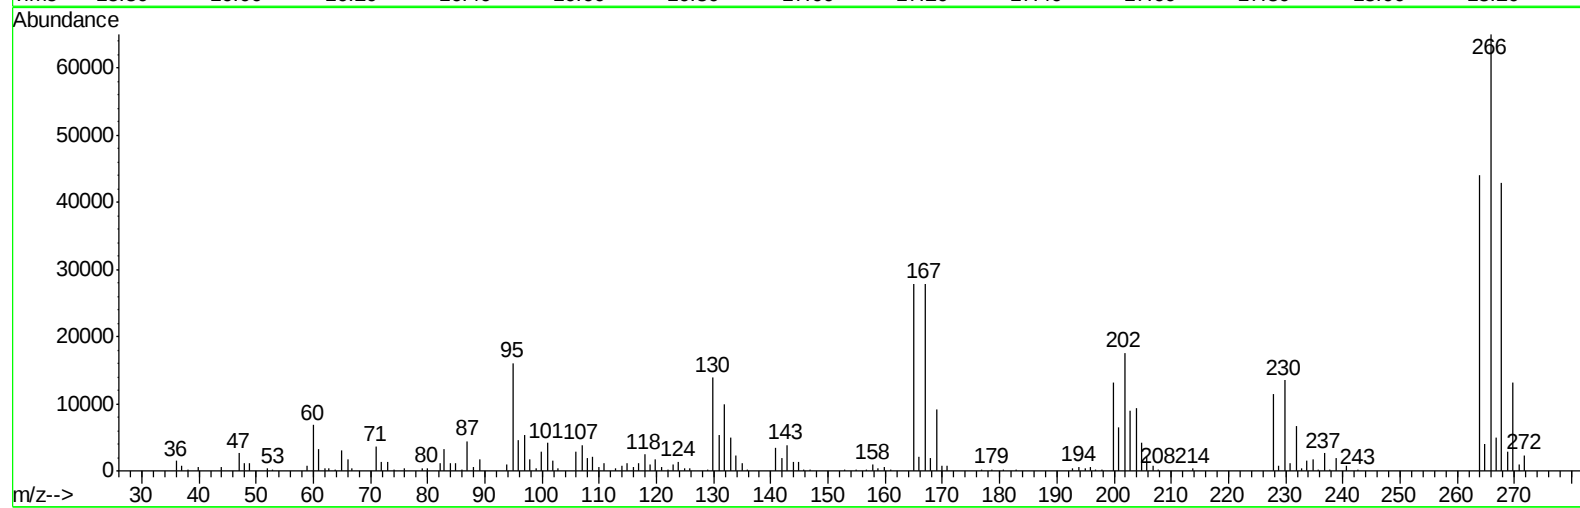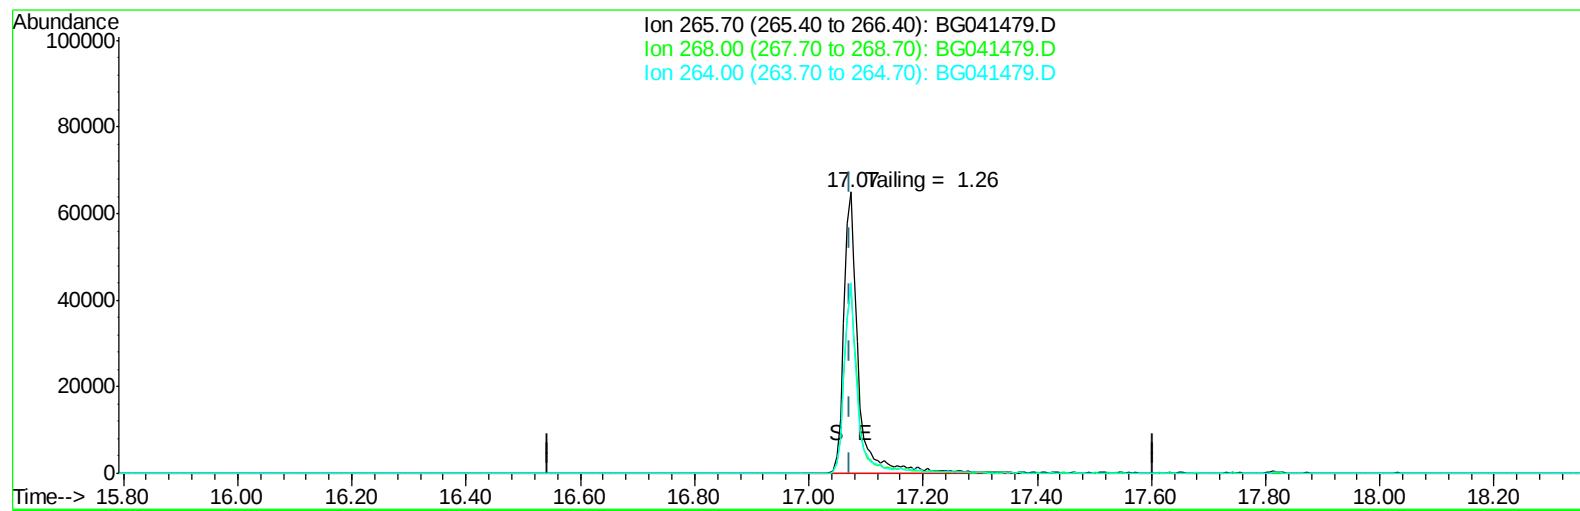

TIC: BG041479.D

(70) Pentachlorophenol (C)

17.073min (-0.001) 316063.30ng

response 111756

Ion	Exp%	Act%
265.70	100	100
268.00	58.70	66.08
264.00	59.20	67.79
0.00	0.00	0.00