

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
 Data File : BG061739.D
 Acq On : 27 Jun 2024 14:57
 Operator : MA/JU
 Sample : P2934-21
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4B57

Quant Time: Jun 27 15:34:17 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 12:23:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.054	152	58544	20.000	ng/u1	0.00
20) Naphthalene-d8	10.869	136	289067	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.688	164	191613	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.431	188	454167	20.000	ng/u1	0.00
79) Chrysene-d12	21.691	240	368374	20.000	ng/u1	0.00
88) Perylene-d12	24.911	264	408685	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.454	96	7303	4.506	ng/uL	0.00
4) Pyridine-d5	3.871	84	107572	21.954	ng/u1	0.00
7) Phenol-d5	7.196	99	136526	21.481	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.379	67	87974	22.205	ng/u1	0.00
11) 2-Chlorophenol-d4	7.578	132	96216	22.061	ng/u1	0.00
15) 4-Methylphenol-d8	8.748	113	107020	21.782	ng/u1	0.00
21) Nitrobenzene-d5	9.223	128	44416	22.629	ng/u1	0.00
24) 2-Nitrophenol-d4	9.940	143	47550	23.920	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.475	165	104209	22.139	ng/u1	0.00
31) 4-Chloroaniline-d4	10.998	131	148050	20.775	ng/u1	0.00
46) Dimethylphthalate-d6	14.088	166	368965	25.022	ng/u1	0.00
49) Acenaphthylene-d8	14.382	160	411203	25.446	ng/u1	0.00
54) 4-Nitrophenol-d4	14.864	143	51719	20.423	ng/u1	0.00
60) Fluorene-d10	15.675	176	334845	25.939	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.780	200	36835	18.967	ng/u1	0.00
73) Anthracene-d10	17.525	188	536988	25.903	ng/u1	0.00
81) Pyrene-d10	19.811	212	609367	29.615	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.688	264	540740	27.703	ng/u1	0.00
Target Compounds						
80) Fluoranthene	19.476	202	26025	1.090	ng/u1#	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061739.D
Acq On : 27 Jun 2024 14:57
Operator : MA/JU
Sample : P2934-21
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4B57

Quant Time: Jun 27 15:34:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 12:23:53 2024
Response via : Initial Calibration

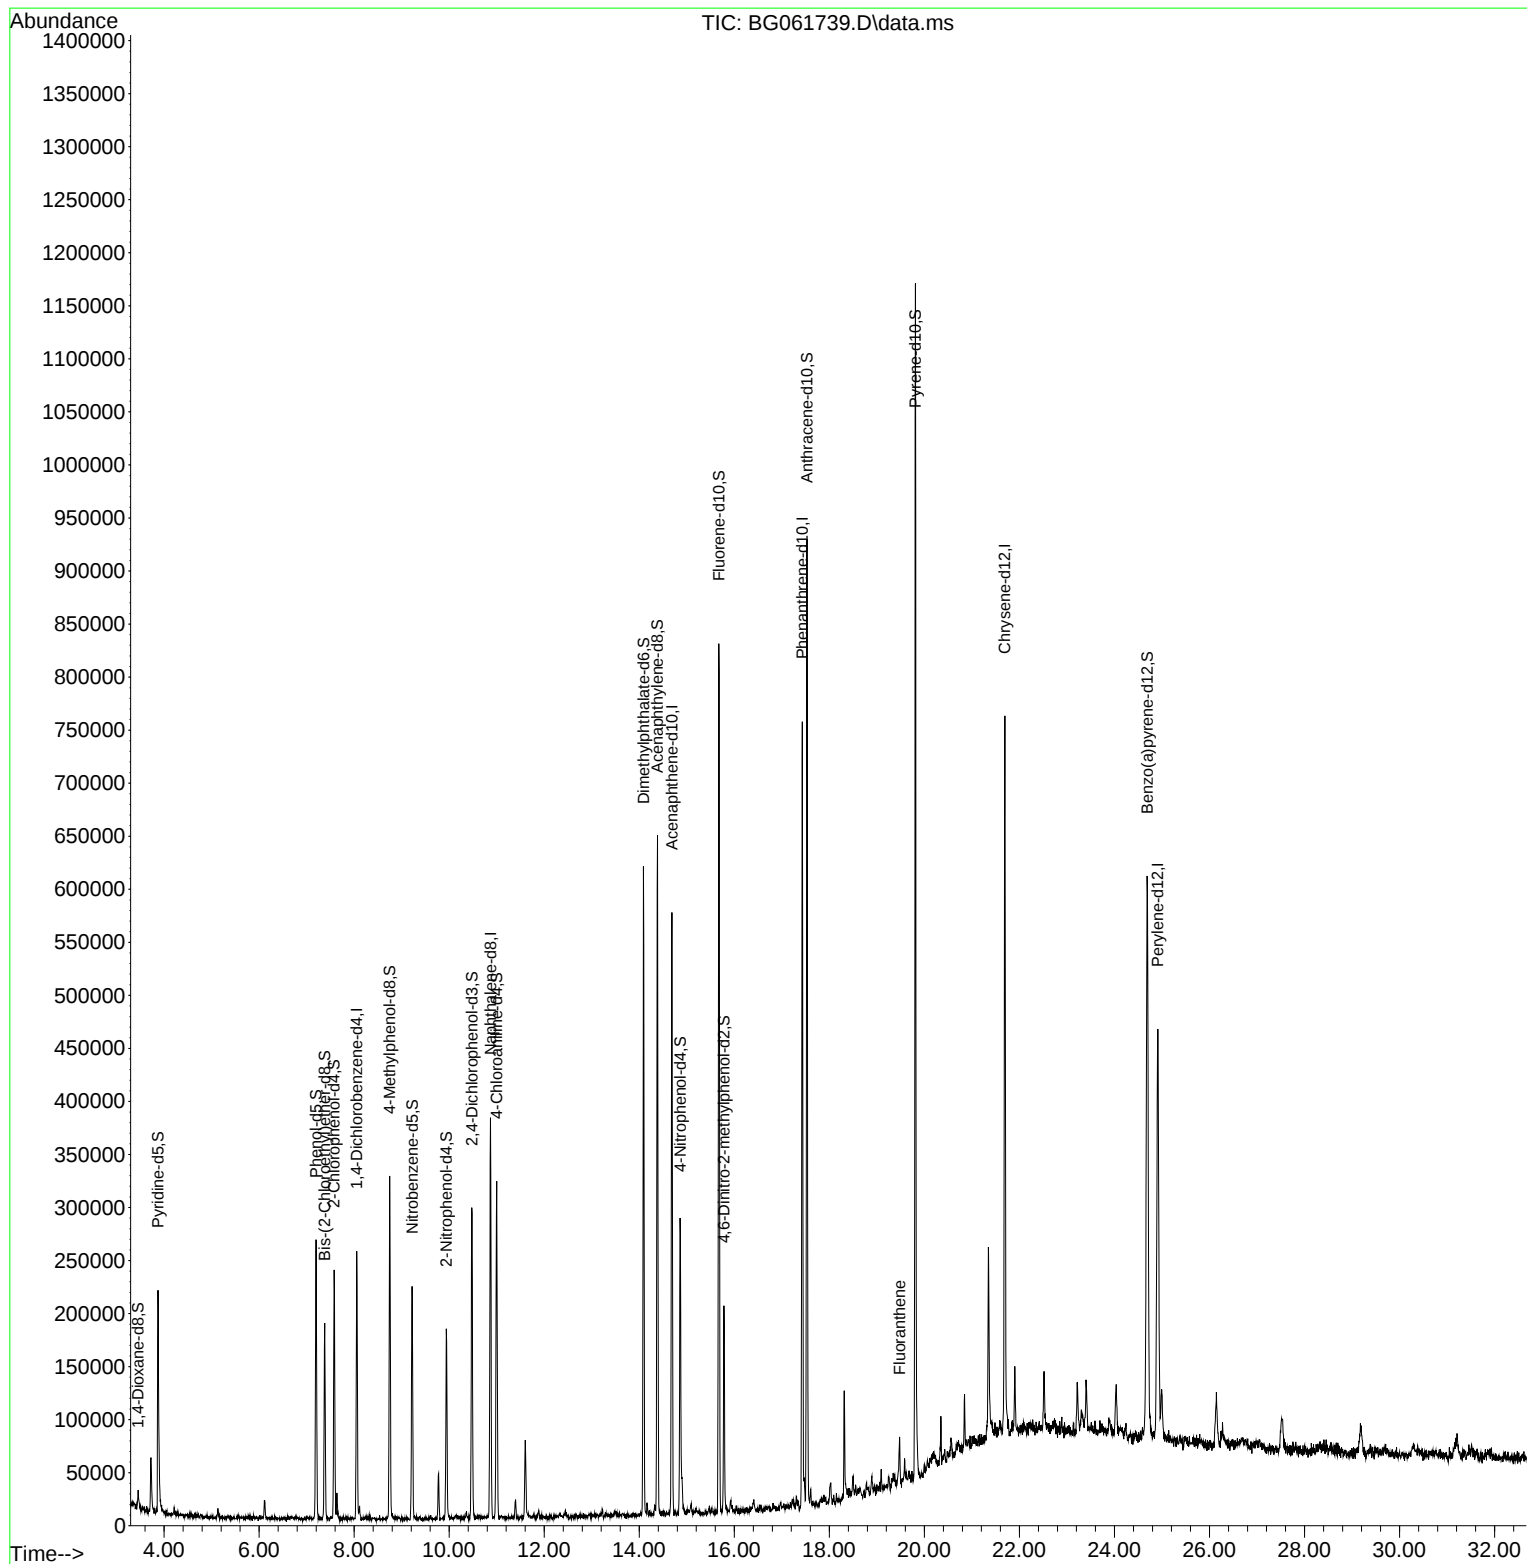

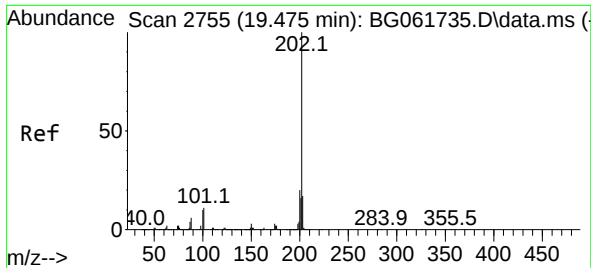

#80
 Fluoranthene
 Concen: 1.090 ng/ul
 RT: 19.476 min Scan# 21
 Delta R.T. 0.001 min
 Lab File: BG061739.D
 Acq: 27 Jun 2024 14:57

Instrument :
 BNA_G
 ClientSampleId :
 A4B57

Tgt Ion	Ratio	Lower	Upper
202	100		
101	15.2	7.8	11.6#
100	7.0	7.7	11.5#

