

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
 Data File : BG061736.D
 Acq On : 27 Jun 2024 11:39
 Operator : MA/JU
 Sample : PB161760BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK760

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.453	25	28	36	rVB	27544	40534	1.76%	0.173%
2	3.694	66	69	71	rBV3	4500	3843	0.17%	0.016%
3	3.870	95	99	113	rBV	320789	552753	24.05%	2.355%
4	4.211	153	157	159	rBV4	5466	7224	0.31%	0.031%
5	4.434	192	195	198	rBV3	2992	3287	0.14%	0.014%
6	5.104	306	309	311	rVB3	3256	3401	0.15%	0.014%
7	5.809	427	429	431	rBV3	3588	3560	0.15%	0.015%
8	5.933	447	450	452	rBV3	3331	3099	0.13%	0.013%
9	6.567	553	558	562	rBV5	3453	6503	0.28%	0.028%
10	6.773	588	593	595	rBV2	3610	4849	0.21%	0.021%
11	7.025	634	636	641	rVB2	2978	4124	0.18%	0.018%
12	7.202	655	666	674	rBV	385584	664354	28.91%	2.831%
13	7.384	690	697	706	rVB	275032	462267	20.11%	1.970%
14	7.501	716	717	720	rVB3	4743	3238	0.14%	0.014%
15	7.584	723	731	739	rVV	336495	574307	24.99%	2.447%
16	7.672	743	746	747	rBV3	3185	3085	0.13%	0.013%
17	7.901	781	785	788	rBV4	2360	3614	0.16%	0.015%
18	8.060	804	812	818	rVB	272302	461964	20.10%	1.968%
19	8.130	821	824	827	rVV3	3901	3934	0.17%	0.017%
20	8.171	827	831	832	rVV3	4112	3876	0.17%	0.017%
21	8.189	832	834	838	rVB3	2848	3398	0.15%	0.014%
22	8.465	877	881	883	rBV3	2723	3609	0.16%	0.015%
23	8.500	886	887	891	rVV3	3835	3554	0.15%	0.015%
24	8.553	891	896	897	rVV5	2845	3389	0.15%	0.014%
25	8.606	902	905	907	rBV3	2794	3607	0.16%	0.015%
26	8.747	923	929	939	rBV	439929	760256	33.08%	3.239%
27	9.223	1003	1010	1018	rBV	329371	576004	25.06%	2.454%
28	9.364	1031	1034	1037	rVB4	2988	3983	0.17%	0.017%
29	9.393	1037	1039	1041	rBV3	3703	3163	0.14%	0.013%
30	9.646	1080	1082	1086	rBV4	1955	3151	0.14%	0.013%
31	9.946	1124	1133	1140	rBV	238163	427156	18.59%	1.820%
32	10.198	1174	1176	1181	rVB3	2247	3122	0.14%	0.013%
33	10.263	1186	1187	1190	rBV3	3948	3990	0.17%	0.017%
34	10.480	1214	1224	1232	rBV	439765	783648	34.10%	3.339%
35	10.533	1232	1233	1237	rVB3	3237	3911	0.17%	0.017%
36	10.733	1265	1267	1272	rVB2	3237	4399	0.19%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
 Data File : BG061736.D
 Acq On : 27 Jun 2024 11:39
 Operator : MA/JU
 Sample : PB161760BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK760

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	10.803	1276	1279	1282	rVB4	3464	4593	0.20%	0.020%
38	10.868	1282	1290	1298	rBV	408030	724749	31.53%	3.088%
39	10.997	1305	1312	1320	rBV	386377	690046	30.02%	2.940%
40	11.279	1357	1360	1363	rBV4	3762	4104	0.18%	0.017%
41	11.467	1390	1392	1395	rBV2	3863	3628	0.16%	0.015%
42	11.814	1448	1451	1452	rBV2	4201	3180	0.14%	0.014%
43	12.037	1485	1489	1492	rBV5	4527	5586	0.24%	0.024%
44	12.061	1492	1493	1497	rVB2	3538	4125	0.18%	0.018%
45	12.172	1508	1512	1513	rBV3	2542	3641	0.16%	0.016%
46	12.449	1555	1559	1563	rVB3	11917	17012	0.74%	0.072%
47	12.496	1565	1567	1571	rVB2	4542	4676	0.20%	0.020%
48	12.901	1634	1636	1640	rVB3	3448	3994	0.17%	0.017%
49	13.060	1661	1663	1665	rBV3	4089	4499	0.20%	0.019%
50	13.154	1678	1679	1682	rBV3	2898	3432	0.15%	0.015%
51	13.265	1695	1698	1699	rBV2	3483	3300	0.14%	0.014%
52	13.653	1762	1764	1766	rBV3	5408	5044	0.22%	0.021%
53	14.094	1831	1839	1846	rBV	793630	1170853	50.94%	4.989%
54	14.382	1882	1888	1895	rBV	888643	1378690	59.99%	5.874%
55	14.575	1919	1921	1924	rVB3	4365	3437	0.15%	0.015%
56	14.687	1934	1940	1947	rVB	653833	979392	42.61%	4.173%
57	14.863	1962	1970	1981	rBV	424238	676247	29.42%	2.881%
58	15.222	2028	2031	2032	rBV2	3989	3533	0.15%	0.015%
59	15.269	2035	2039	2040	rBV3	2586	3176	0.14%	0.014%
60	15.357	2052	2054	2056	rVB2	3616	3201	0.14%	0.014%
61	15.680	2101	2109	2116	rBV	1127009	1714949	74.62%	7.307%
62	15.786	2121	2127	2132	rBV	276697	407415	17.73%	1.736%
63	15.833	2134	2135	2137	rVB	6862	3099	0.13%	0.013%
64	15.880	2140	2143	2146	rVB3	3296	4400	0.19%	0.019%
65	15.915	2146	2149	2151	rBV4	6180	7925	0.34%	0.034%
66	16.091	2177	2179	2182	rBV	4049	4367	0.19%	0.019%
67	16.179	2190	2194	2197	rVB4	4461	5982	0.26%	0.025%
68	16.838	2303	2306	2309	rBV3	2867	4013	0.17%	0.017%
69	17.108	2350	2352	2355	rBV4	5292	5215	0.23%	0.022%
70	17.131	2355	2356	2360	rVV2	4628	4029	0.18%	0.017%
71	17.190	2362	2366	2367	rVB4	4572	4896	0.21%	0.021%
72	17.249	2374	2376	2380	rVB5	3747	4079	0.18%	0.017%
73	17.431	2401	2407	2415	rVB	855168	1262469	54.93%	5.379%
74	17.531	2417	2424	2431	rBV	1328478	1957979	85.19%	8.343%
75	17.613	2436	2438	2440	rBV2	4509	4201	0.18%	0.018%
76	17.877	2480	2483	2484	rBV3	3524	3087	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
 Data File : BG061736.D
 Acq On : 27 Jun 2024 11:39
 Operator : MA/JU
 Sample : PB161760BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK760

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

77	18.101	2516	2521	2523	rVB5	6376	10081	0.44%	0.043%
78	18.236	2542	2544	2546	rVB2	5013	3170	0.14%	0.014%
79	18.389	2569	2570	2572	rBV2	5082	4083	0.18%	0.017%
80	18.970	2667	2669	2671	rVB3	5202	3138	0.14%	0.013%
81	19.305	2725	2726	2730	rBV4	6032	7609	0.33%	0.032%
82	19.376	2735	2738	2743	rVV4	21578	37747	1.64%	0.161%
83	19.446	2747	2750	2755	rVB3	19538	29680	1.29%	0.126%
84	19.811	2806	2812	2822	rVB	1588939	2298355	100.00%	9.793%
85	21.697	3126	3133	3141	rBV	744118	1271606	55.33%	5.418%
86	24.693	3633	3643	3653	rBV	777219	2089356	90.91%	8.903%
87	24.916	3672	3681	3690	rVB	445470	1207928	52.56%	5.147%




Sum of corrected areas: 23469152

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061736.D
Acq On : 27 Jun 2024 11:39
Operator : MA/JU
Sample : PB161760BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK760

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

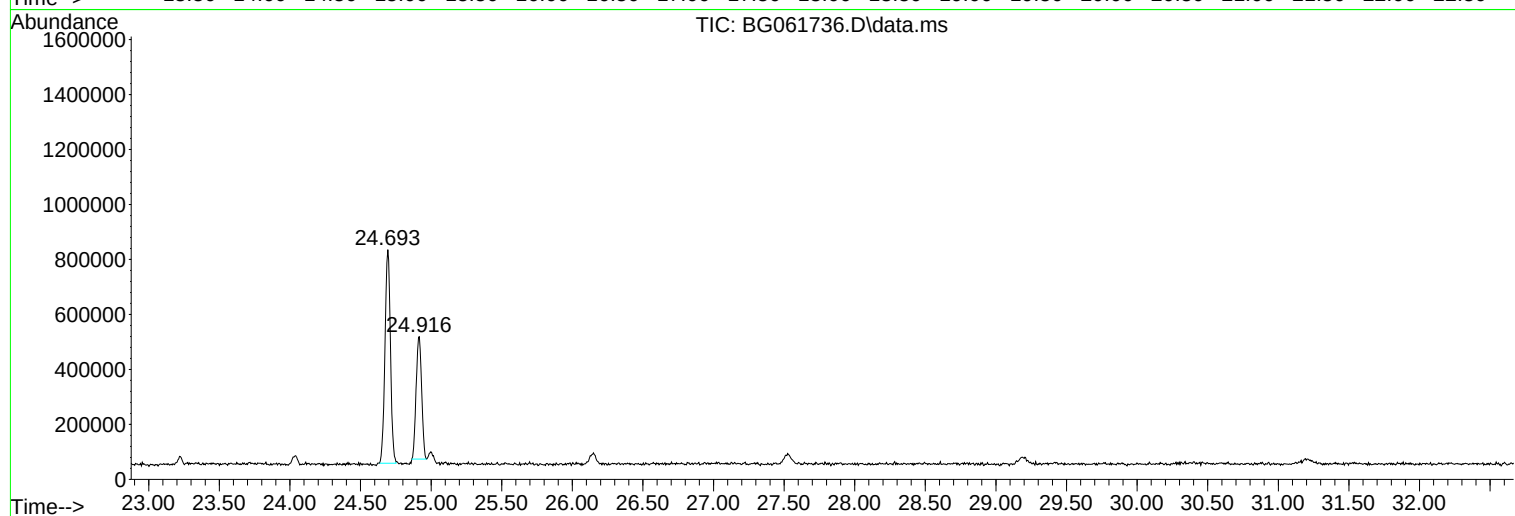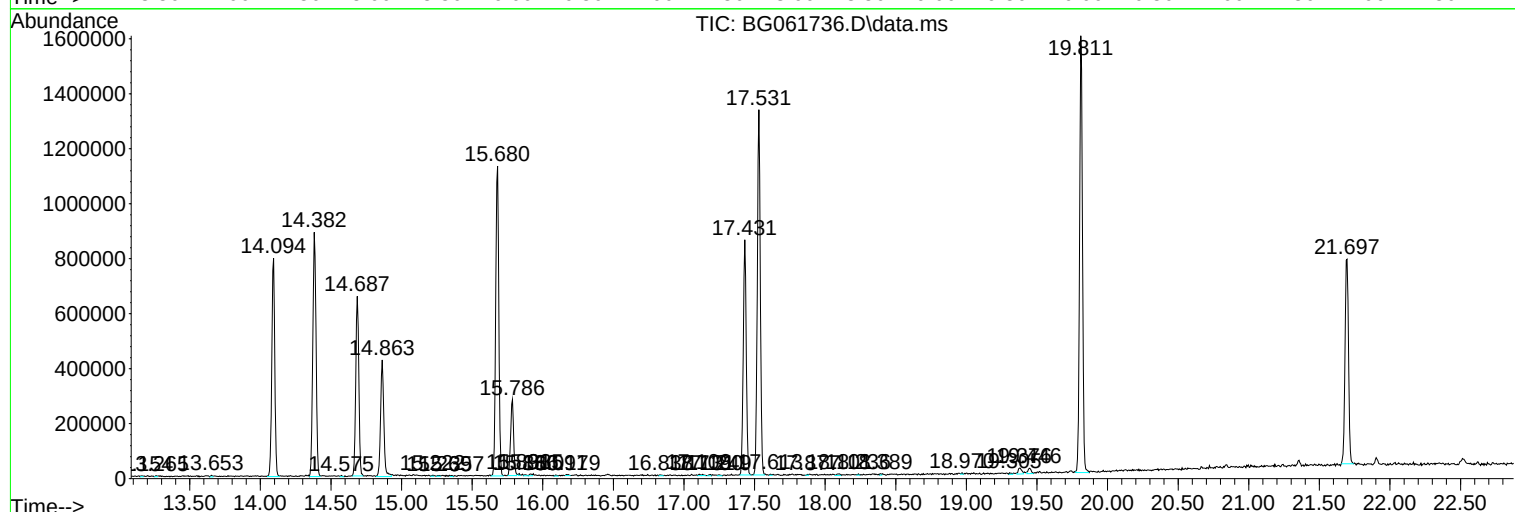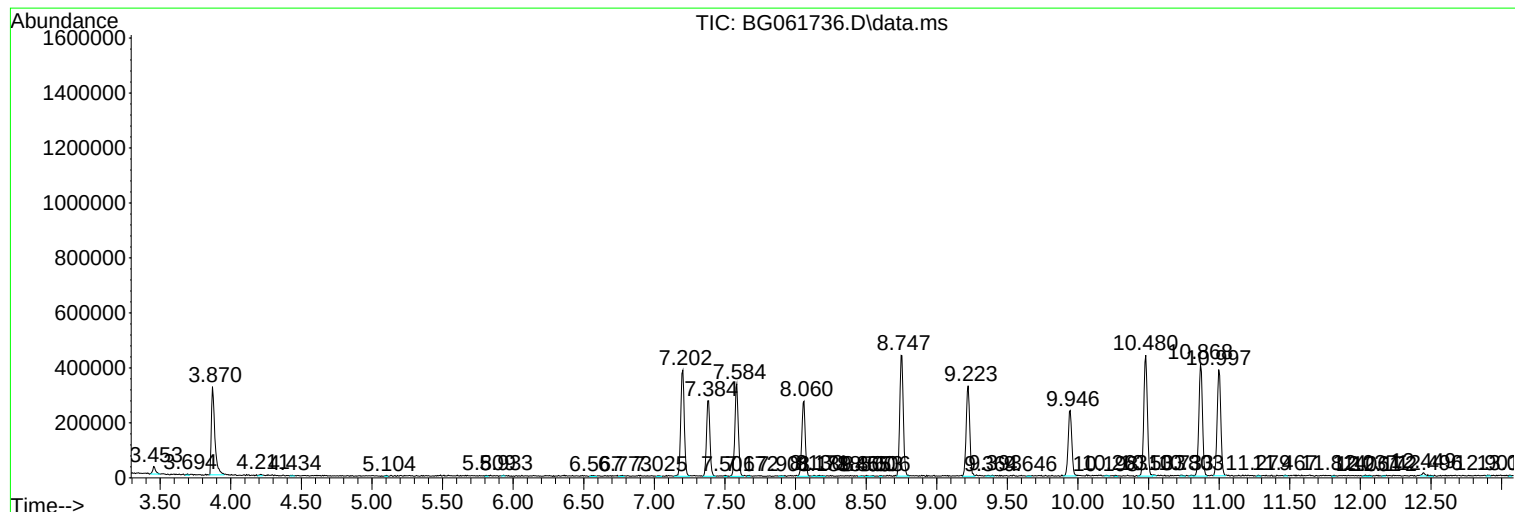

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061736.D
Acq On : 27 Jun 2024 11:39
Operator : MA/JU
Sample : PB161760BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK760

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061736.D
Acq On : 27 Jun 2024 11:39
Operator : MA/JU
Sample : PB161760BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK760

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc