

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
 Data File : BG061742.D
 Acq On : 27 Jun 2024 17:00
 Operator : MA/JU
 Sample : PB161760BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK760

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.459	25	29	34	rVB	29065	42583	1.72%	0.163%
2	3.870	95	99	118	rBV	327809	596784	24.06%	2.280%
3	4.216	154	158	165	rVB5	7531	13368	0.54%	0.051%
4	4.557	214	216	220	rBV3	4180	4011	0.16%	0.015%
5	5.157	314	318	319	rVB3	3758	3620	0.15%	0.014%
6	5.227	328	330	335	rVB2	2963	3641	0.15%	0.014%
7	5.333	346	348	352	rVB	3760	3760	0.15%	0.014%
8	5.638	397	400	402	rBV3	3764	3803	0.15%	0.015%
9	6.079	474	475	479	rVB3	5460	3927	0.16%	0.015%
10	7.201	658	666	673	rBV	444580	750247	30.25%	2.866%
11	7.383	689	697	703	rBV	314697	515085	20.77%	1.968%
12	7.583	722	731	739	rVB	389029	666592	26.87%	2.547%
13	8.059	805	812	818	rVB	307423	521699	21.03%	1.993%
14	8.511	887	889	892	rBV2	2820	3802	0.15%	0.015%
15	8.699	918	921	923	rBV3	2687	3722	0.15%	0.014%
16	8.752	923	930	938	rVB	509394	864383	34.85%	3.302%
17	9.222	1002	1010	1017	rBV	393591	694915	28.02%	2.655%
18	9.734	1095	1097	1102	rBV3	3502	5548	0.22%	0.021%
19	9.822	1110	1112	1116	rVB2	3195	3696	0.15%	0.014%
20	9.945	1124	1133	1141	rBV	311668	567996	22.90%	2.170%
21	10.480	1215	1224	1232	rBV	486284	881444	35.54%	3.367%
22	10.867	1283	1290	1299	rVB	447721	809628	32.64%	3.093%
23	10.997	1303	1312	1320	rBV	444151	778896	31.40%	2.976%
24	11.931	1468	1471	1473	rVB3	4005	4094	0.17%	0.016%
25	12.195	1511	1516	1518	rBV3	3474	4607	0.19%	0.018%
26	12.278	1527	1530	1533	rVB3	3249	4144	0.17%	0.016%
27	12.448	1554	1559	1565	rBV3	9252	15203	0.61%	0.058%
28	13.647	1760	1763	1765	rBV4	4678	5186	0.21%	0.020%
29	13.799	1786	1789	1791	rVB3	3872	4431	0.18%	0.017%
30	14.087	1832	1838	1844	rBV	877299	1277496	51.50%	4.880%
31	14.381	1879	1888	1896	rVB2	1000899	1545065	62.29%	5.903%
32	14.457	1898	1901	1904	rVV4	5373	7445	0.30%	0.028%
33	14.487	1904	1906	1910	rVB4	3561	5237	0.21%	0.020%
34	14.640	1929	1932	1933	rBV2	4347	3851	0.16%	0.015%
35	14.687	1933	1940	1947	rVB	700755	1092268	44.04%	4.173%
36	14.863	1963	1970	1977	rBV	499452	784207	31.62%	2.996%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
 Data File : BG061742.D
 Acq On : 27 Jun 2024 17:00
 Operator : MA/JU
 Sample : PB161760BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK760

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	15.298	2042	2044	2048	rBV2	5250	6101	0.25%	0.023%
38	15.415	2061	2064	2066	rBV2	3025	4473	0.18%	0.017%
39	15.533	2080	2084	2086	rVB3	2657	3579	0.14%	0.014%
40	15.674	2102	2108	2117	rVB	1211146	1865581	75.21%	7.127%
41	15.779	2120	2126	2134	rBV	364289	569264	22.95%	2.175%
42	15.920	2145	2150	2151	rBV4	6026	7018	0.28%	0.027%
43	15.938	2151	2153	2156	rVB3	4215	3997	0.16%	0.015%
44	16.161	2190	2191	2193	rBV2	4301	4334	0.17%	0.017%
45	16.332	2217	2220	2223	rBV2	4248	5910	0.24%	0.023%
46	16.455	2239	2241	2245	rVB3	5211	5271	0.21%	0.020%
47	16.620	2264	2269	2271	rBV3	2804	5344	0.22%	0.020%
48	16.719	2284	2286	2288	rBV	5739	5238	0.21%	0.020%
49	16.825	2301	2304	2305	rBV2	4060	4305	0.17%	0.016%
50	16.919	2319	2320	2323	rBV	3610	4539	0.18%	0.017%
51	17.001	2332	2334	2336	rBV3	3162	3996	0.16%	0.015%
52	17.090	2346	2349	2352	rBV2	5212	7100	0.29%	0.027%
53	17.301	2384	2385	2388	rVB3	4633	3789	0.15%	0.014%
54	17.430	2400	2407	2413	rBV	937275	1384479	55.82%	5.289%
55	17.530	2415	2424	2432	rBV2	1415987	2166373	87.34%	8.276%
56	17.648	2443	2444	2448	rBV3	5078	4553	0.18%	0.017%
57	17.777	2465	2466	2470	rBV3	5917	8251	0.33%	0.032%
58	18.394	2569	2571	2574	rBV3	4961	4829	0.19%	0.018%
59	18.582	2601	2603	2605	rBV3	4565	4594	0.19%	0.018%
60	18.705	2622	2624	2628	rBV4	5637	7490	0.30%	0.029%
61	19.070	2685	2686	2691	rBV4	5715	6211	0.25%	0.024%
62	19.375	2735	2738	2744	rVB7	23705	35524	1.43%	0.136%
63	19.446	2747	2750	2754	rVB3	17712	23500	0.95%	0.090%
64	19.634	2780	2782	2785	rVB4	5818	5191	0.21%	0.020%
65	19.810	2806	2812	2819	rBV	1805553	2480371	100.00%	9.476%
66	20.010	2844	2846	2847	rBV2	7847	4028	0.16%	0.015%
67	21.690	3126	3132	3140	rVB2	838743	1371006	55.27%	5.238%
68	24.029	3525	3530	3538	rVB4	58106	125926	5.08%	0.481%
69	24.692	3633	3643	3655	rVB2	830871	2231472	89.97%	8.525%
70	24.904	3671	3679	3688	rBV2	485439	1306259	52.66%	4.990%




Sum of corrected areas: 26176280

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061742.D
Acq On : 27 Jun 2024 17:00
Operator : MA/JU
Sample : PB161760BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK760

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

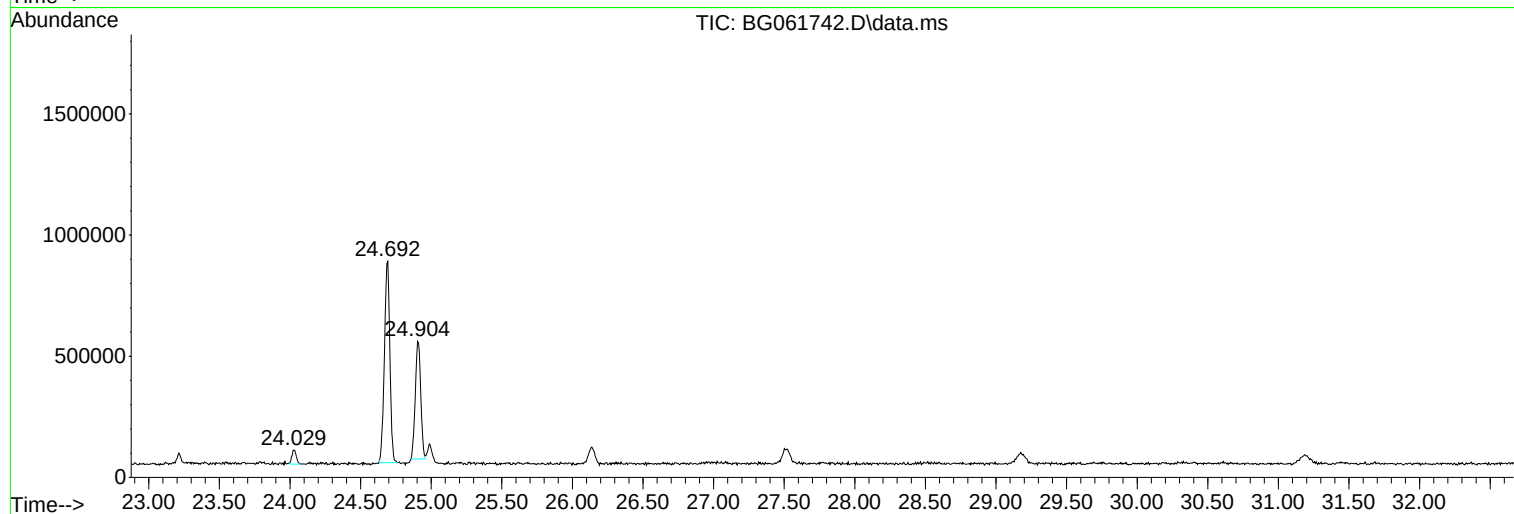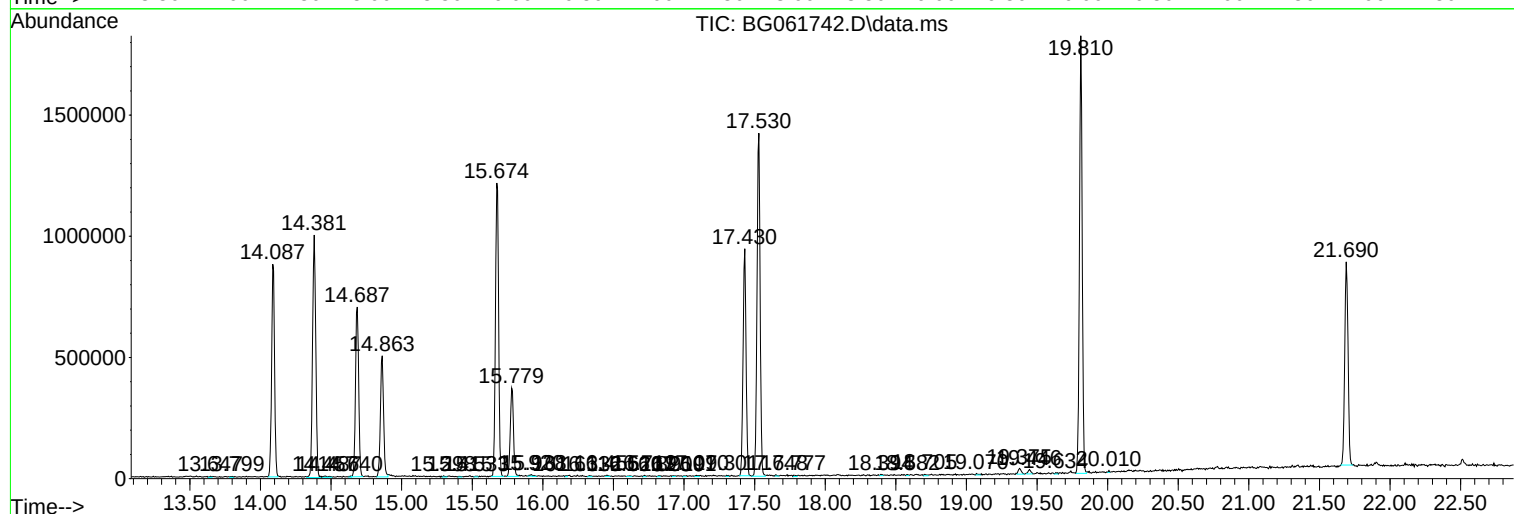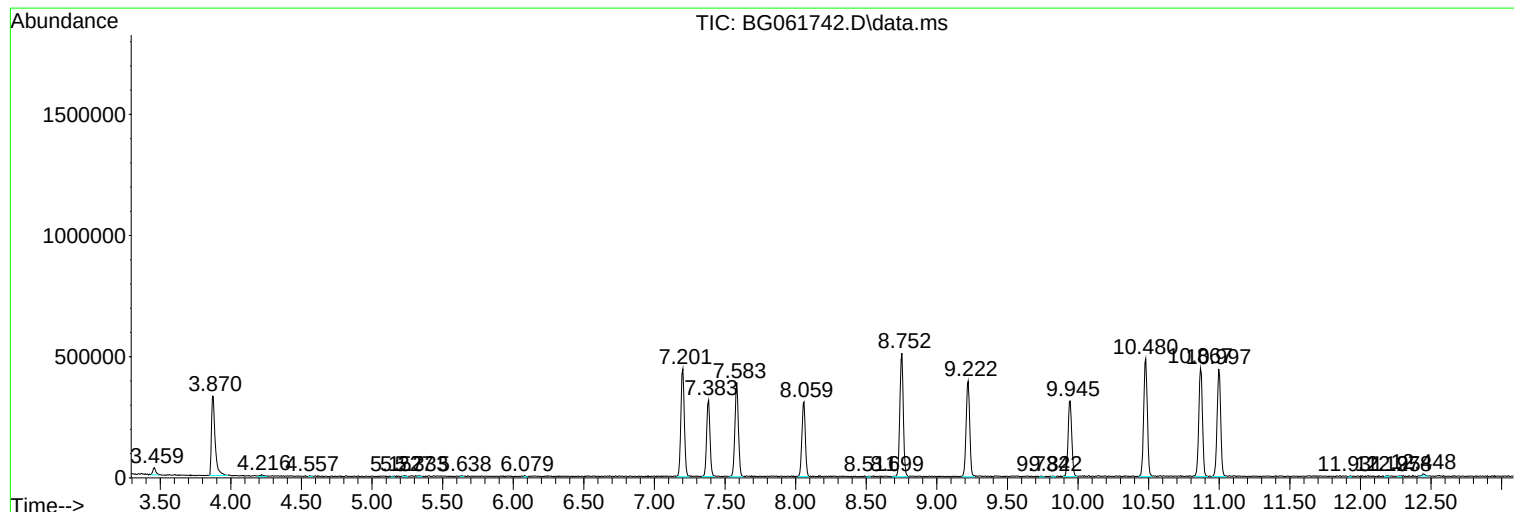

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061742.D
Acq On : 27 Jun 2024 17:00
Operator : MA/JU
Sample : PB161760BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK760

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061742.D
Acq On : 27 Jun 2024 17:00
Operator : MA/JU
Sample : PB161760BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK760

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------