

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
 Data File : BG061743.D
 Acq On : 27 Jun 2024 17:42
 Operator : MA/JU
 Sample : PB161561BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK561

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061743.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.459	24	29	34	rBV3	25800	42664	1.88%	0.174%
2	3.870	95	99	116	rBV	325656	562156	24.79%	2.288%
3	4.058	129	131	133	rBV2	4158	3818	0.17%	0.016%
4	4.205	155	156	162	rBV4	4527	4509	0.20%	0.018%
5	4.399	187	189	192	rVB4	3528	3524	0.16%	0.014%
6	4.846	262	265	267	rBV3	2233	3060	0.13%	0.012%
7	4.945	280	282	286	rVB4	3515	3803	0.17%	0.015%
8	4.992	286	290	293	rBV4	4635	6519	0.29%	0.027%
9	5.233	329	331	334	rVB3	3665	3242	0.14%	0.013%
10	5.263	334	336	338	rBV4	3436	3651	0.16%	0.015%
11	5.639	396	400	403	rVB3	3019	4012	0.18%	0.016%
12	5.756	418	420	425	rBV3	3451	4079	0.18%	0.017%
13	6.532	551	552	555	rVB2	3646	3278	0.14%	0.013%
14	6.790	593	596	598	rBV	3389	4308	0.19%	0.018%
15	6.972	625	627	631	rVB3	2898	3752	0.17%	0.015%
16	7.202	656	666	674	rBV	391992	688295	30.35%	2.801%
17	7.331	686	688	689	rBV2	3608	3159	0.14%	0.013%
18	7.384	689	697	706	rVB	275628	469925	20.72%	1.912%
19	7.584	723	731	738	rVV	360599	594231	26.20%	2.418%
20	7.648	741	742	748	rVV3	3720	4688	0.21%	0.019%
21	7.713	748	753	754	rVB2	2999	3791	0.17%	0.015%
22	8.054	804	811	818	rBV	291192	507480	22.38%	2.065%
23	8.576	895	900	902	rBV3	3576	6202	0.27%	0.025%
24	8.670	912	916	919	rVB4	2380	3416	0.15%	0.014%
25	8.753	922	930	937	rBV	461770	795282	35.07%	3.236%
26	8.958	963	965	968	rBV3	3027	3742	0.17%	0.015%
27	9.223	1002	1010	1018	rBV2	352112	616438	27.18%	2.509%
28	9.364	1030	1034	1036	rVB3	2988	3616	0.16%	0.015%
29	9.399	1036	1040	1044	rBV5	3749	4871	0.21%	0.020%
30	9.434	1044	1046	1049	rBV3	3542	3658	0.16%	0.015%
31	9.728	1092	1096	1097	rVB2	2704	3059	0.13%	0.012%
32	9.746	1097	1099	1103	rBV4	3172	4141	0.18%	0.017%
33	9.940	1125	1132	1139	rBV	284220	517024	22.80%	2.104%
34	10.110	1155	1161	1164	rVB3	2995	4512	0.20%	0.018%
35	10.474	1215	1223	1231	rBV	436830	791661	34.91%	3.222%
36	10.762	1270	1272	1275	rVB2	3511	4002	0.18%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
 Data File : BG061743.D
 Acq On : 27 Jun 2024 17:42
 Operator : MA/JU
 Sample : PB161561BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK561

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	10.868	1281	1290	1300	rVB	433685	800335	35.29%	3.257%
38	10.944	1300	1303	1305	rBV2	3332	4315	0.19%	0.018%
39	10.997	1305	1312	1322	rBV	398150	715644	31.56%	2.912%
40	11.491	1392	1396	1399	rBV3	2413	3062	0.14%	0.012%
41	11.996	1480	1482	1486	rVB2	2949	3305	0.15%	0.013%
42	12.131	1504	1505	1509	rBV2	2647	3943	0.17%	0.016%
43	12.284	1529	1531	1534	rBV4	3175	3374	0.15%	0.014%
44	12.443	1554	1558	1562	rBV3	10417	12283	0.54%	0.050%
45	12.666	1592	1596	1599	rBV4	3121	3929	0.17%	0.016%
46	12.889	1632	1634	1637	rVB4	4198	4296	0.19%	0.017%
47	12.918	1637	1639	1642	rBV3	3738	3954	0.17%	0.016%
48	13.324	1703	1708	1711	rBV4	2577	4571	0.20%	0.019%
49	13.477	1729	1734	1735	rBV2	3181	4978	0.22%	0.020%
50	13.530	1740	1743	1745	rVB	4779	3666	0.16%	0.015%
51	13.847	1795	1797	1800	rVB2	3826	3343	0.15%	0.014%
52	14.088	1832	1838	1846	rVB	818722	1164006	51.33%	4.737%
53	14.152	1846	1849	1851	rVB3	2651	3072	0.14%	0.013%
54	14.176	1851	1853	1857	rBV2	3283	3240	0.14%	0.013%
55	14.252	1862	1866	1871	rVB3	2245	3797	0.17%	0.015%
56	14.381	1881	1888	1895	rVB	884368	1372167	60.51%	5.584%
57	14.575	1918	1921	1923	rBV3	3556	4144	0.18%	0.017%
58	14.687	1932	1940	1948	rVB	699817	1063915	46.92%	4.329%
59	14.763	1951	1953	1958	rBV3	4016	6324	0.28%	0.026%
60	14.863	1963	1970	1976	rBV	440655	696296	30.71%	2.833%
61	14.963	1985	1987	1990	rVB4	5132	4693	0.21%	0.019%
62	15.063	2003	2004	2007	rBV2	3991	3960	0.17%	0.016%
63	15.280	2038	2041	2043	rBV3	3497	3715	0.16%	0.015%
64	15.327	2045	2049	2050	rVV2	3303	3861	0.17%	0.016%
65	15.363	2053	2055	2058	rBV	5688	5686	0.25%	0.023%
66	15.674	2101	2108	2118	rBV	1137949	1731395	76.35%	7.046%
67	15.780	2118	2126	2132	rBV	363825	522201	23.03%	2.125%
68	15.915	2145	2149	2153	rVB5	8023	11941	0.53%	0.049%
69	15.950	2153	2155	2159	rBV2	2623	3673	0.16%	0.015%
70	16.179	2192	2194	2197	rVB4	4400	4764	0.21%	0.019%
71	16.285	2210	2212	2215	rBV2	4185	3687	0.16%	0.015%
72	16.420	2233	2235	2238	rVB3	4719	4191	0.18%	0.017%
73	16.455	2238	2241	2244	rBV3	6177	8735	0.39%	0.036%
74	16.620	2267	2269	2271	rBV3	4568	3745	0.17%	0.015%
75	16.931	2321	2322	2325	rBV2	3722	3328	0.15%	0.014%
76	17.002	2332	2334	2336	rVB2	4868	3085	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061743.D
Acq On : 27 Jun 2024 17:42
Operator : MA/JU
Sample : PB161561BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK561

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Title : SVOA CALIBRATION

77	17.078	2345	2347	2350	rBV3	3232	4263	0.19%	0.017%
78	17.213	2368	2370	2371	rBV	5632	3061	0.13%	0.012%
79	17.431	2400	2407	2413	rBV	912878	1372881	60.54%	5.587%
80	17.531	2417	2424	2432	rVB2	1296957	1993443	87.91%	8.112%
81	17.660	2444	2446	2448	rVB3	4958	3882	0.17%	0.016%
82	18.206	2537	2539	2541	rBV2	3687	4308	0.19%	0.018%
83	18.794	2635	2639	2640	rBV	5998	7536	0.33%	0.031%
84	18.812	2640	2642	2644	rVB3	6151	4452	0.20%	0.018%
85	19.146	2697	2699	2701	rBV2	7034	6196	0.27%	0.025%
86	19.376	2734	2738	2743	rVV4	17978	27543	1.21%	0.112%
87	19.440	2747	2749	2754	rVB	19320	21745	0.96%	0.088%
88	19.810	2805	2812	2820	rBV	1581818	2267675	100.00%	9.228%
89	21.691	3125	3132	3142	rBV	890320	1431132	63.11%	5.824%
90	24.687	3633	3642	3658	rVB3	766593	2114245	93.23%	8.604%
91	24.904	3670	3679	3689	rBV	495338	1407176	62.05%	5.726%




Sum of corrected areas: 24573725

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061743.D
Acq On : 27 Jun 2024 17:42
Operator : MA/JU
Sample : PB161561BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK561

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

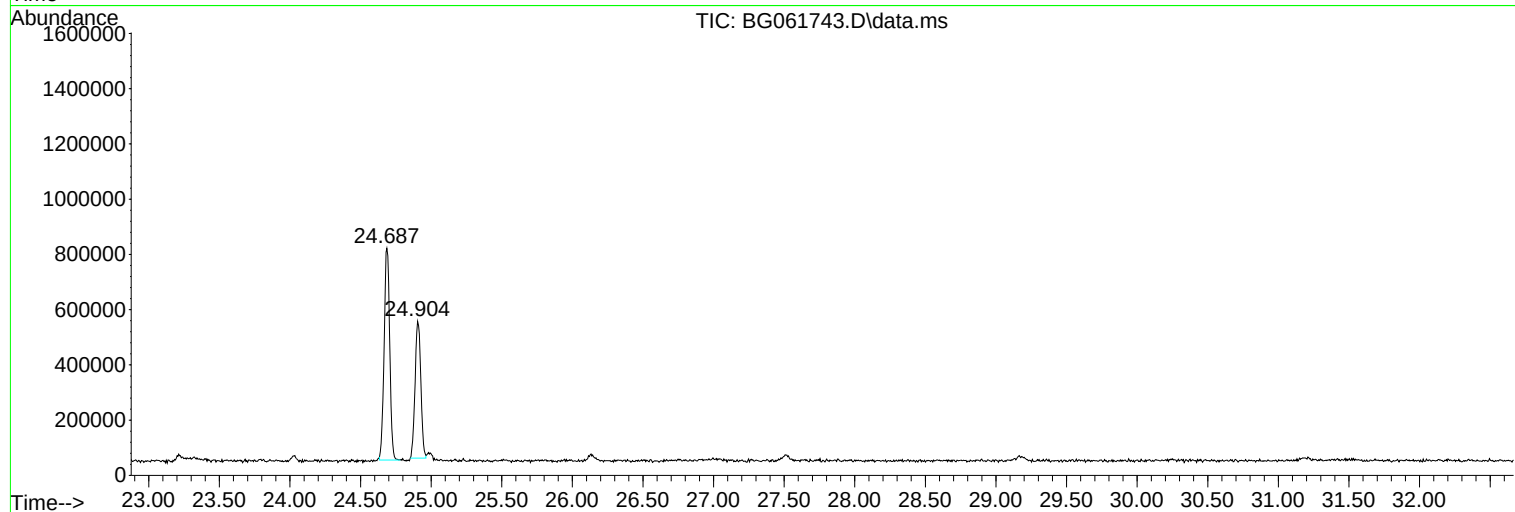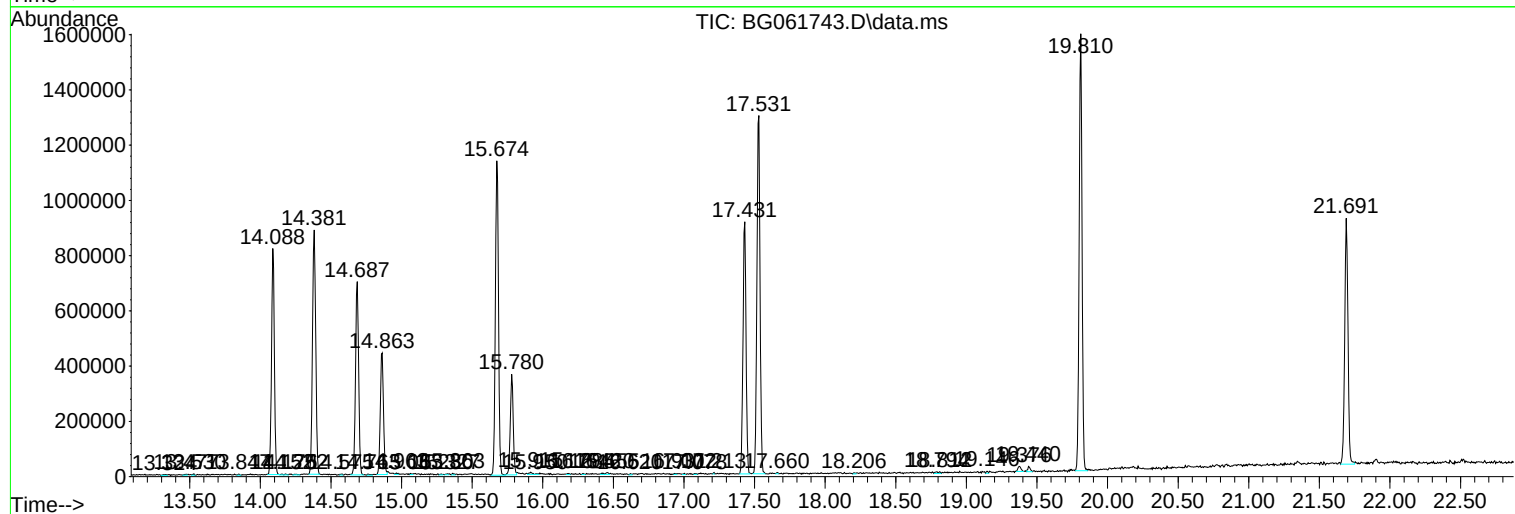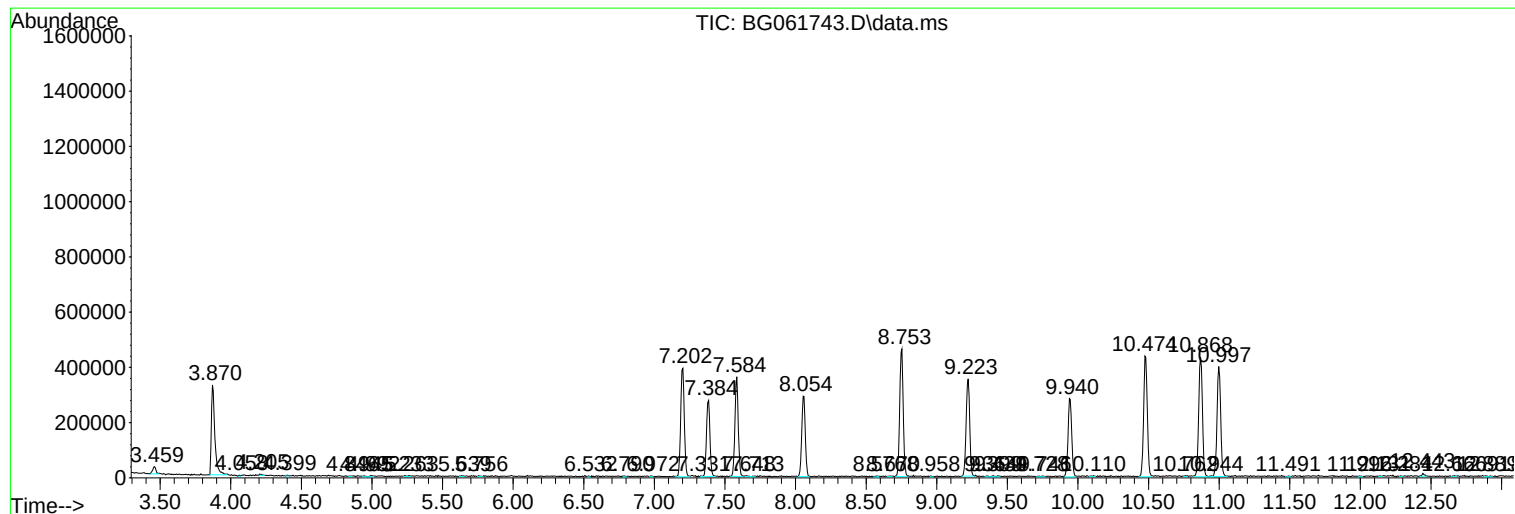

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061743.D
Acq On : 27 Jun 2024 17:42
Operator : MA/JU
Sample : PB161561BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK561

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061743.D
Acq On : 27 Jun 2024 17:42
Operator : MA/JU
Sample : PB161561BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK561

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc