

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
 Data File : BG061748.D
 Acq On : 27 Jun 2024 21:07
 Operator : MA/JU
 Sample : P3055-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E08D7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BG061748.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	7	12	16	rBV6	7678	12642	0.40%	0.046%
2	3.458	24	29	38	rVB3	21373	41484	1.32%	0.150%
3	3.558	44	46	50	rVB4	5983	6187	0.20%	0.022%
4	3.875	98	100	110	rBV	66606	122094	3.88%	0.442%
5	4.216	155	158	161	rVB4	7567	8870	0.28%	0.032%
6	4.580	217	220	223	rBV3	2824	4188	0.13%	0.015%
7	5.144	312	316	317	rVB4	4252	5508	0.17%	0.020%
8	6.966	621	626	627	rBV3	2889	4241	0.13%	0.015%
9	7.095	644	648	652	rBV4	3868	5197	0.17%	0.019%
10	7.130	652	654	657	rVB2	4289	4656	0.15%	0.017%
11	7.195	657	665	673	rBV2	171229	303716	9.64%	1.098%
12	7.383	690	697	707	rBV	406923	674992	21.43%	2.441%
13	7.583	724	731	738	rBV	464690	782277	24.84%	2.829%
14	8.053	805	811	819	rVB	265637	458905	14.57%	1.660%
15	8.746	923	929	940	rVB	404450	697572	22.15%	2.523%
16	9.157	990	999	1002	rBV6	6785	16058	0.51%	0.058%
17	9.222	1002	1010	1017	rBV	533577	933082	29.63%	3.374%
18	9.563	1065	1068	1070	rVB3	4271	4831	0.15%	0.017%
19	9.945	1124	1133	1139	rBV	436981	778749	24.73%	2.816%
20	10.103	1158	1160	1164	rBV2	2896	4242	0.13%	0.015%
21	10.479	1216	1224	1231	rBV	630430	1127948	35.82%	4.079%
22	10.867	1282	1290	1297	rBV2	396722	714423	22.68%	2.584%
23	10.996	1305	1312	1319	rBV2	136925	248334	7.89%	0.898%
24	11.513	1398	1400	1405	rVB2	3731	4441	0.14%	0.016%
25	11.960	1473	1476	1478	rBV	3592	4726	0.15%	0.017%
26	12.318	1535	1537	1540	rBV2	3420	4259	0.14%	0.015%
27	12.442	1556	1558	1564	rVB5	11178	17341	0.55%	0.063%
28	13.840	1795	1796	1800	rVB	4618	4328	0.14%	0.016%
29	14.087	1832	1838	1845	rBV	1139302	1670990	53.06%	6.043%
30	14.381	1881	1888	1899	rVB	1256857	1944717	61.75%	7.033%
31	14.539	1911	1915	1916	rBV3	4174	4745	0.15%	0.017%
32	14.686	1933	1940	1947	rVB	628866	974945	30.96%	3.526%
33	14.857	1963	1969	1976	rBV2	171533	265389	8.43%	0.960%
34	15.092	2003	2009	2011	rBV5	10637	13867	0.44%	0.050%
35	15.409	2061	2063	2066	rVB3	3964	4438	0.14%	0.016%
36	15.673	2102	2108	2116	rVB	1669628	2466527	78.32%	8.920%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
 Data File : BG061748.D
 Acq On : 27 Jun 2024 21:07
 Operator : MA/JU
 Sample : P3055-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E08D7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
 Title : SVOA CALIBRATION

37	15.779	2119	2126	2135	rBV	571906	807534	25.64%	2.920%
38	15.902	2146	2147	2155	rVB6	9029	15244	0.48%	0.055%
39	16.231	2201	2203	2207	rVB3	5547	7360	0.23%	0.027%
40	16.566	2257	2260	2263	rBV2	5109	5099	0.16%	0.018%
41	17.089	2345	2349	2352	rBV3	3994	8127	0.26%	0.029%
42	17.424	2400	2406	2413	rBV	806134	1213209	38.52%	4.387%
43	17.524	2417	2423	2433	rVV	1827278	2794064	88.72%	10.104%
44	18.088	2517	2519	2524	rVB4	10038	10035	0.32%	0.036%
45	18.211	2537	2540	2542	rBV4	6354	7636	0.24%	0.028%
46	18.376	2566	2568	2573	rBV6	4346	6661	0.21%	0.024%
47	19.140	2696	2698	2699	rBV	6200	4328	0.14%	0.016%
48	19.275	2719	2721	2723	rBV2	6371	5732	0.18%	0.021%
49	19.369	2735	2737	2743	rVB3	28272	37246	1.18%	0.135%
50	19.445	2746	2750	2753	rVB2	22360	28110	0.89%	0.102%
51	19.733	2796	2799	2804	rBV6	10352	12456	0.40%	0.045%
52	19.810	2805	2812	2822	rVV	2180340	3149365	100.00%	11.389%
53	20.773	2974	2976	2979	rVB3	17125	15601	0.50%	0.056%
54	21.690	3126	3132	3138	rBV2	690254	1139700	36.19%	4.121%
55	24.686	3632	3642	3654	rVB2	1087662	2925756	92.90%	10.580%
56	24.904	3670	3679	3688	rBV2	397230	1095916	34.80%	3.963%
57	26.102	3881	3883	3884	rBV2	21685	15481	0.49%	0.056%
58	30.021	4548	4550	4551	rBV	13436	7608	0.24%	0.028%




Sum of corrected areas: 27653177

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061748.D
Acq On : 27 Jun 2024 21:07
Operator : MA/JU
Sample : P3055-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E08D7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

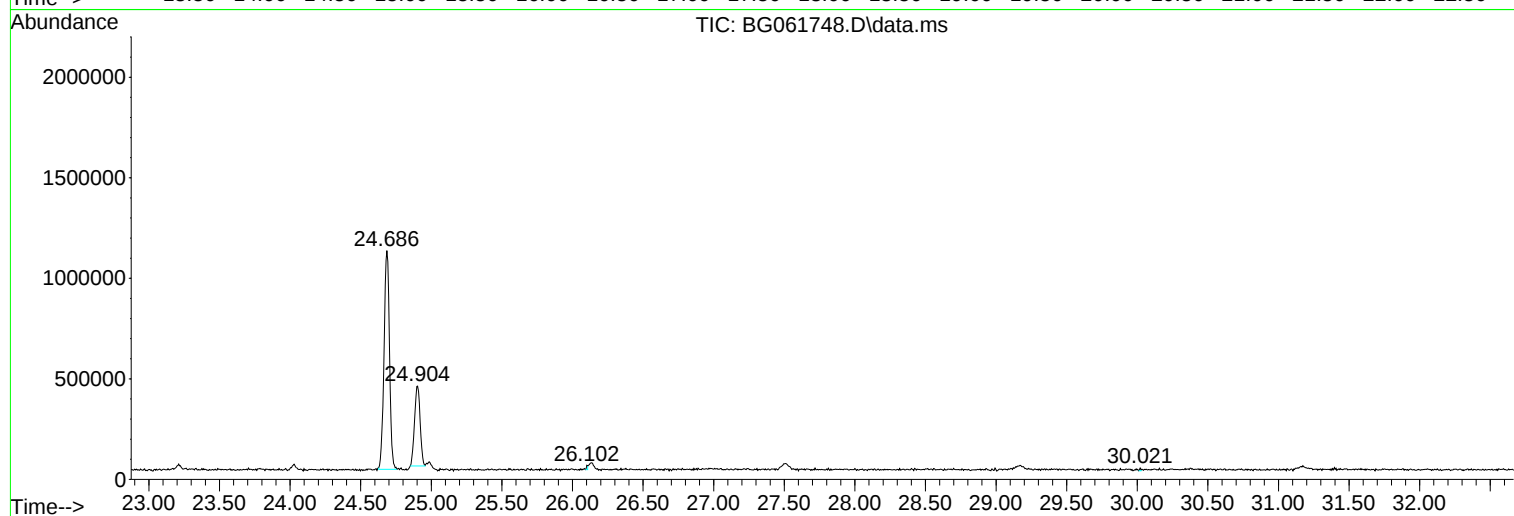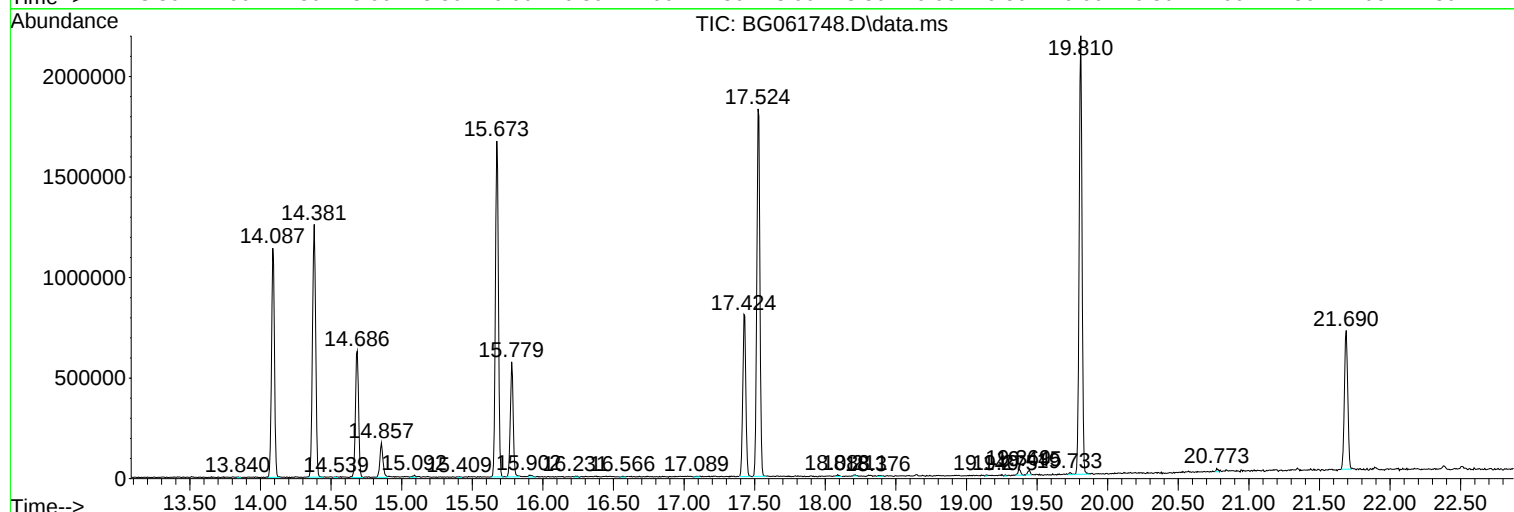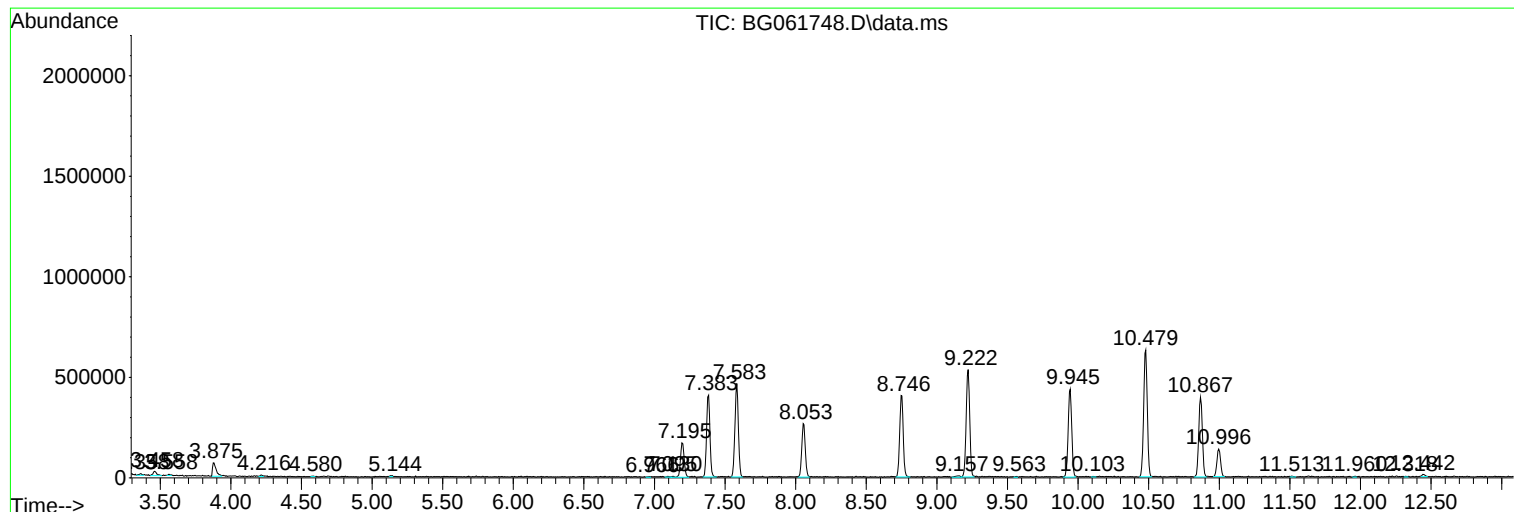

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061748.D
Acq On : 27 Jun 2024 21:07
Operator : MA/JU
Sample : P3055-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E08D7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062724\
Data File : BG061748.D
Acq On : 27 Jun 2024 21:07
Operator : MA/JU
Sample : P3055-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E08D7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG062024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc