
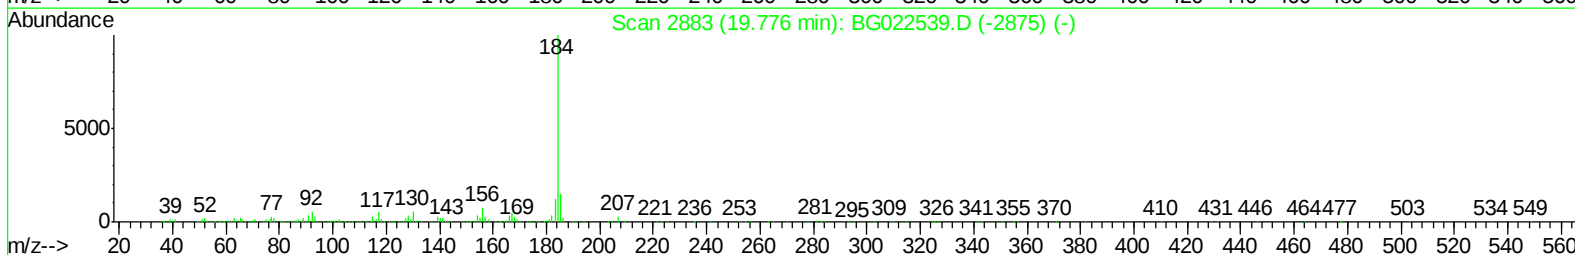
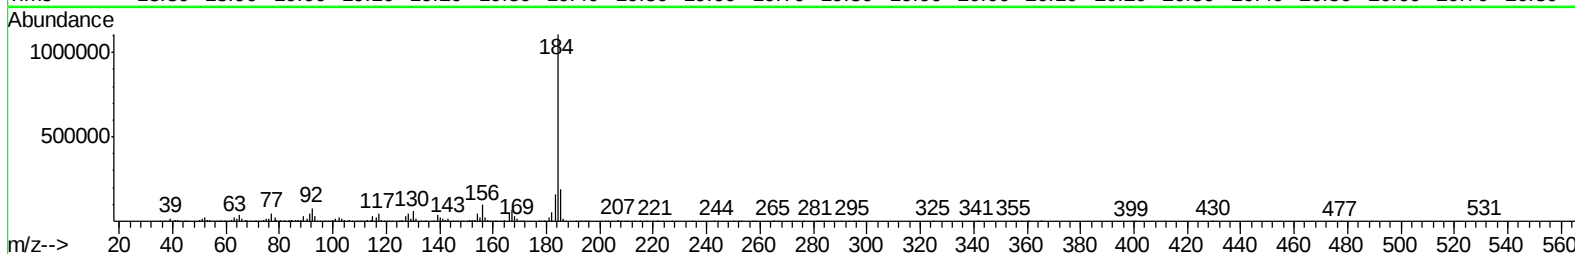


Data Path : Z:\HPCHEM1\BNA_G\Data\BG062816\
 Data File : BG022668.D
 Acq On : 28 Jun 2016 8:48
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 07:26:52 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 24 20:14:59 2016
 Response via : Initial Calibration

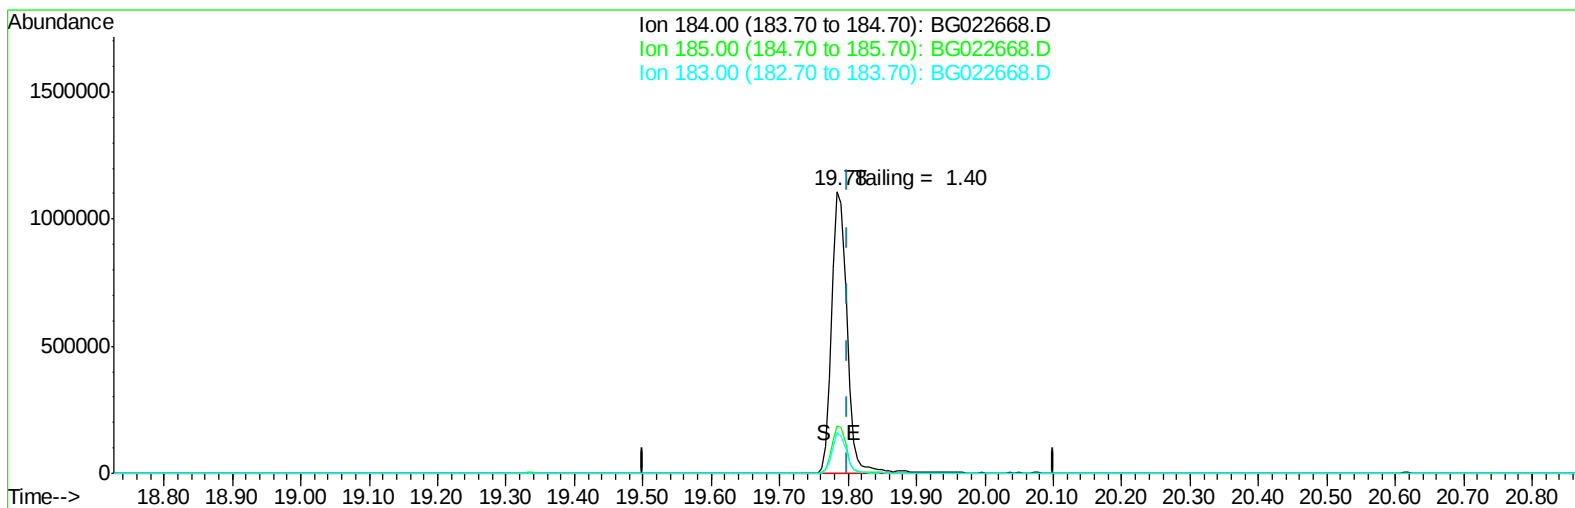

TIC: BG022668.D

(76) Benzidine




19.784min (-0.016) 73031.91ng

response 1710600

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	16.91
183.00	13.40	14.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG062816\
Data File : BG022668.D
Acq On : 28 Jun 2016 8:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 07:26:52 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

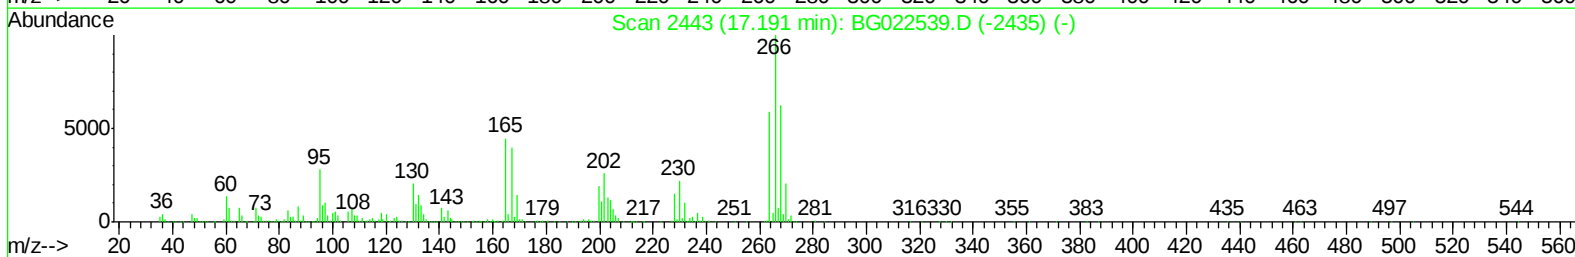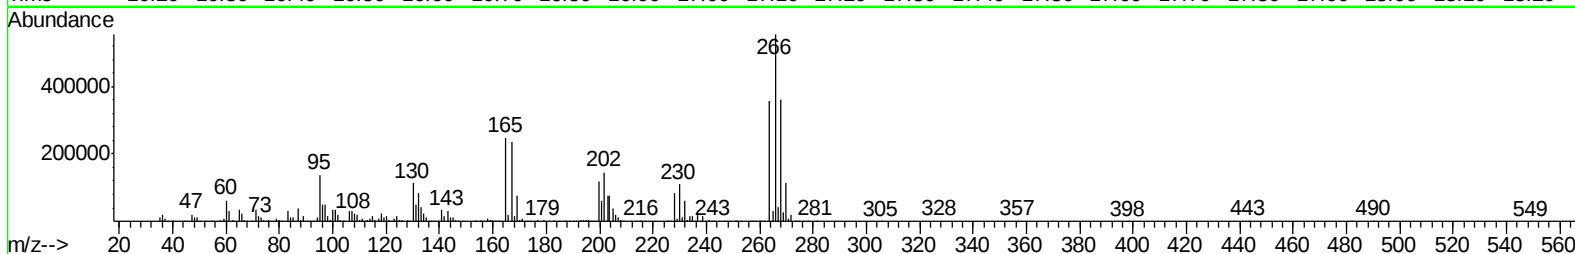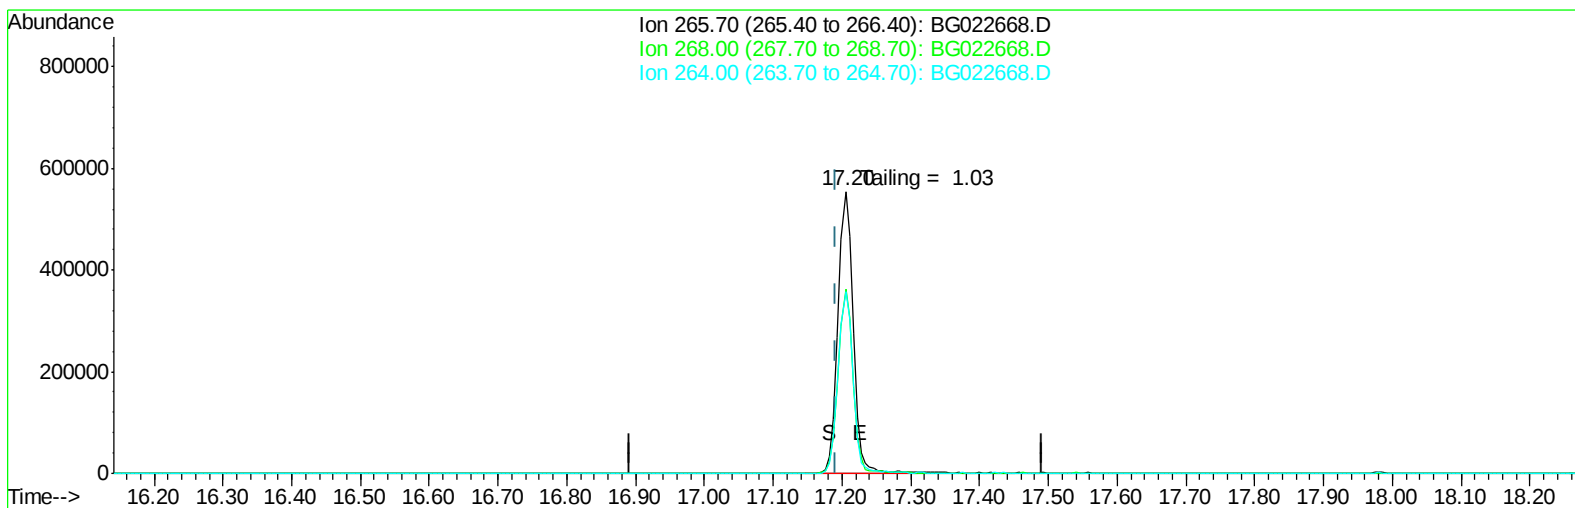

TIC: BG022668.D

(69) Pentachlorophenol (C)

17.205min (+0.013) 50640.44ng

response 838979

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	65.32
264.00	63.20	64.69
0.00	0.00	0.00