
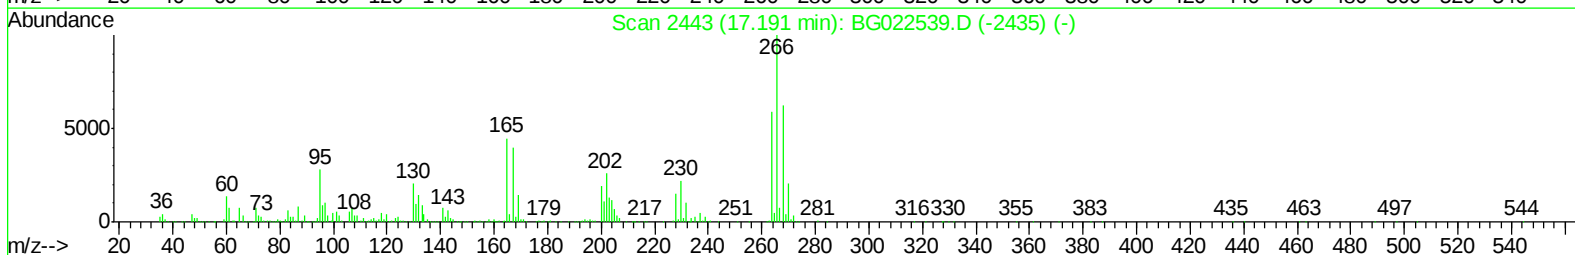
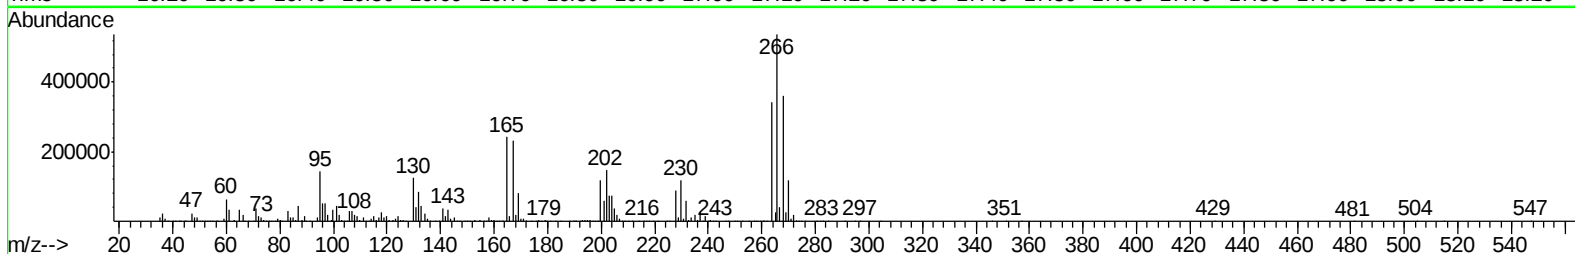


Data Path : Z:\HPCHEM1\BNA_G\Data\BG062816\
Data File : BG022679.D
Acq On : 28 Jun 2016 17:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 07:27:36 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

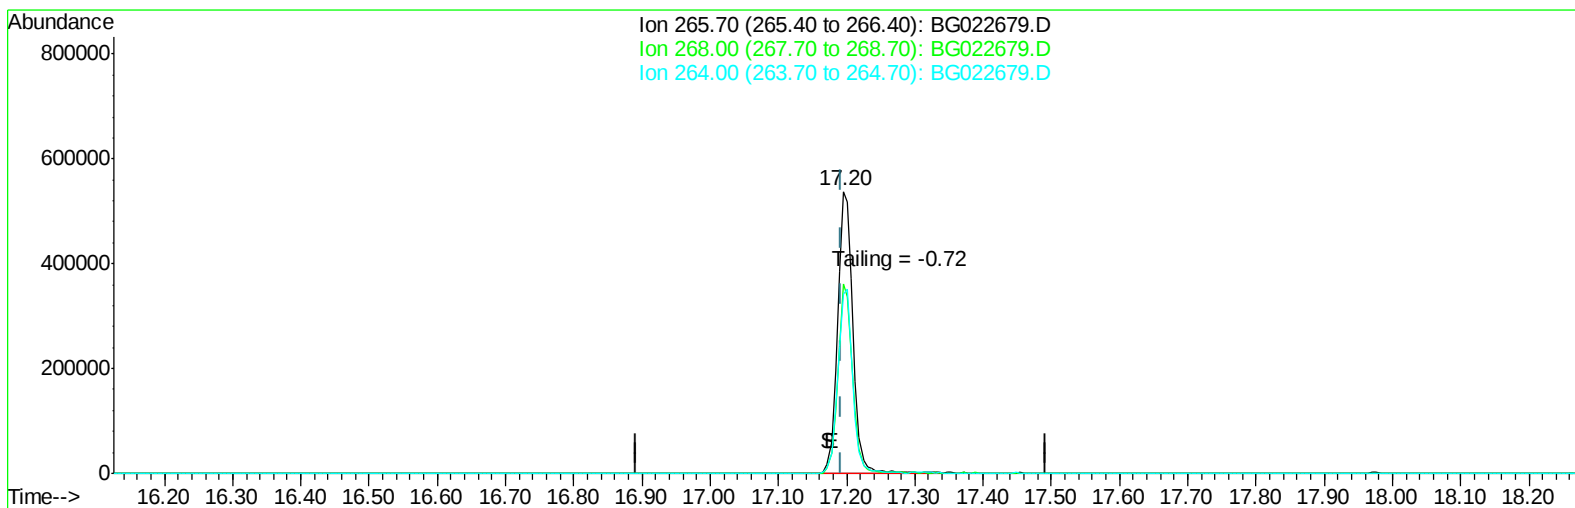

TIC: BG022679.D

(69) Pentachlorophenol (C)




17.195min (+0.003) 393005.35ng m

response 857012

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	67.22
264.00	63.20	63.43
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG062816\
Data File : BG022679.D
Acq On : 28 Jun 2016 17:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 07:27:36 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

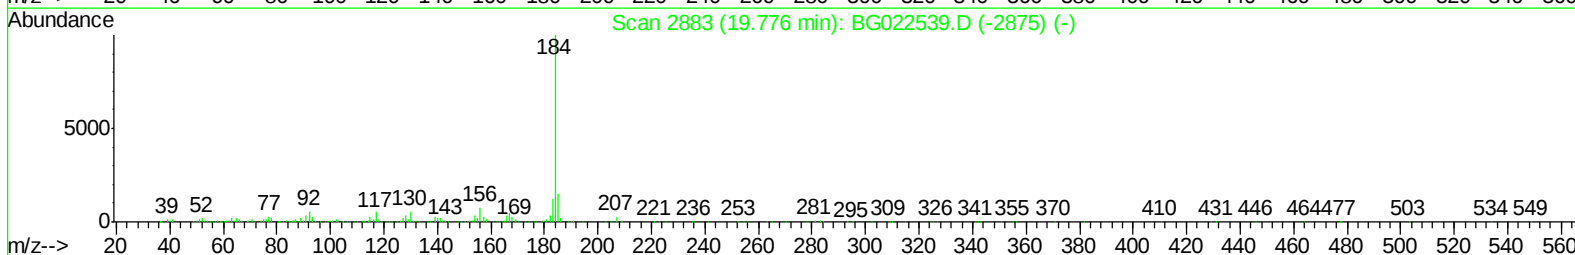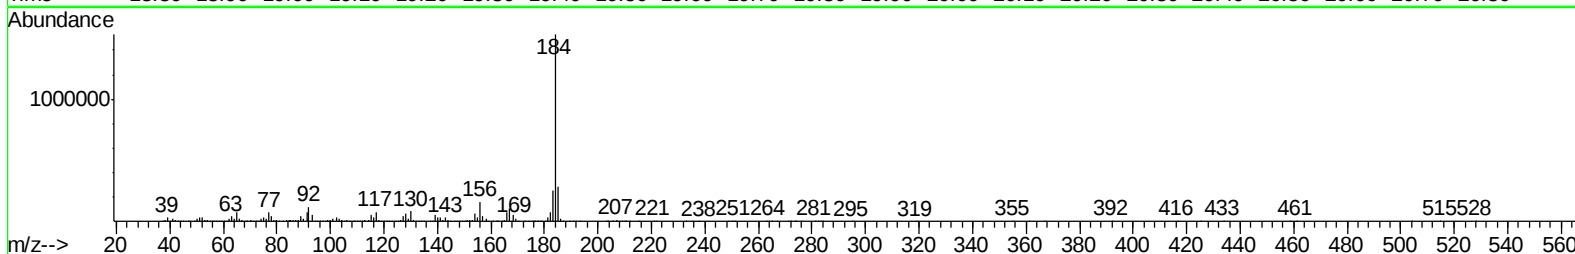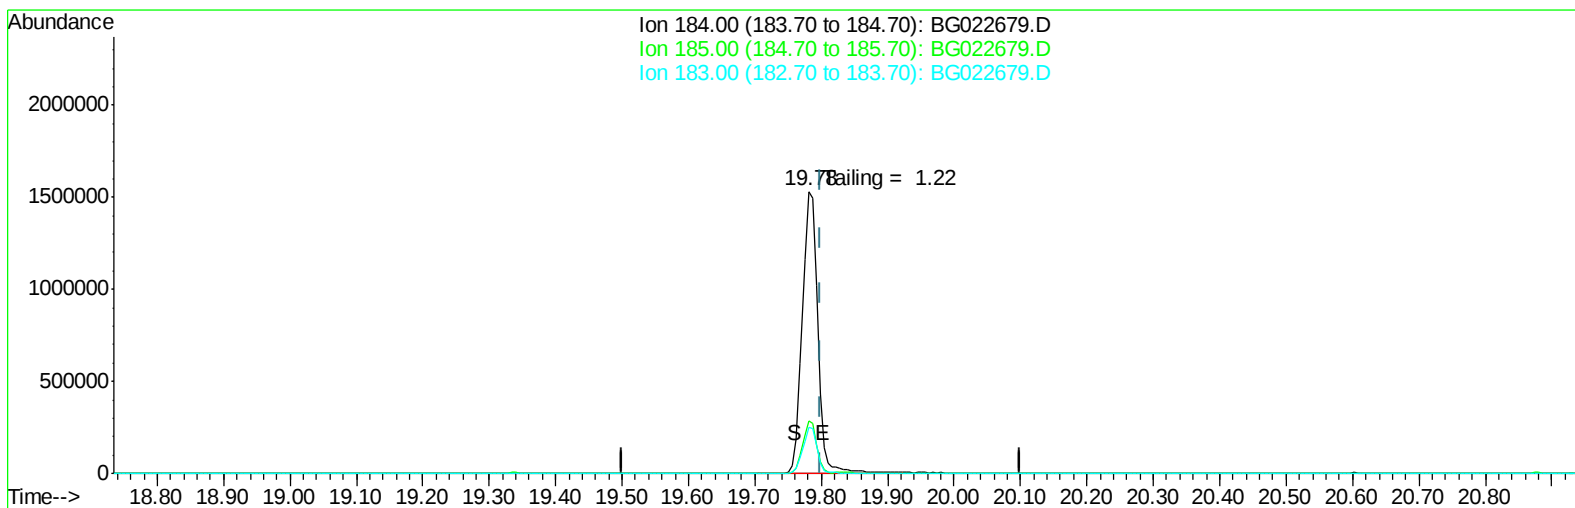

TIC: BG022679.D

(76) Benzidine

19.780min (-0.020) 831653.32ng

response 2452648

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	18.49
183.00	13.40	16.53#
0.00	0.00	0.00