


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062816\
 Data File : BG022679.D
 Acq On : 28 Jun 2016 17:06
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 20:14:59 2016

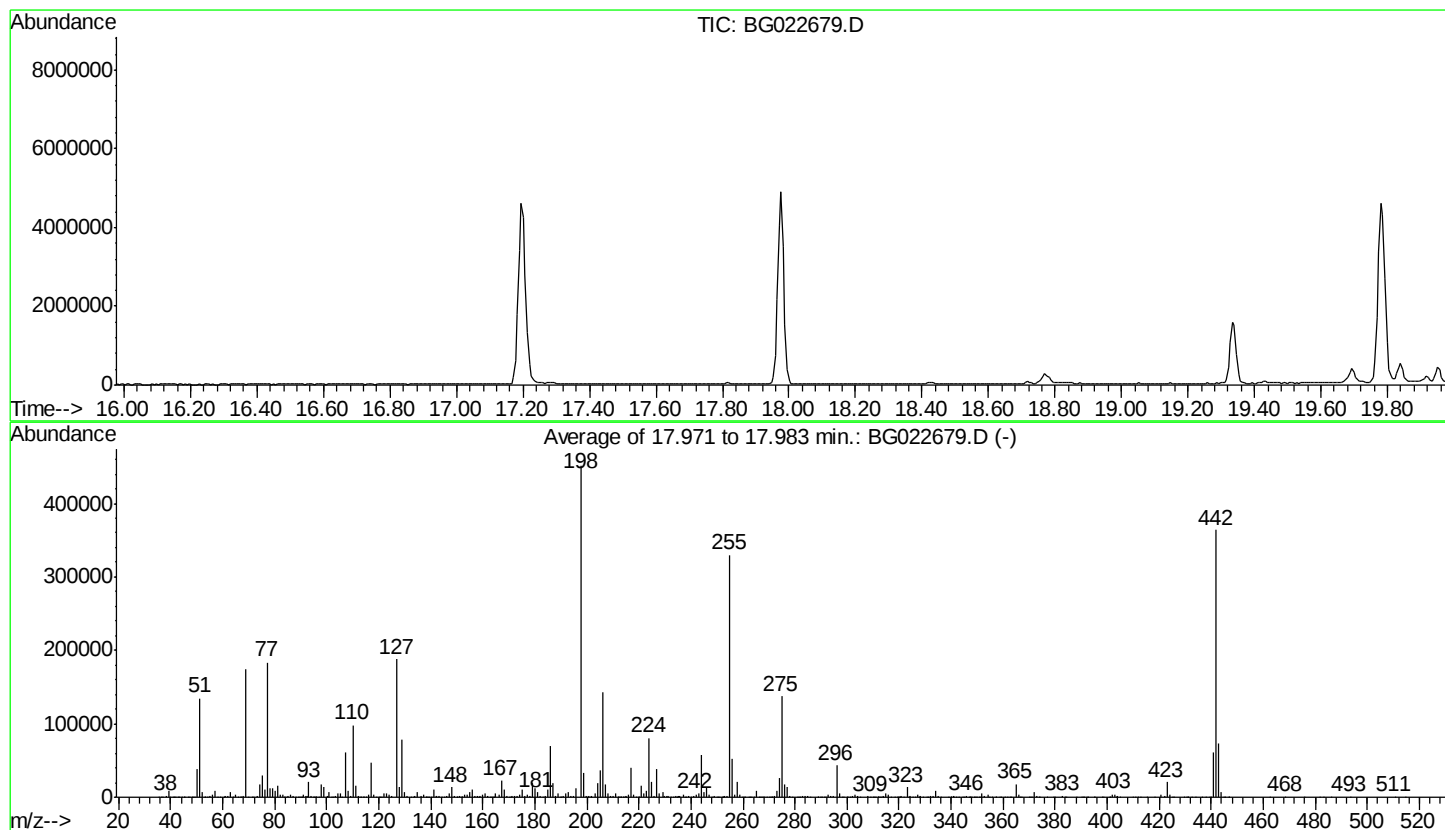

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	134656	PASS
68	69	0.00	2	0.6	1001	PASS
69	198	0.00	100	38.5	173832	PASS
70	69	0.00	2	0.5	841	PASS
127	198	10	80	41.7	188096	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	451541	PASS
199	198	5	9	7.2	32698	PASS
275	198	10	60	30.5	137512	PASS
365	198	1	100	4.0	18223	PASS
441	442	0.01	24	16.7	60714	PASS
442	198	50	100	80.7	364202	PASS
443	442	15	24	20.3	73938	PASS