

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG062817\
 Data File : BG027733.D
 Acq On : 29 Jun 2017 9:17
 Operator : SJ/JU
 Sample : I3926-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP1-B-COMP

Quant Time: Jun 29 12:20:01 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 19:26:37 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.48	152	33921	20.00	ng	0.00
21) Naphthalene-d8	11.29	136	156993	20.00	ng	0.00
38) Acenaphthene-d10	15.06	164	90978	20.00	ng	0.00
63) Phenanthrene-d10	17.81	188	246637	20.00	ng	0.00
75) Chrysene-d12	22.17	240	264020	20.00	ng	0.00
86) Perylene-d12	25.78	264	254676	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.06	112	333395	151.35	ng	0.00
7) Phenol-d6	7.62	99	436027	129.57	ng	0.00
23) Nitrobenzene-d5	9.64	82	287439	102.06	ng	0.00
41) 2,4,6-Tribromophenol	16.55	330	228429	183.06	ng	0.00
44) 2-Fluorobiphenyl	13.69	172	673727	105.76	ng	0.00
78) Terphenyl-d14	20.39	244	1312134	116.51	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG062817\
Data File : BG027733.D
Acq On : 29 Jun 2017 9:17
Operator : SJ/JU
Sample : I3926-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP1-B-COMP

Quant Time: Jun 29 12:20:01 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 19:26:37 2017
Response via : Initial Calibration

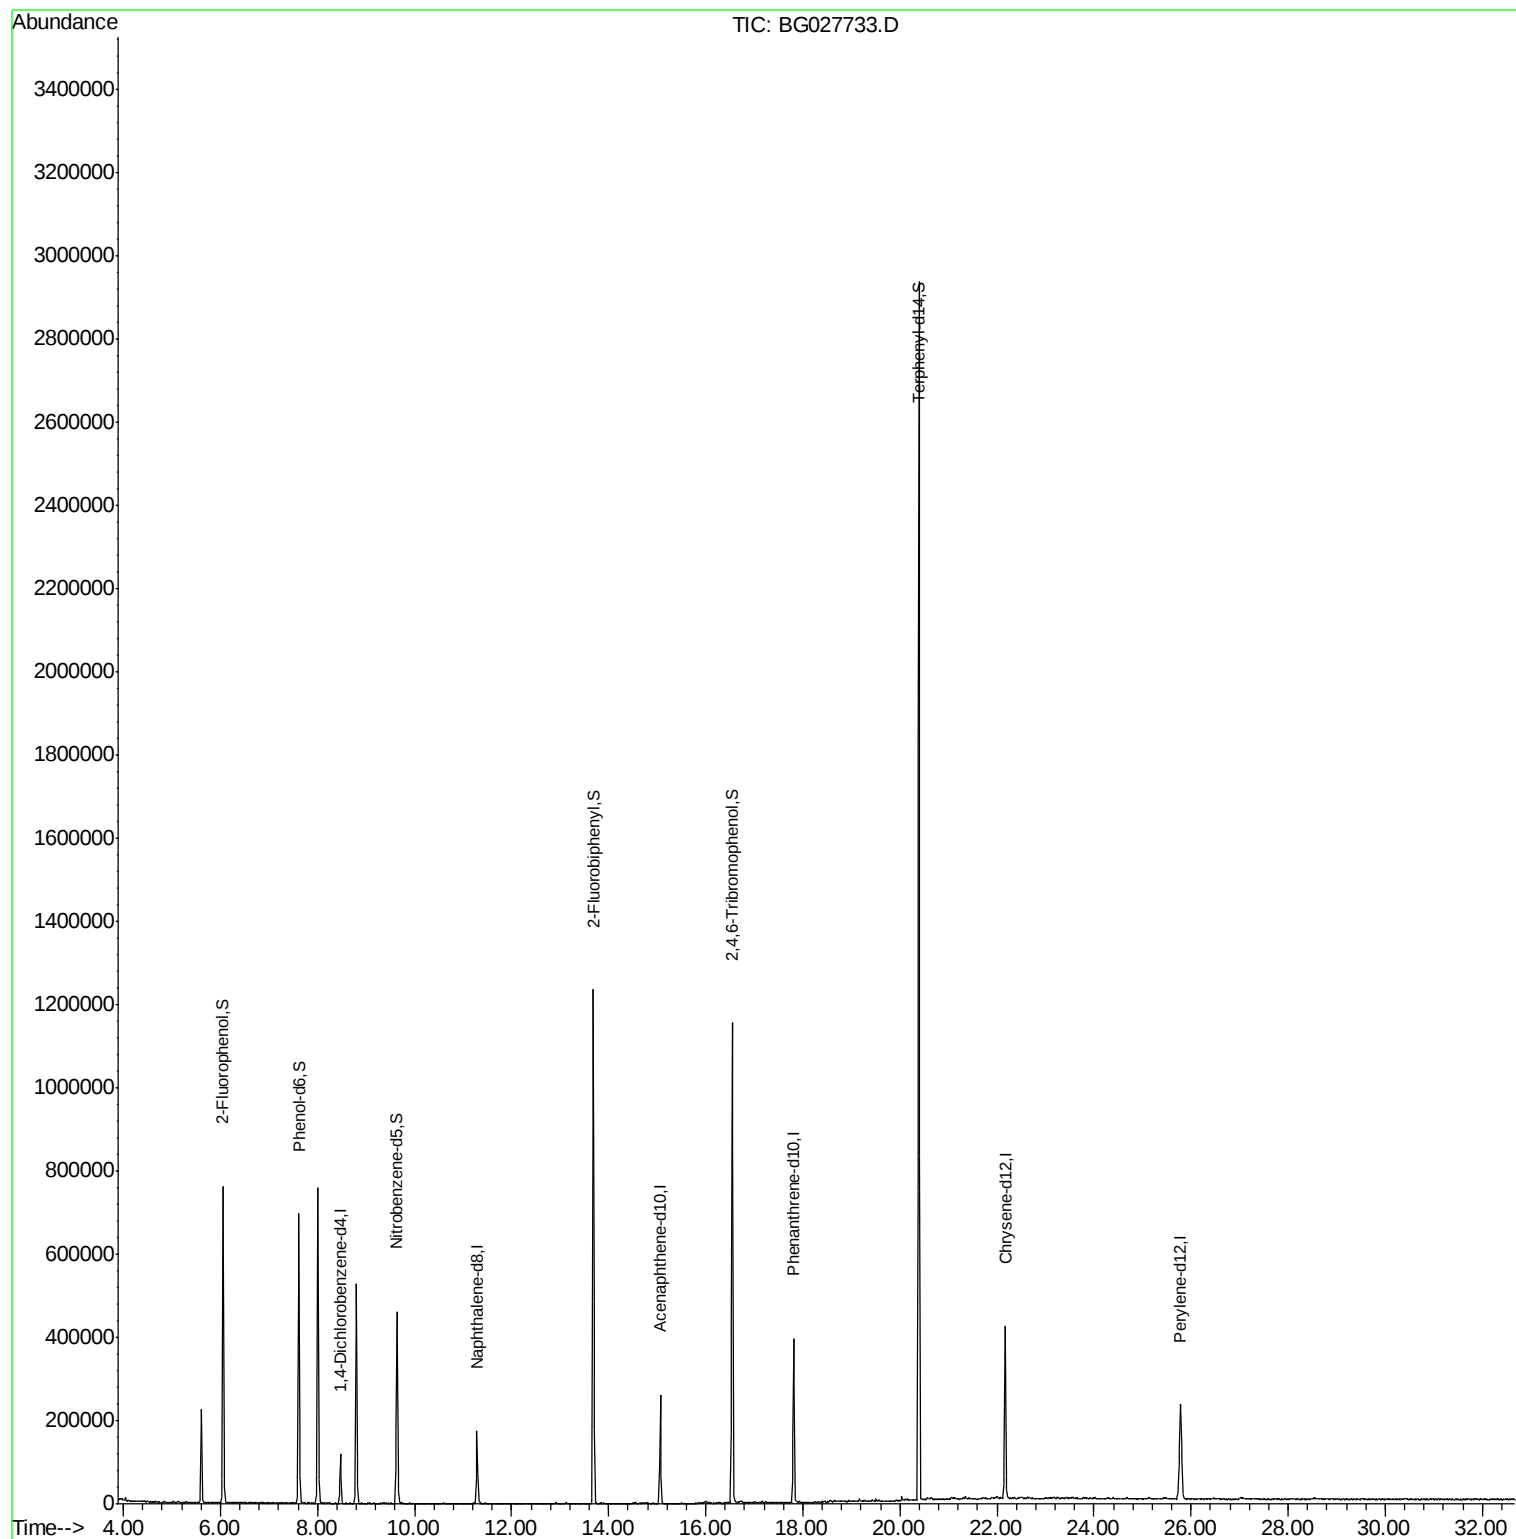




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.48 min Scan# 781
Delta R.T. -0.00 min
Lab File: BG027733.D
Acq: 29 Jun 2017 9:17

Instrument :
BNA_G
ClientSampleId :
SP1-B-COMP

Tgt Ion:152 Resp: 33921
Ion Ratio Lower Upper
152 100
150 150.8 114.0 171.0
115 58.9 48.1 72.1




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

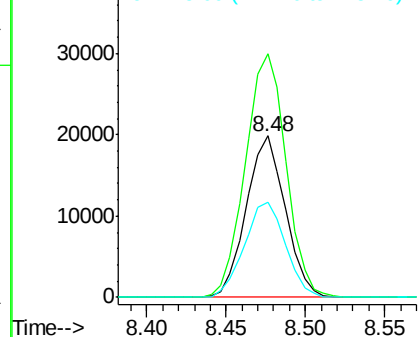



#5


2-Fluorophenol
Concen: 151.351 ng
RT: 6.06 min Scan# 369
Delta R.T. -0.00 min
Lab File: BG027733.D
Acq: 29 Jun 2017 9:17

Tgt Ion:112 Resp: 333395
Ion Ratio Lower Upper
112 100
64 72.4 61.8 92.6
63 37.1 37.2 55.8#



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

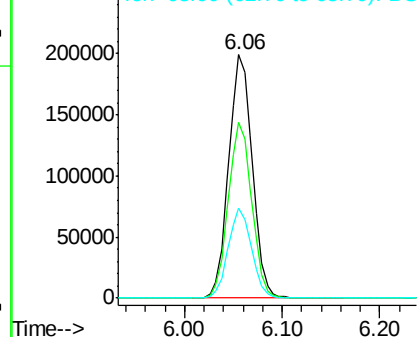

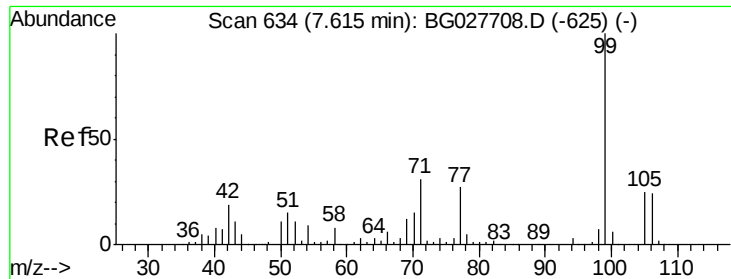

#7

Phenol-d6

Concen: 129.570 ng

RT: 7.62 min Scan# 635

Delta R.T. 0.00 min

Lab File: BG027733.D

Acq: 29 Jun 2017 9:17

Instrument :

BNA_G

ClientSampleId :

SP1-B-COMP


Tgt Ion: 99 Resp: 436027

Ion Ratio Lower Upper




99 100

42 18.5 20.5 30.7#

71 31.3 37.6 56.4#



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

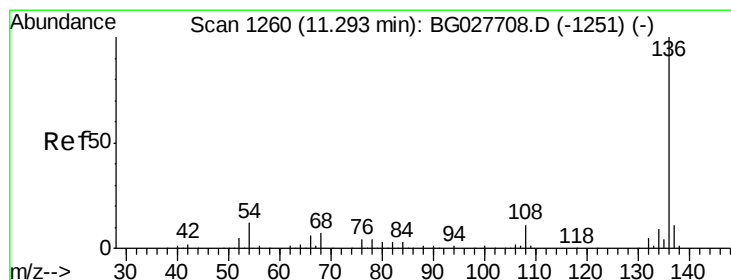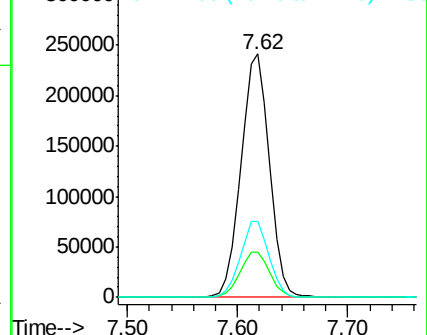

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.29 min Scan# 1260

Delta R.T. -0.00 min

Lab File: BG027733.D

Acq: 29 Jun 2017 9:17

Tgt Ion: 136 Resp: 156993


Ion Ratio Lower Upper

136 100



137 11.6 8.9 13.3


54 12.8 9.3 13.9

68 7.3 5.1 7.7

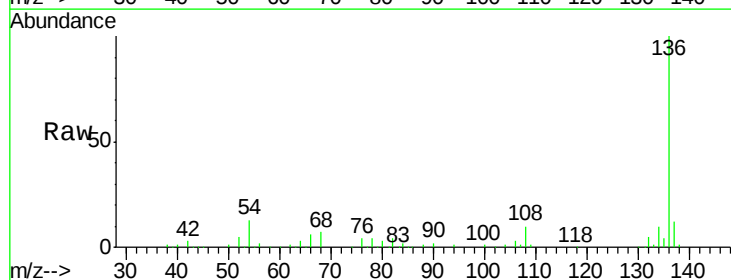

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

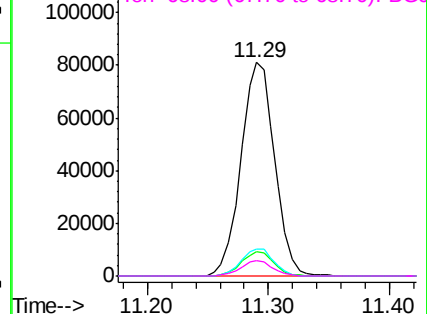


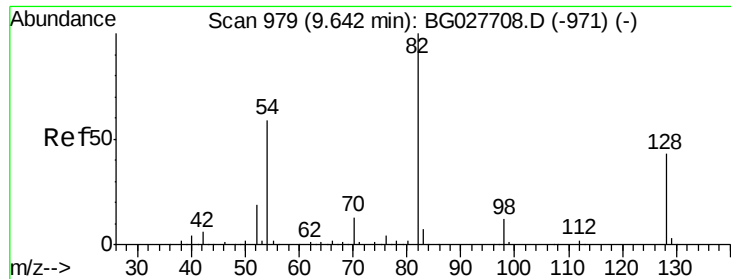




#23
 Nitrobenzene-d5
 Concen: 102.056 ng
 RT: 9.64 min Scan# 979
 Delta R.T. -0.00 min
 Lab File: BG027733.D
 Acq: 29 Jun 2017 9:17

Instrument :
 BNA_G
 ClientSampleId :
 SP1-B-COMP

Tgt Ion: 82 Resp: 287439
 Ion Ratio Lower Upper
 82 100
 128 43.0 26.4 39.6#
 54 58.0 49.4 74.2




Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC


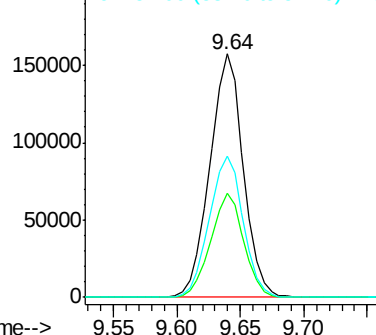



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.06 min Scan# 1902
 Delta R.T. -0.00 min
 Lab File: BG027733.D
 Acq: 29 Jun 2017 9:17

Tgt Ion: 164 Resp: 90978
 Ion Ratio Lower Upper
 164 100
 162 106.0 85.1 127.7
 160 50.0 34.7 52.1



Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC




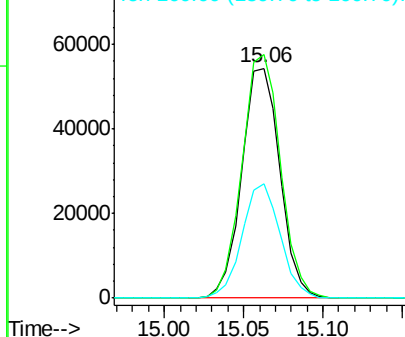


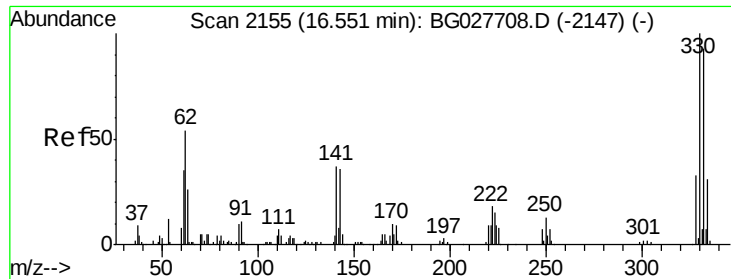

#41
 2,4,6-Tribromophenol
 Concen: 183.056 ng
 RT: 16.55 min Scan# 2155
 Delta R.T. -0.00 min
 Lab File: BG027733.D
 Acq: 29 Jun 2017 9:17




Instrument :
 BNA_G
 ClientSampleId :
 SP1-B-COMP


Tgt Ion:330 Resp: 228429
 Ion Ratio Lower Upper
 330 100
 332 95.4 77.3 115.9
 141 37.1 32.1 48.1

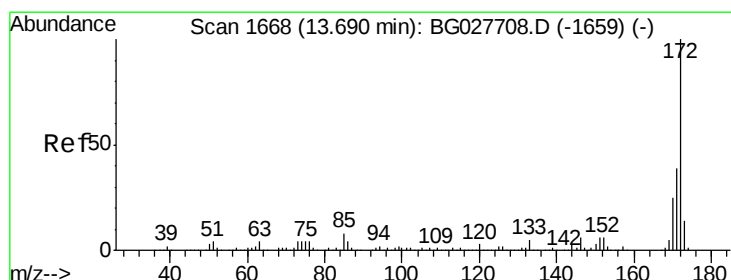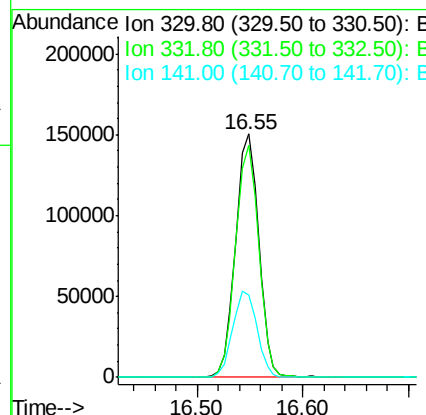

#44
 2-Fluorobiphenyl
 Concen: 105.761 ng
 RT: 13.69 min Scan# 1668
 Delta R.T. -0.00 min
 Lab File: BG027733.D
 Acq: 29 Jun 2017 9:17

Tgt Ion:172 Resp: 673727
 Ion Ratio Lower Upper
 172 100
 171 37.7 32.2 48.2
 170 23.9 21.8 32.6

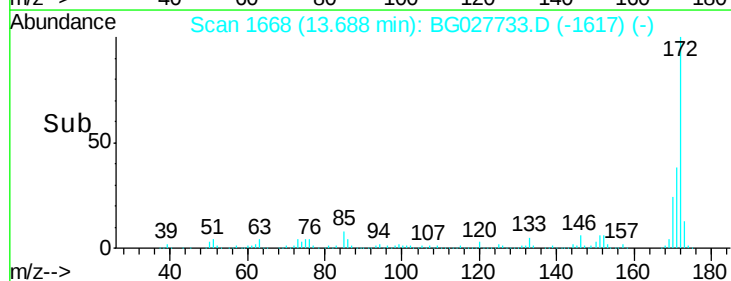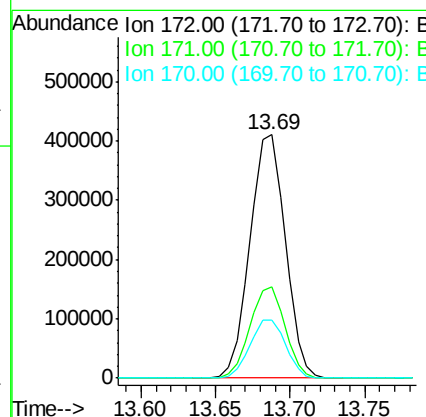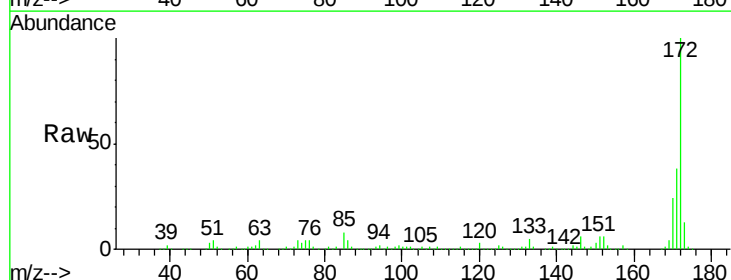


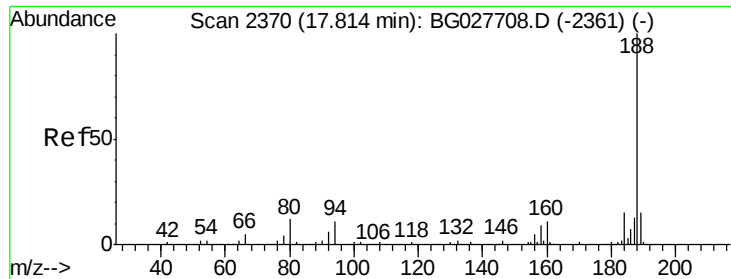




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.81 min Scan# 2369
Delta R.T. -0.01 min
Lab File: BG027733.D
Acq: 29 Jun 2017 9:17

Instrument :
BNA_G
ClientSampleId :
SP1-B-COMP

Tgt Ion:188 Resp: 246637
Ion Ratio Lower Upper
188 100
94 10.5 5.8 8.8#
80 12.9 7.5 11.3#

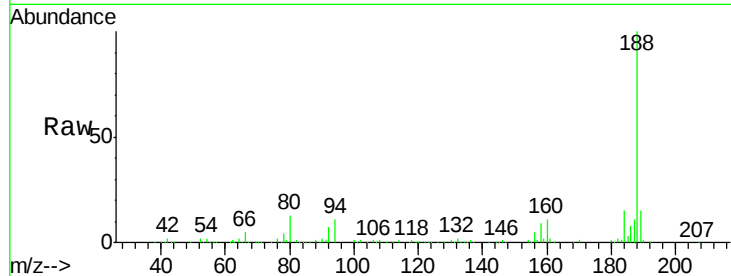


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

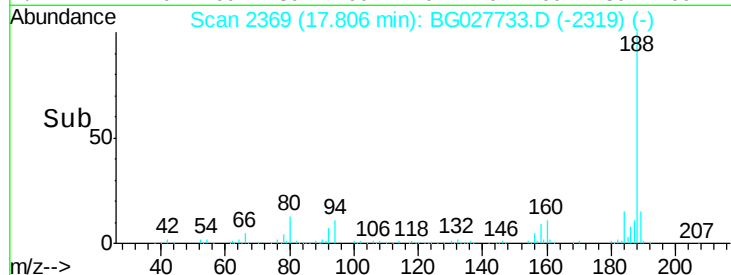
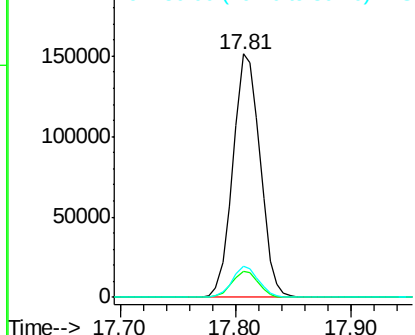


#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.17 min Scan# 3112
Delta R.T. -0.00 min
Lab File: BG027733.D
Acq: 29 Jun 2017 9:17

Tgt Ion:240 Resp: 264020
Ion Ratio Lower Upper
240 100
120 13.9 5.7 8.5#
236 26.6 22.2 33.4



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

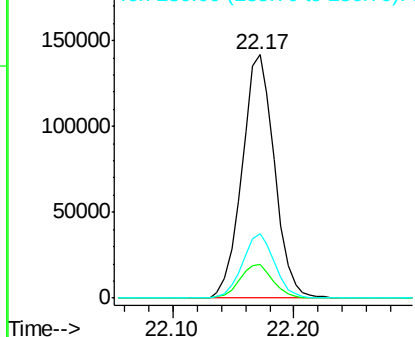



#78

Terphenyl-d14

Concen: 116.511 ng

RT: 20.39 min Scan# 2809

Delta R.T. 0.00 min

Lab File: BG027733.D

Acq: 29 Jun 2017 9:17

Instrument :

BNA_G

ClientSampleId :

SP1-B-COMP


Tgt Ion:244 Resp: 1312134

Ion Ratio Lower Upper

244 100

212 7.7 10.0 15.0#



122 12.4 8.6 12.8



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

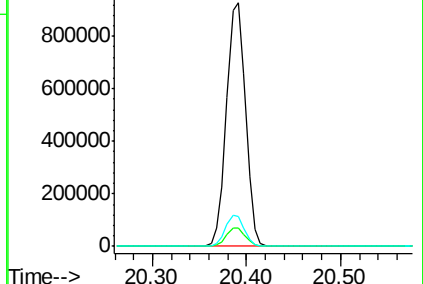

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.78 min Scan# 3726

Delta R.T. -0.01 min

Lab File: BG027733.D

Acq: 29 Jun 2017 9:17


Tgt Ion:264 Resp: 254676

Ion Ratio Lower Upper

264 100

260 23.5 21.8 32.8

265 22.4 18.2 27.4



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

