


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG062817\
 Data File : BG027722.D
 Acq On : 29 Jun 2017 2:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 19:26:37 2017

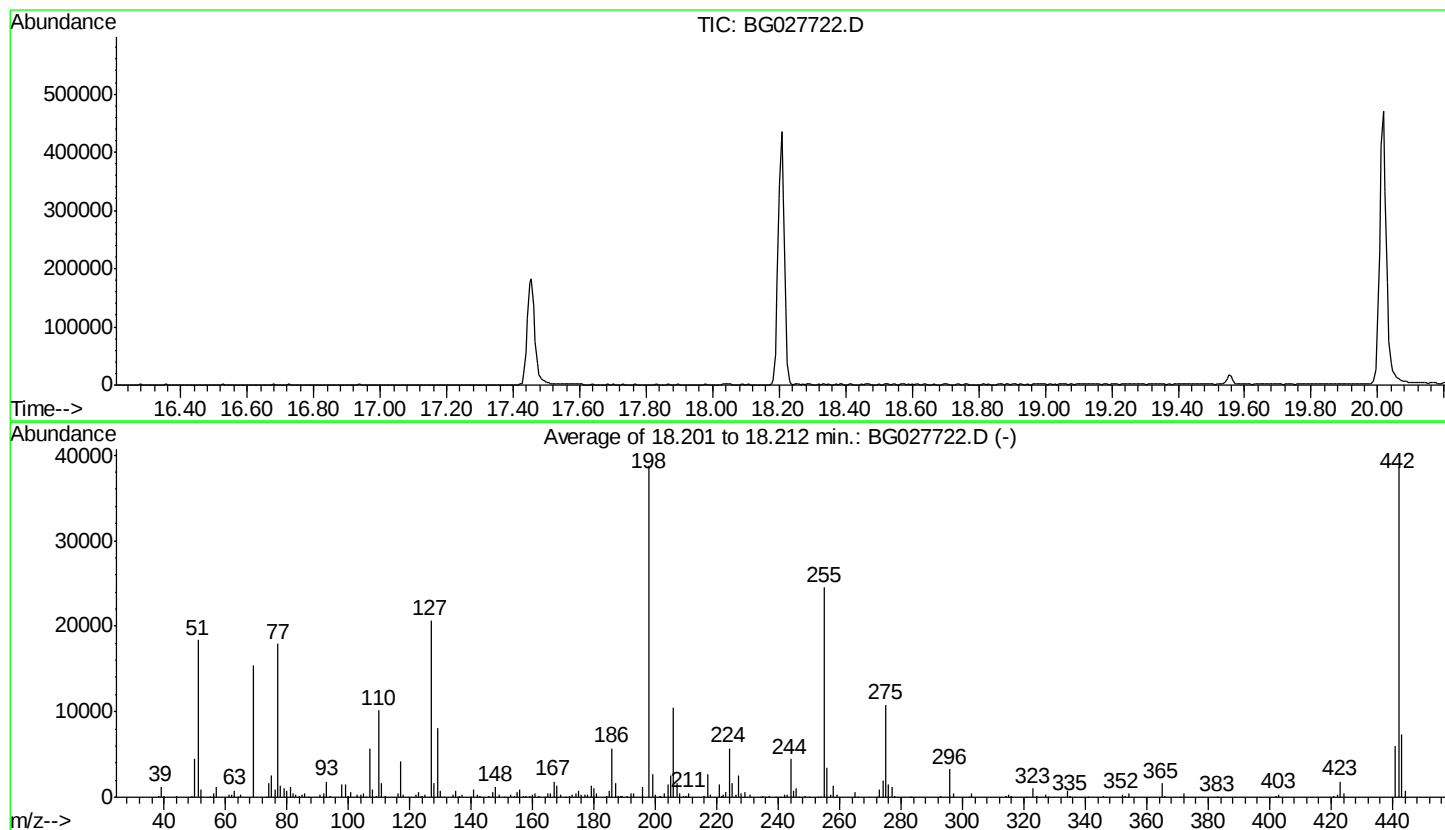

AutoFind: Scans 2436, 2437, 2438; Background Corrected with Scan 2429

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	18363	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.9	15488	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.2	20630	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38770	PASS
199	198	5	9	7.1	2750	PASS
275	198	10	60	27.9	10804	PASS
365	198	1	100	4.2	1620	PASS
441	442	0.01	24	15.4	5964	PASS
442	198	50	100	99.8	38688	PASS
443	442	15	24	19.1	7400	PASS