
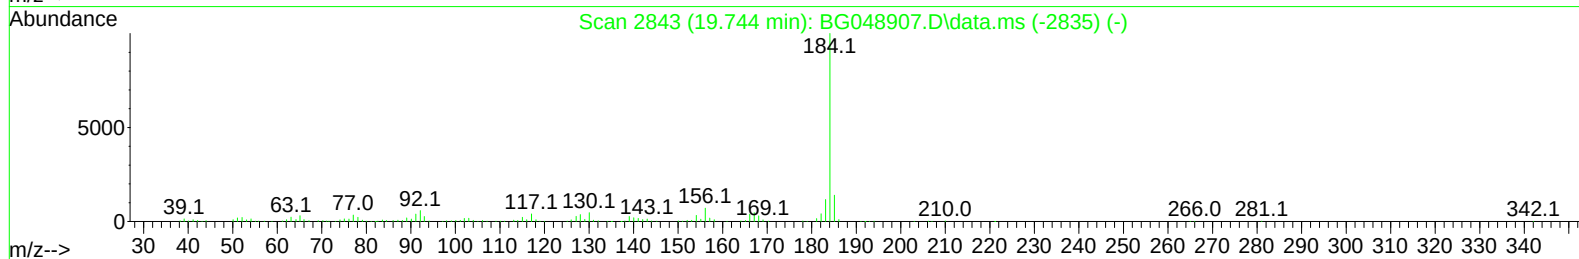
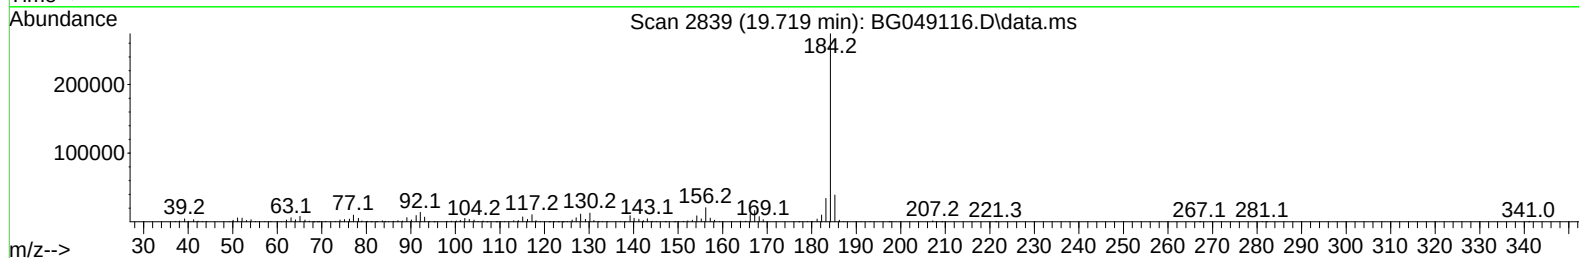


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062821\
Data File : BG049116.D
Acq On : 28 Jun 2021 11:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 12:56:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

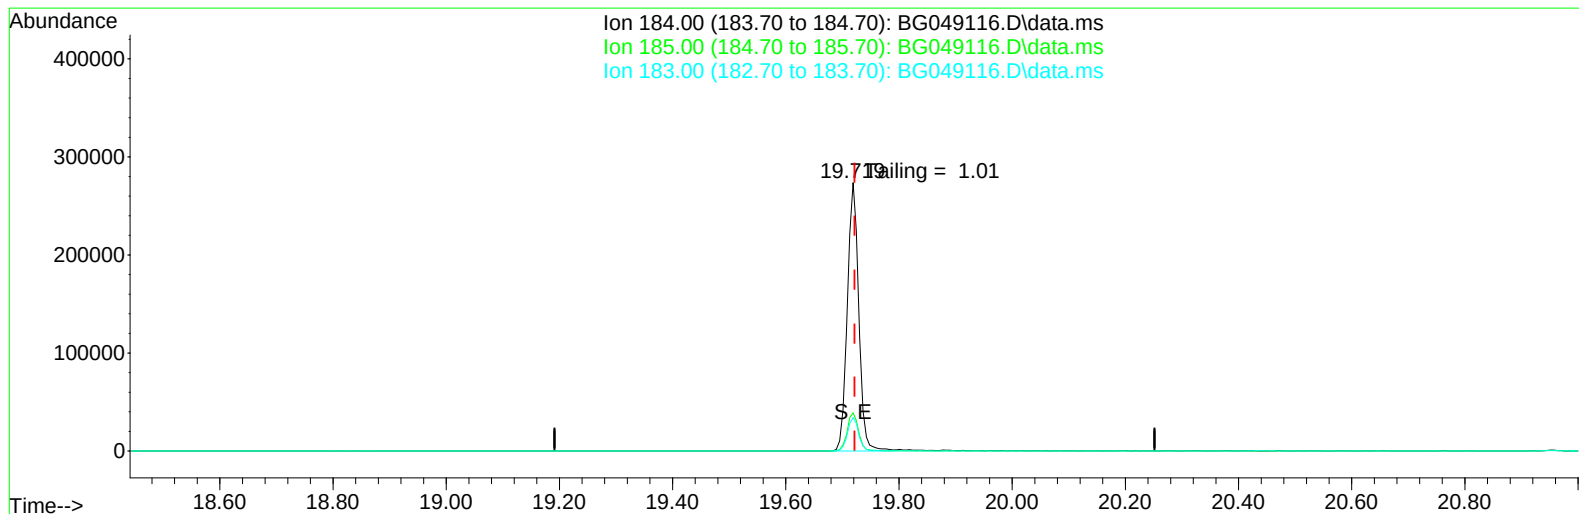




TIC: BG049116.D\data.ms

(77) Benzidine**19.719min (-0.002) 307665.33 ng****response 384270**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.27
183.00	11.70	12.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062821\
Data File : BG049116.D
Acq On : 28 Jun 2021 11:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 12:56:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

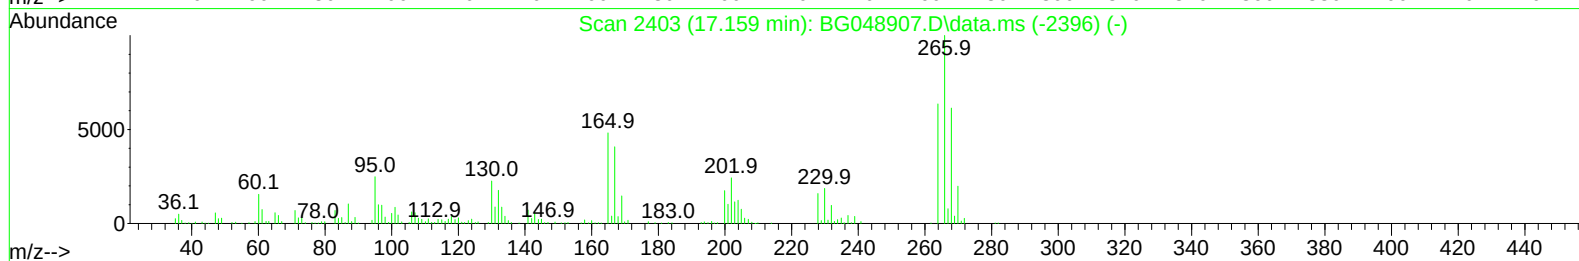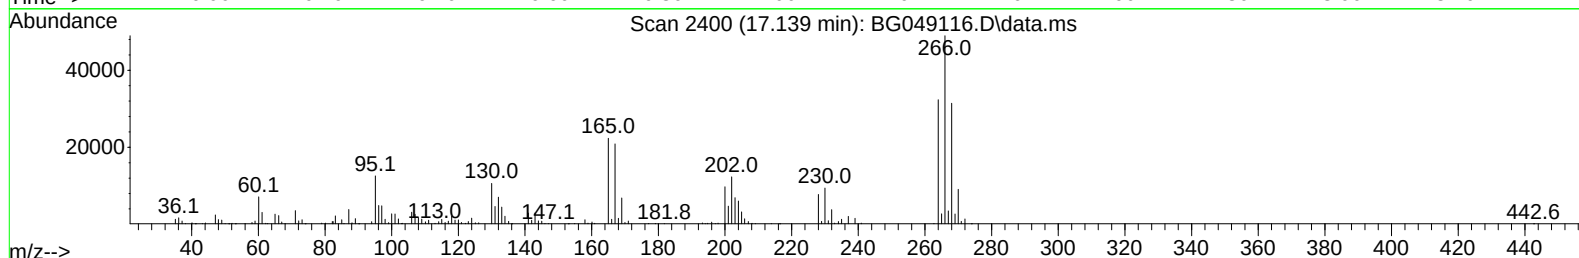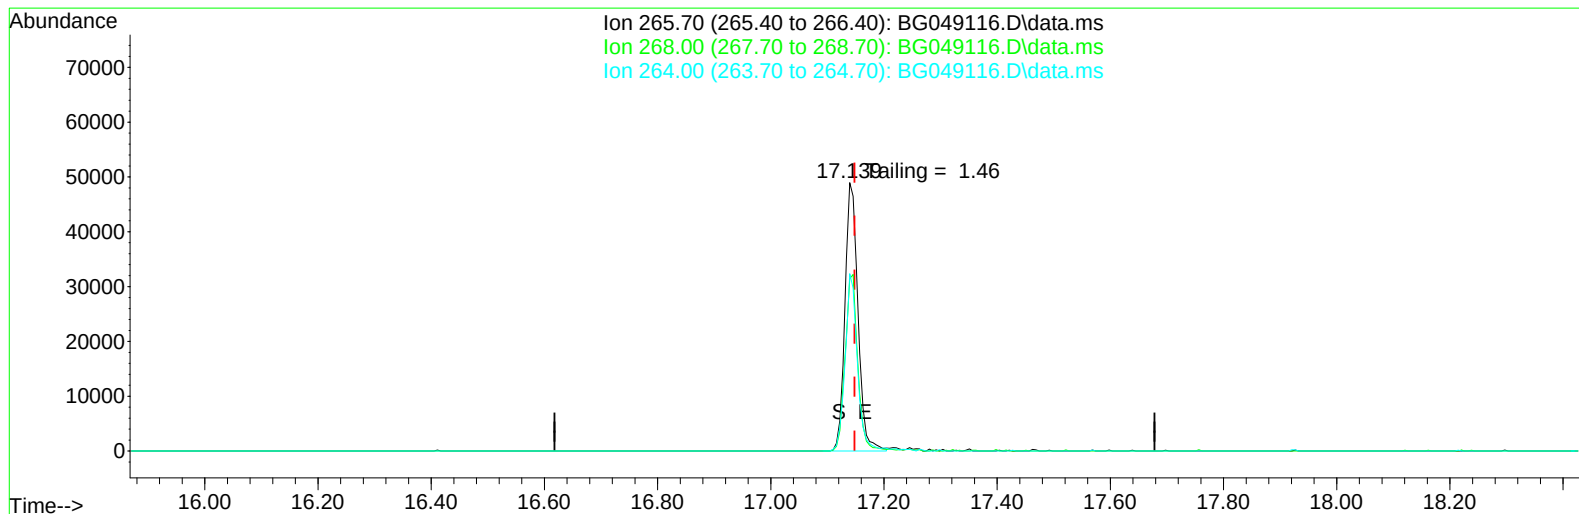

TIC: BG049116.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.008) 0.00 ng

response 78393

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.24
264.00	61.30	66.03
0.00	0.00	0.00