
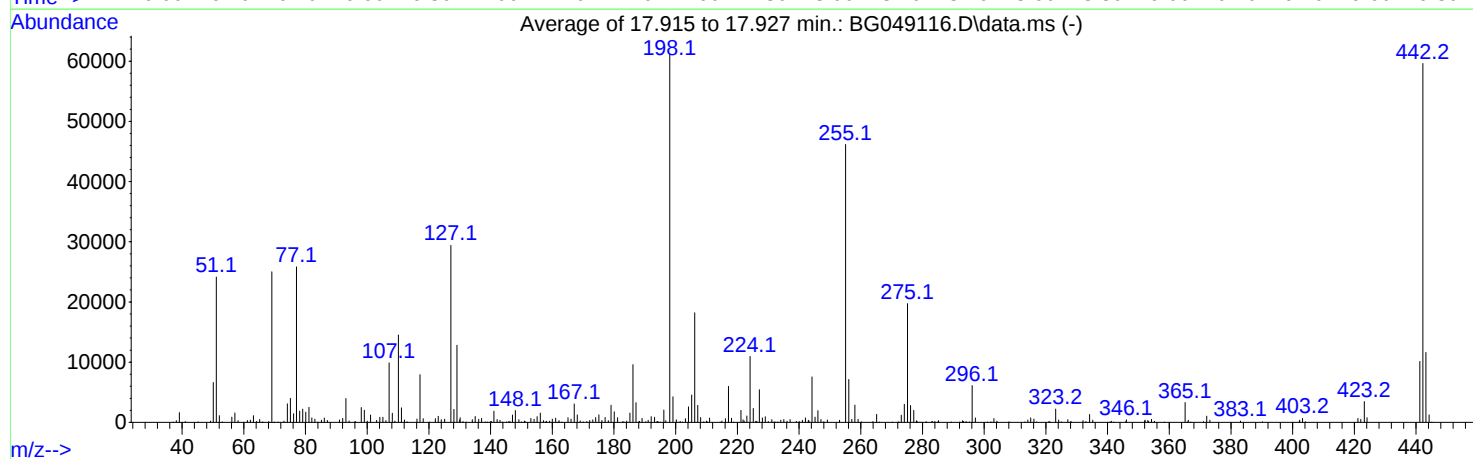


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062821\
 Data File : BG049116.D
 Acq On : 28 Jun 2021 11:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 24 11:02:36 2021

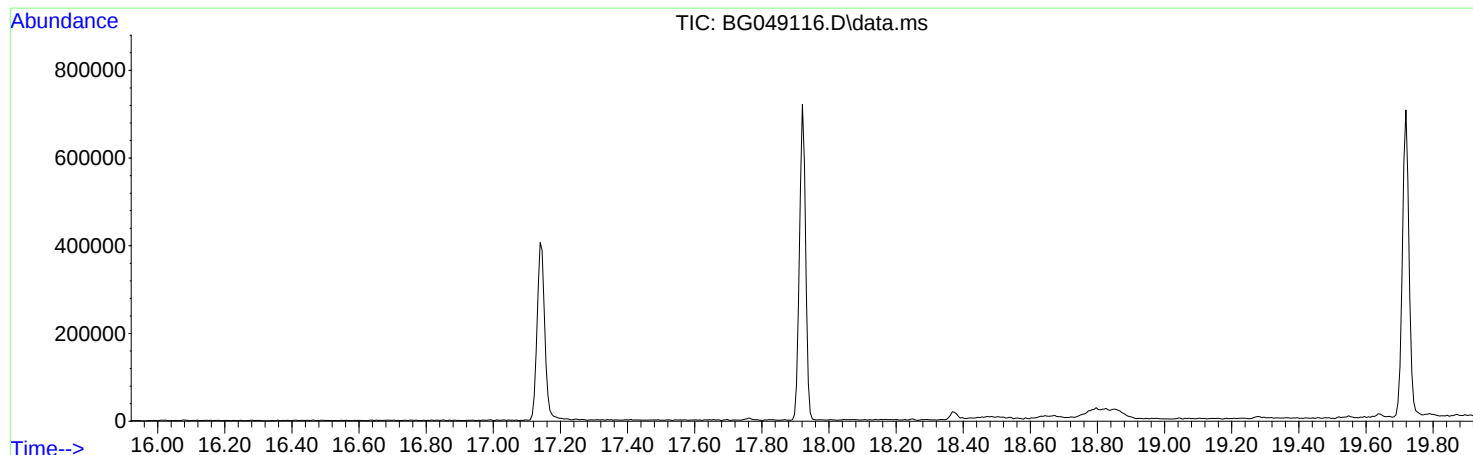




AutoFind: Scans 2532, 2533, 2534; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	24125	PASS
68	69	0.00	2	0.5	126	PASS
69	198	0.00	100	40.9	25008	PASS
70	69	0.00	2	0.3	67	PASS
127	198	10	80	48.1	29403	PASS
197	198	0.00	2	0.4	261	PASS
198	198	100	100	100.0	61109	PASS
199	198	5	9	7.0	4260	PASS
275	198	10	60	32.3	19725	PASS
365	198	1	100	5.4	3291	PASS
441	198	0.01	100	16.6	10133	PASS
442	442	100	100	100.0	59621	PASS
443	442	15	24	19.5	11620	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062821\
 Data File : BG049116.D
 Acq On : 28 Jun 2021 11:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 28 12:56:30 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 24 11:02:36 2021
 Response via : Initial Calibration

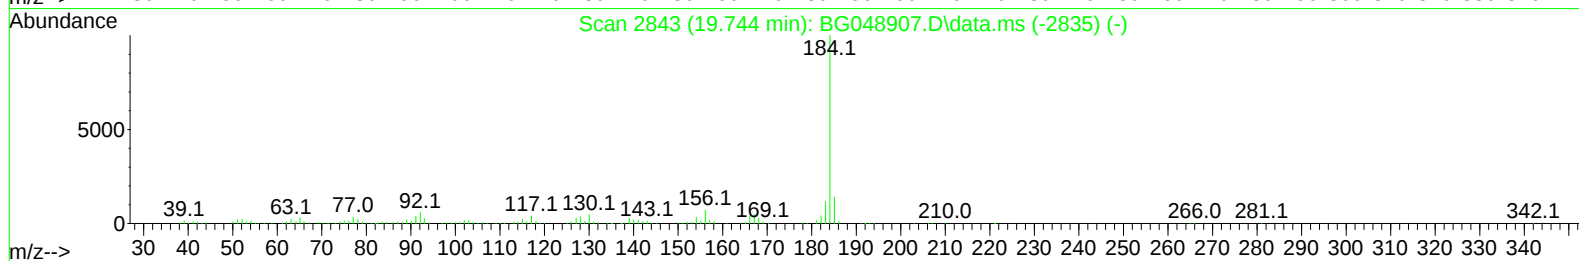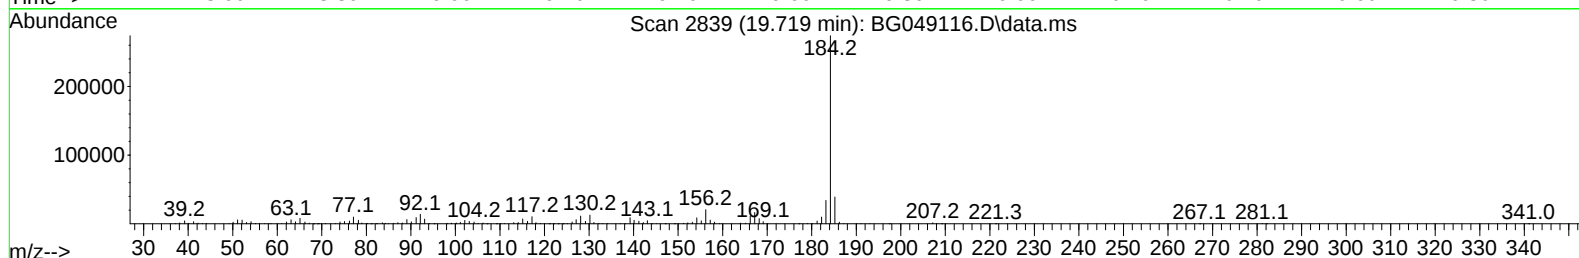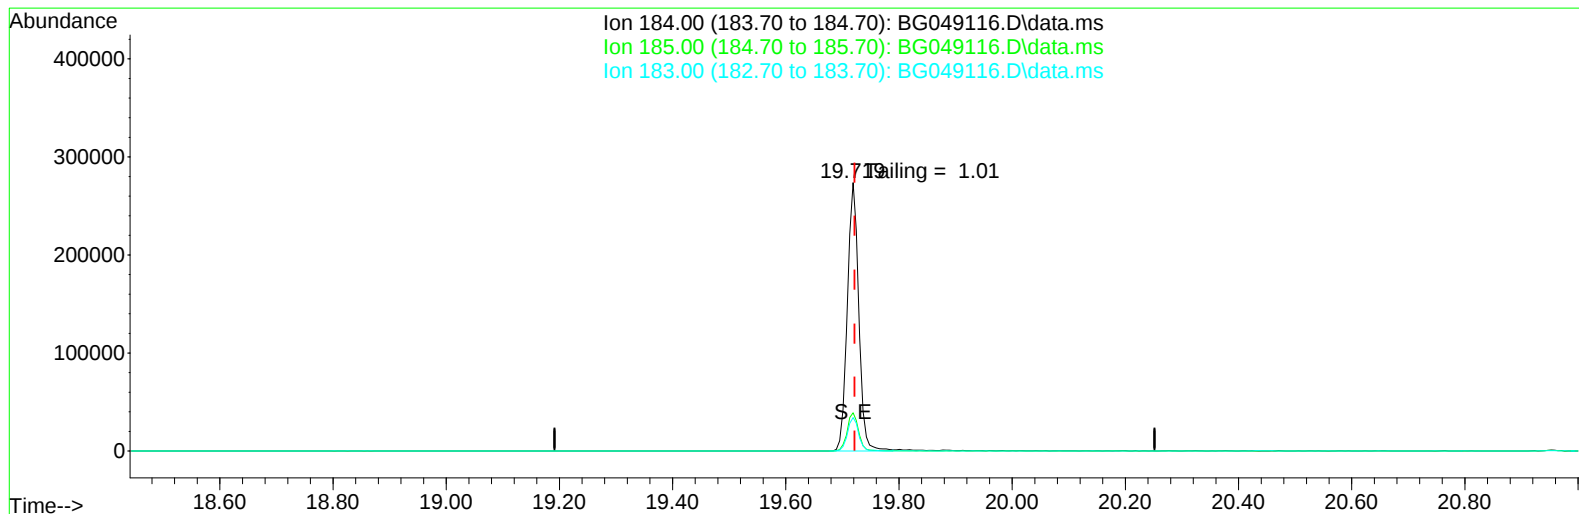

TIC: BG049116.D\data.ms

(77) Benzidine

19.719min (-0.002) 307665.33 ng




response 384270

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.27
183.00	11.70	12.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062821\
Data File : BG049116.D
Acq On : 28 Jun 2021 11:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 12:56:30 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

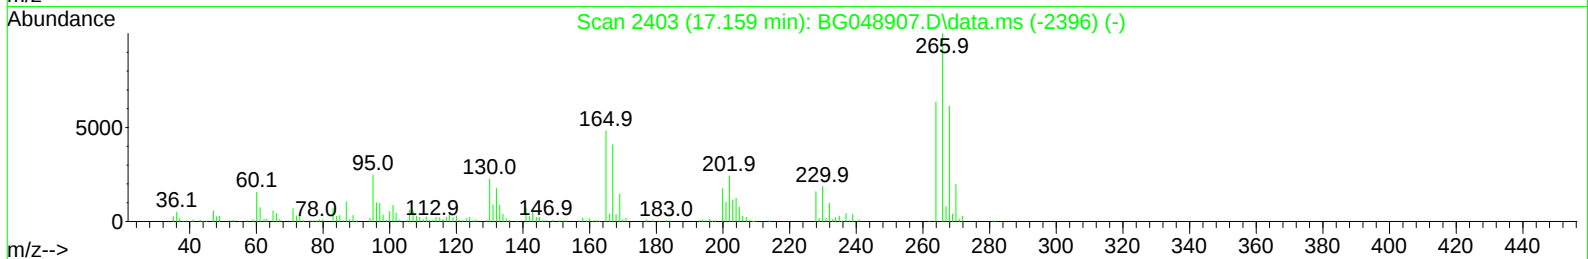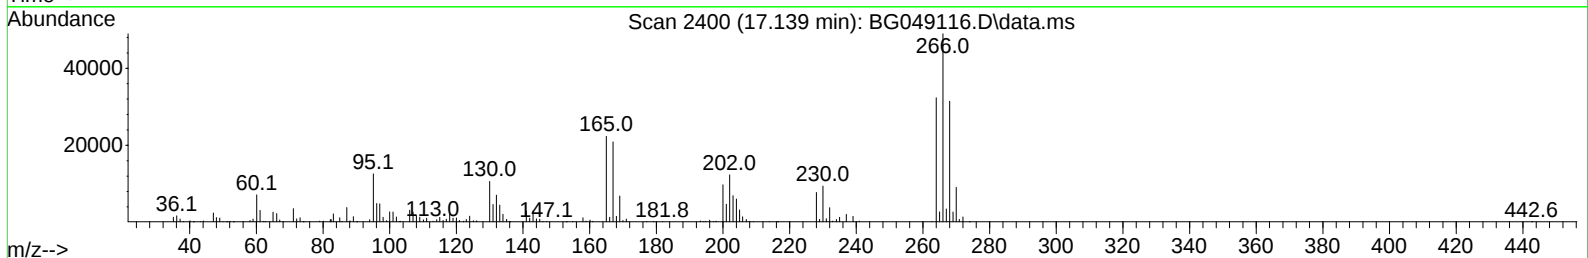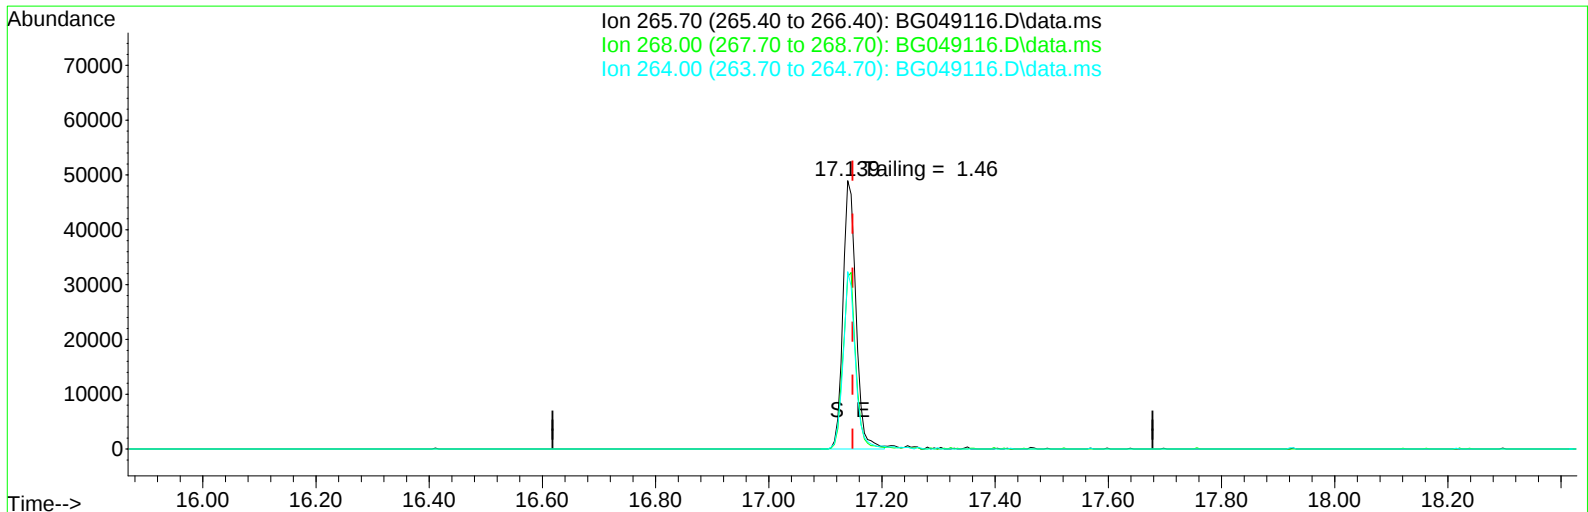

TIC: BG049116.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.008) 0.00 ng

response 78393

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.24
264.00	61.30	66.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
28/6/2021	BNA_G	BG049116.D
Compound Name	Response	Retention Time
DDT	211607	20.95
DDD	826	20.5
DDE	153	20
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
979	212586	0.46

Instrument :
BNA_G
ClientSampleId :
DFTPP