
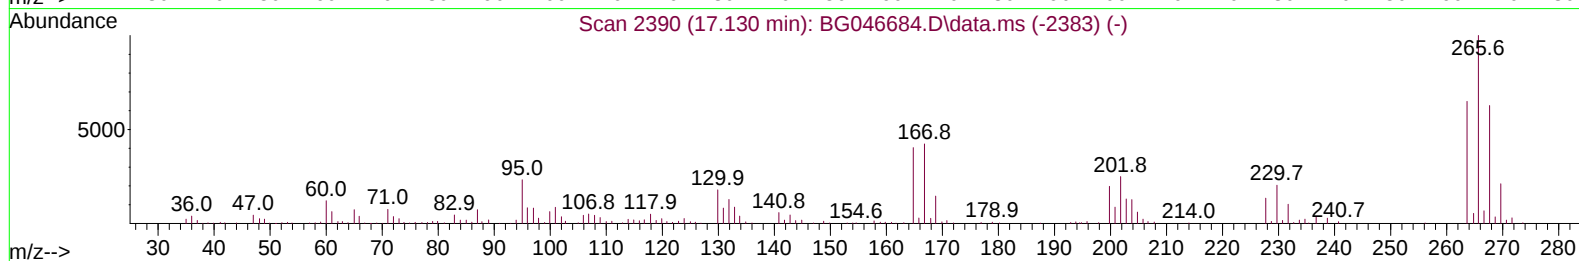
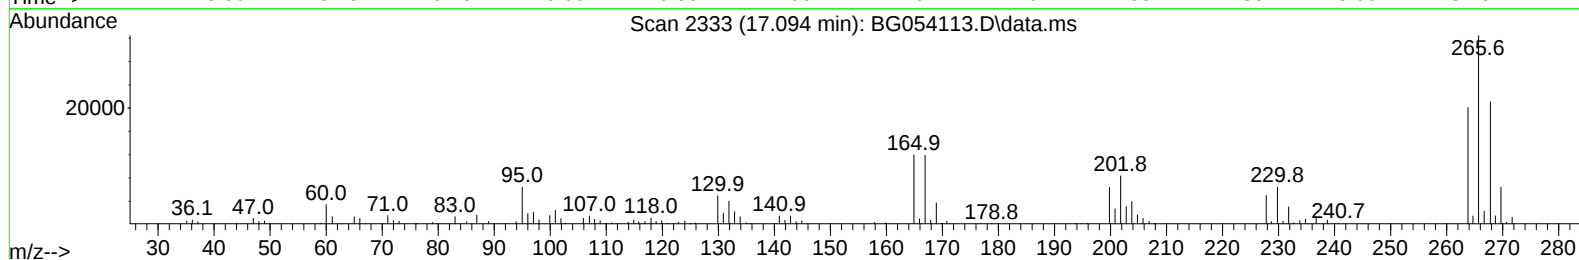


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062822\
Data File : BG054113.D
Acq On : 28 Jun 2022 9:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 15:07:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 17:56:56 2021
Response via : Initial Calibration

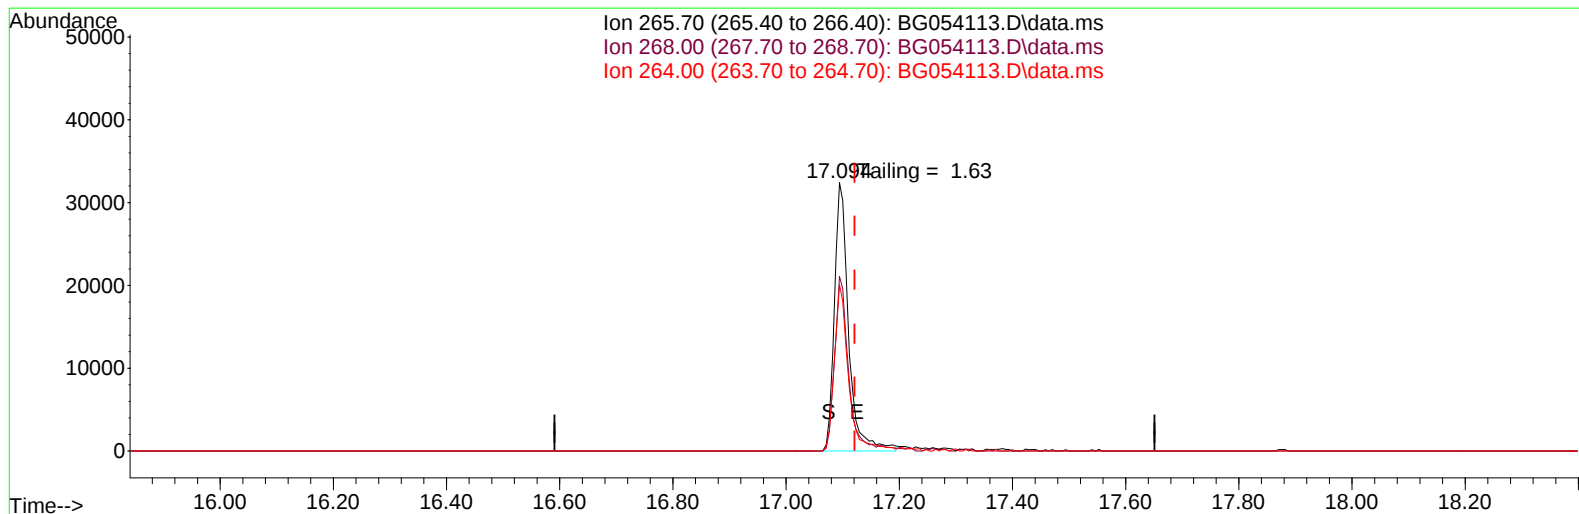

TIC: BG054113.D\data.ms

(70) Pentachlorophenol (C)




17.094min (-0.026) 30202.90 ng

response 57360

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.68
264.00	61.60	66.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062822\
Data File : BG054113.D
Acq On : 28 Jun 2022 9:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 15:07:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 17:56:56 2021
Response via : Initial Calibration

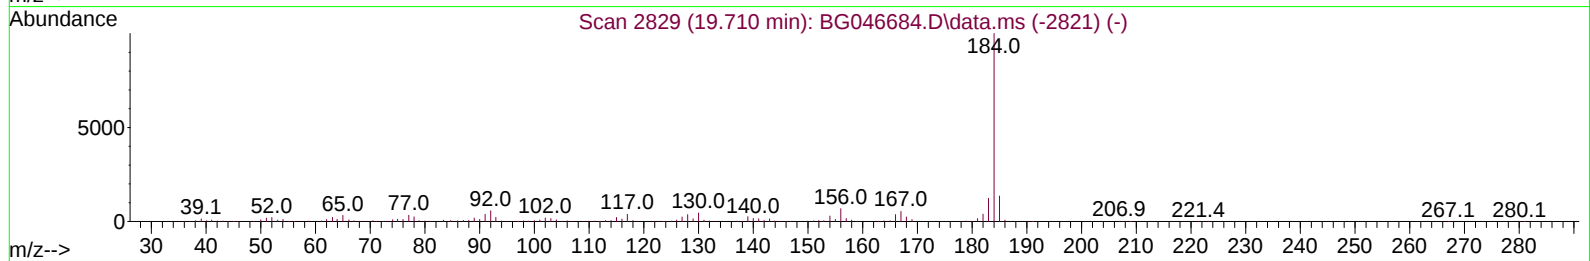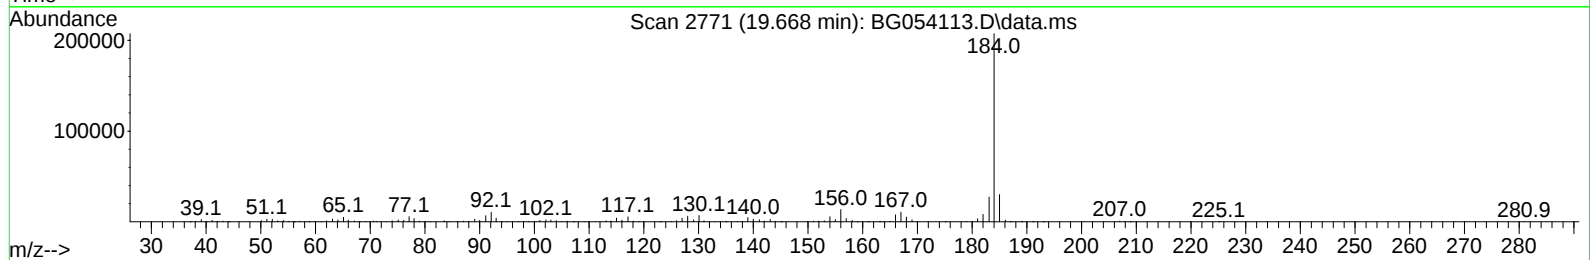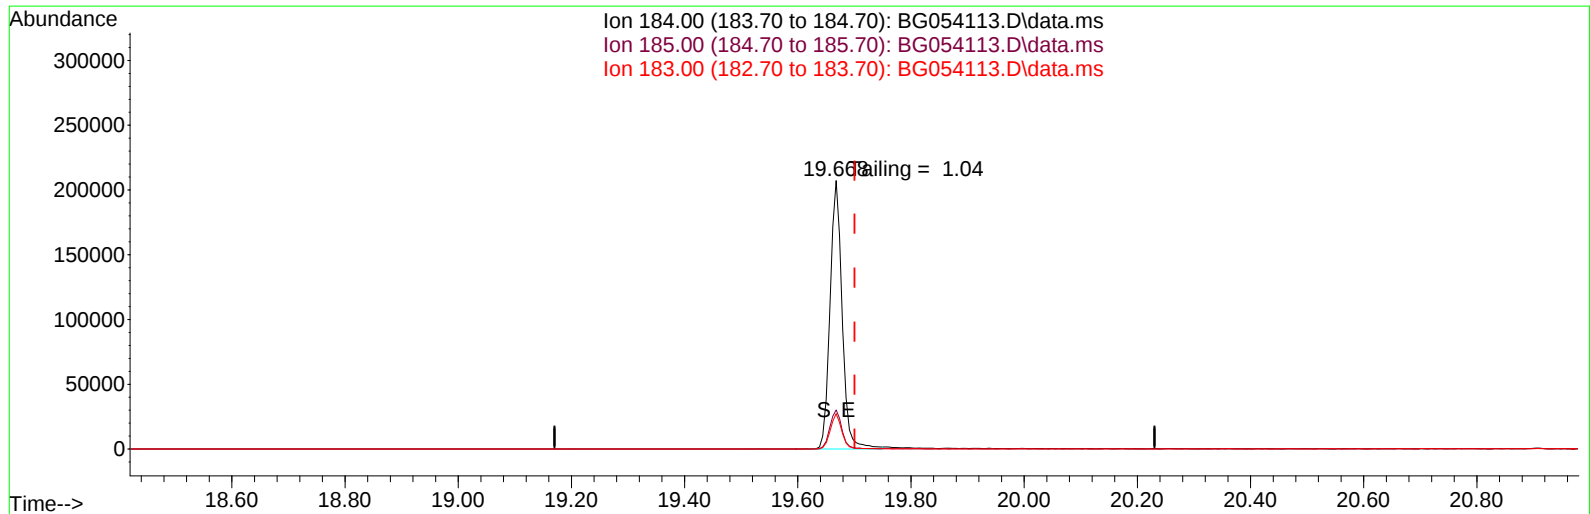

TIC: BG054113.D\data.ms

(77) Benzidine

19.668min (-0.032) 175191.75 ng m

response 307820

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.54
183.00	13.20	13.16
0.00	0.00	0.00