
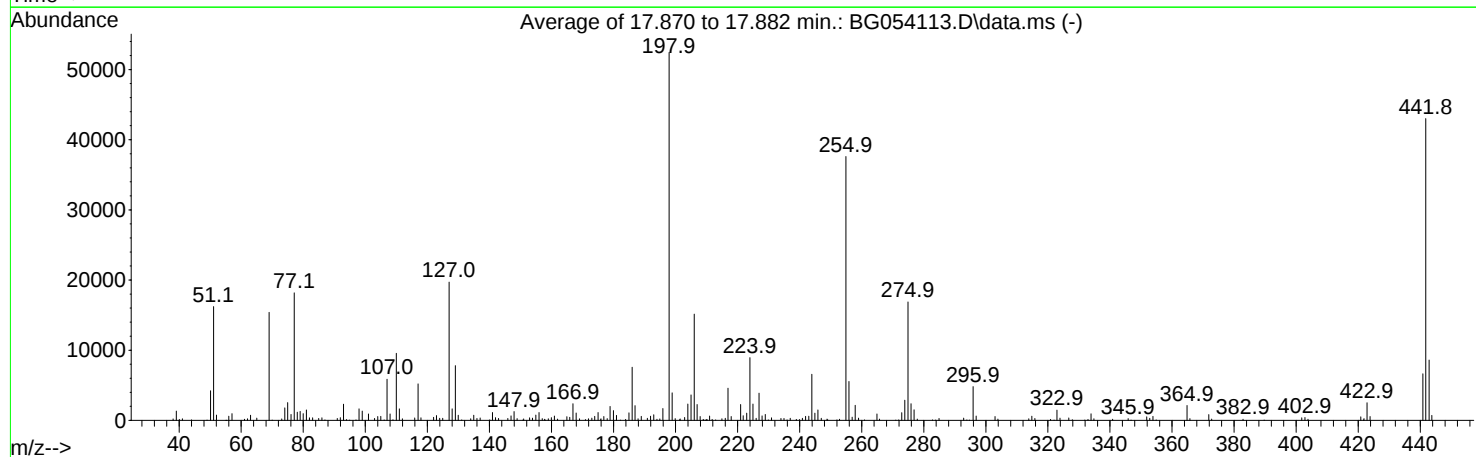


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062822\
 Data File : BG054113.D
 Acq On : 28 Jun 2022 9:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 00:27:54 2022

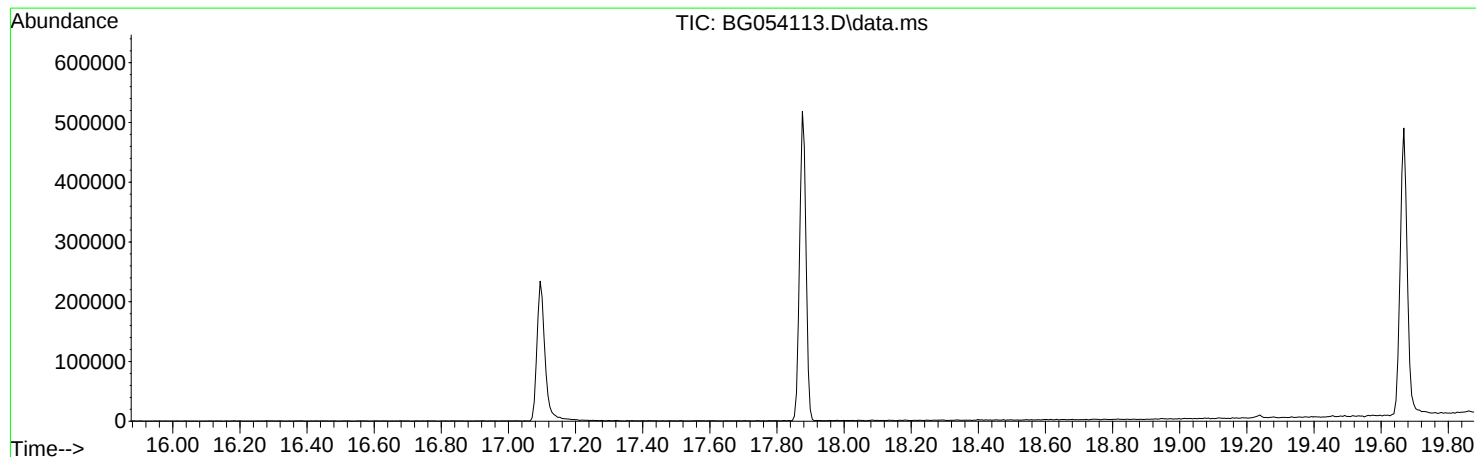




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	16212	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.4	15396	PASS
70	69	0.00	2	0.4	54	PASS
127	198	10	80	37.6	19717	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52435	PASS
199	198	5	9	7.5	3927	PASS
275	198	10	60	32.2	16882	PASS
365	198	1	100	4.1	2124	PASS
441	198	0.01	100	12.7	6639	PASS
442	442	50	100	100.0	43016	PASS
443	442	15	24	20.0	8603	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062822\
 Data File : BG054113.D
 Acq On : 28 Jun 2022 9:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 28 15:07:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 20 17:56:56 2021
 Response via : Initial Calibration

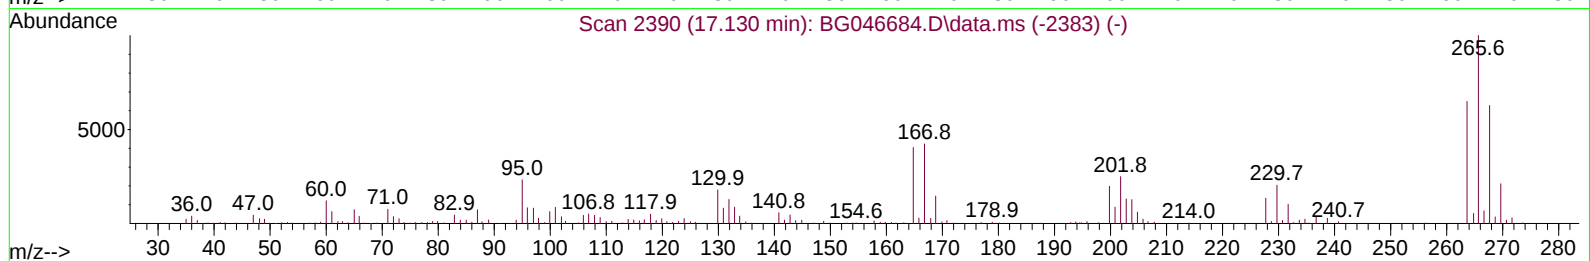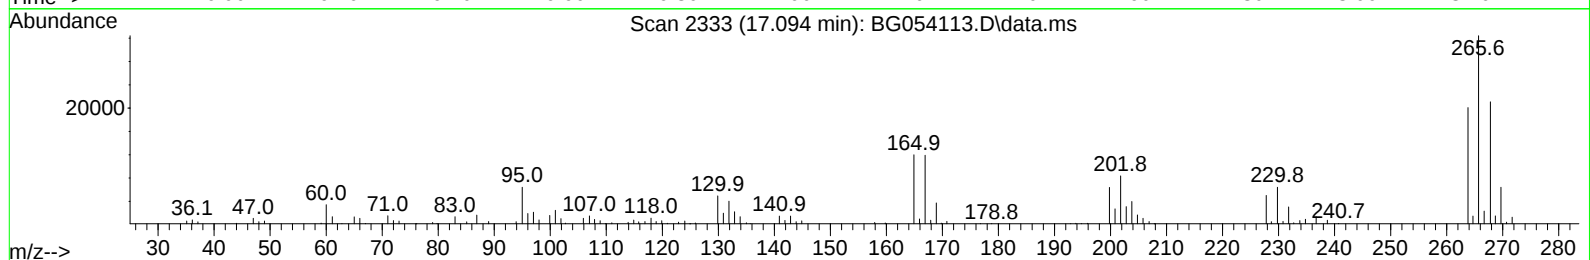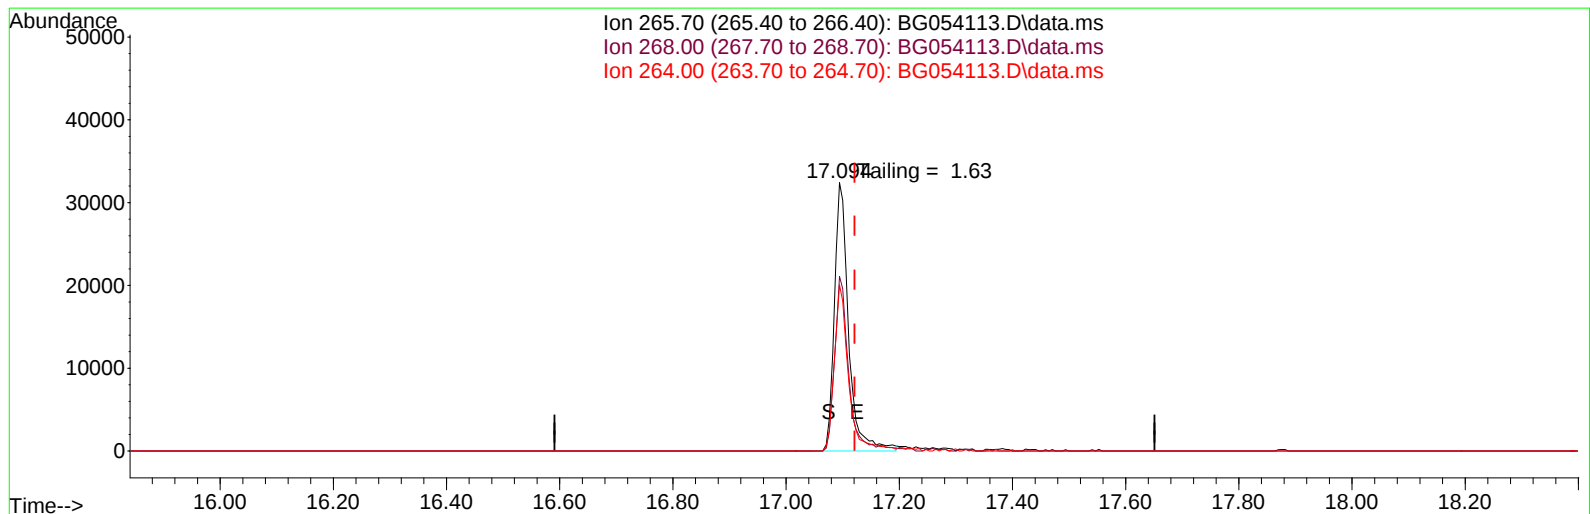

TIC: BG054113.D\data.ms

(70) Pentachlorophenol (C)

17.094min (-0.026) 30202.90 ng




response 57360

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.68
264.00	61.60	66.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062822\
Data File : BG054113.D
Acq On : 28 Jun 2022 9:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 15:07:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 17:56:56 2021
Response via : Initial Calibration

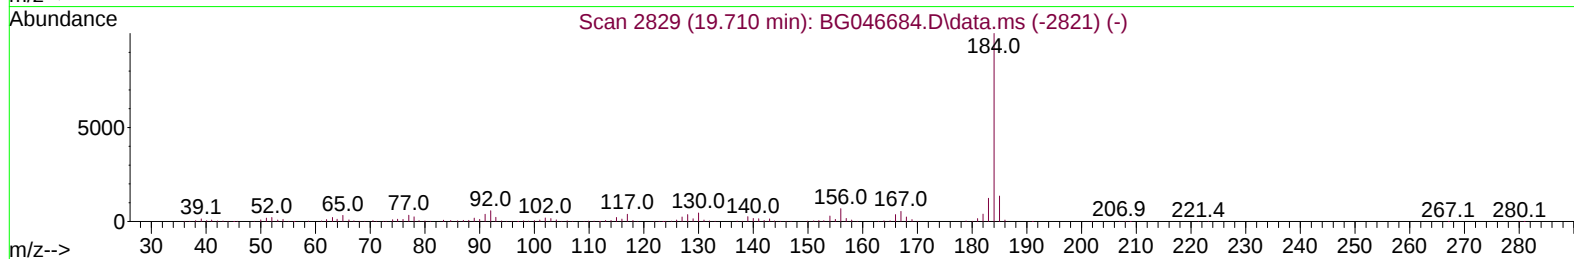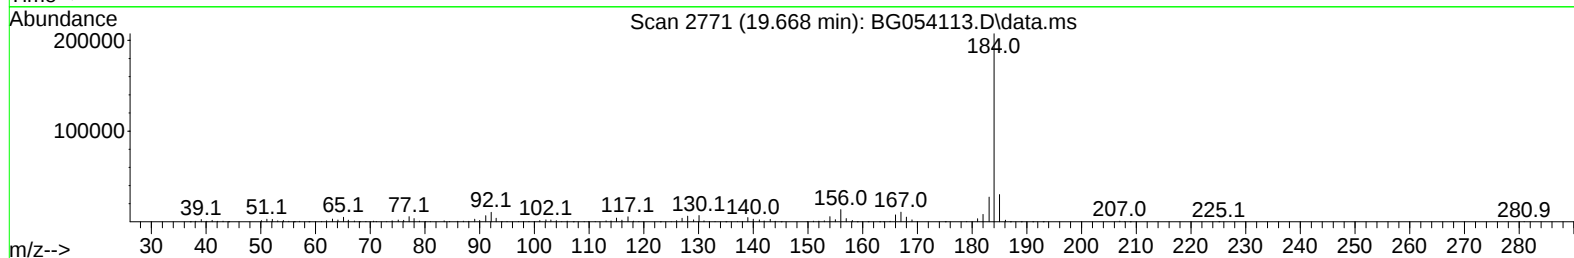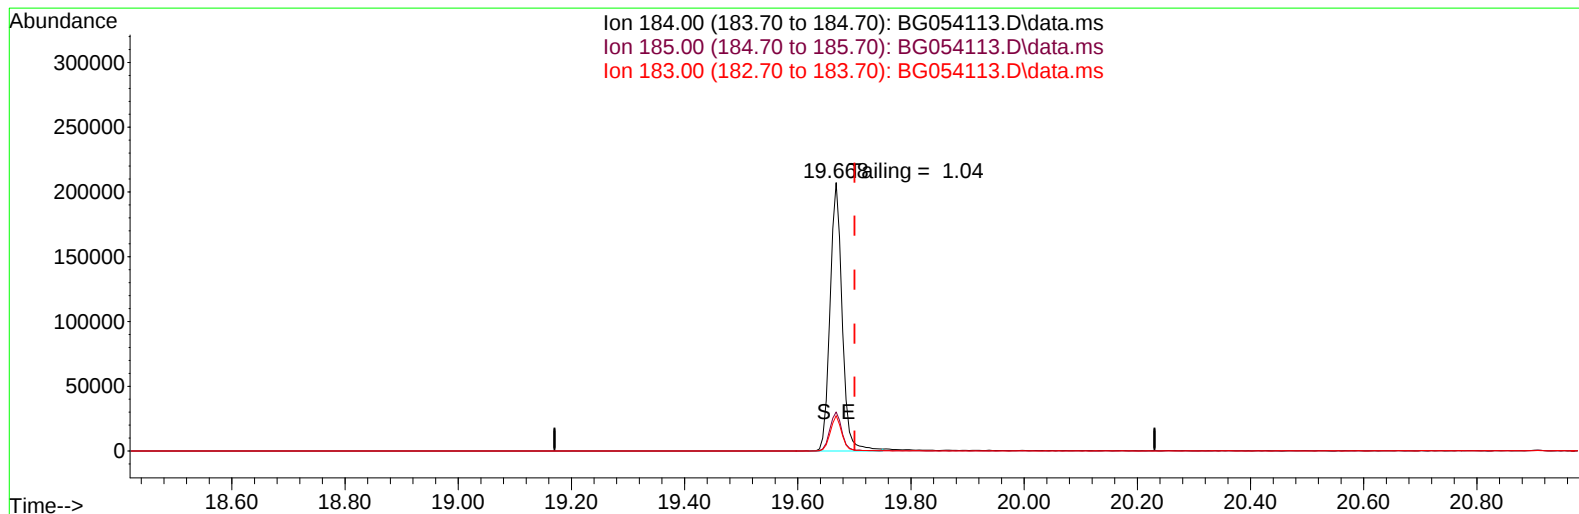

TIC: BG054113.D\data.ms

(77) Benzidine

19.668min (-0.032) 175191.75 ng m

response 307820

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.54
183.00	13.20	13.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/28/2022	BNA_G	<u>BG054113.D</u>
Compound Name	Response	Retention Time
DDT	164832	20.9
DDD	4031	20.46
DDE	860	19.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4891	169723	2.88

Instrument :
BNA_G
ClientSampleId :
DFTPP