
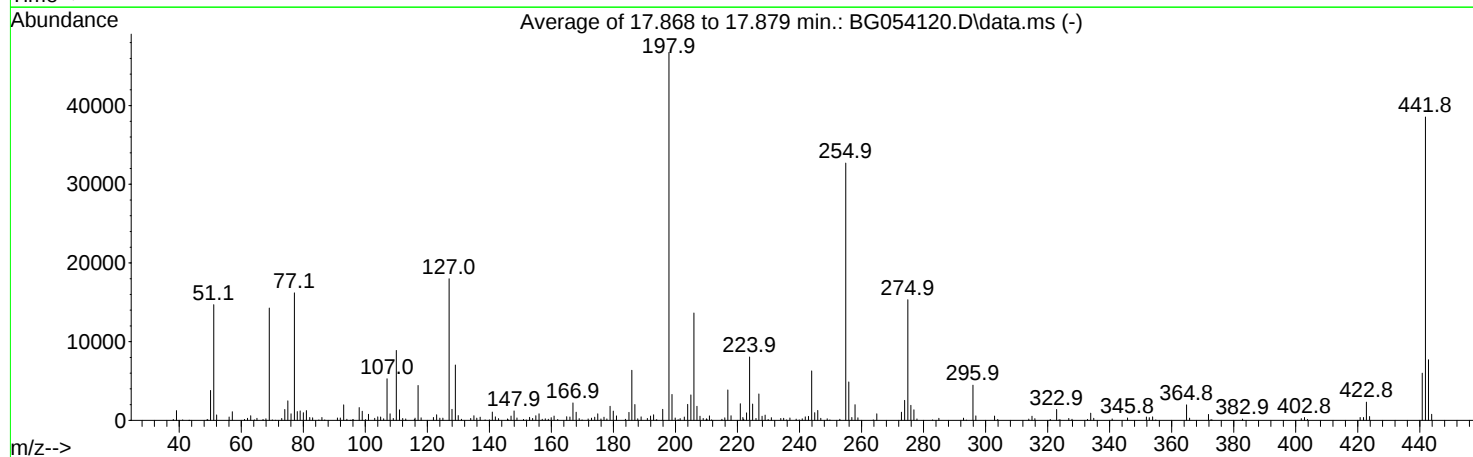


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062822\
 Data File : BG054120.D
 Acq On : 28 Jun 2022 16:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jun 27 00:27:54 2022

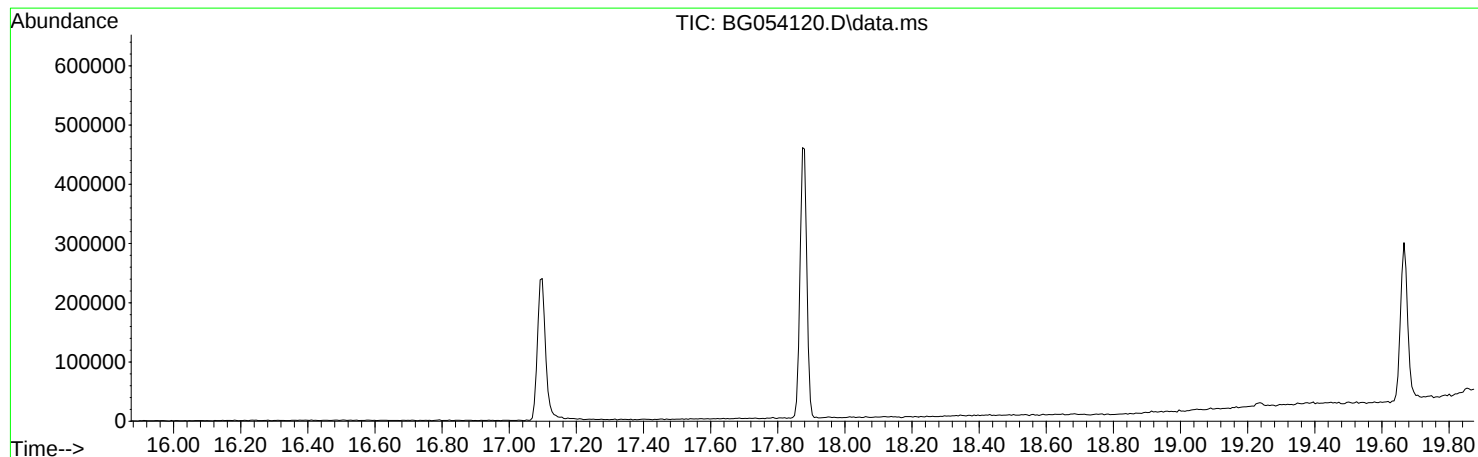




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	14692	PASS
68	69	0.00	2	1.4	199	PASS
69	198	0.00	100	30.5	14273	PASS
70	69	0.00	2	0.5	70	PASS
127	198	10	80	38.5	17984	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46744	PASS
199	198	5	9	7.0	3293	PASS
275	198	10	60	32.8	15324	PASS
365	198	1	100	4.2	1977	PASS
441	198	0.01	100	12.8	6005	PASS
442	442	50	100	100.0	38547	PASS
443	442	15	24	20.0	7713	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062822\
Data File : BG054120.D
Acq On : 28 Jun 2022 16:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 16:44:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

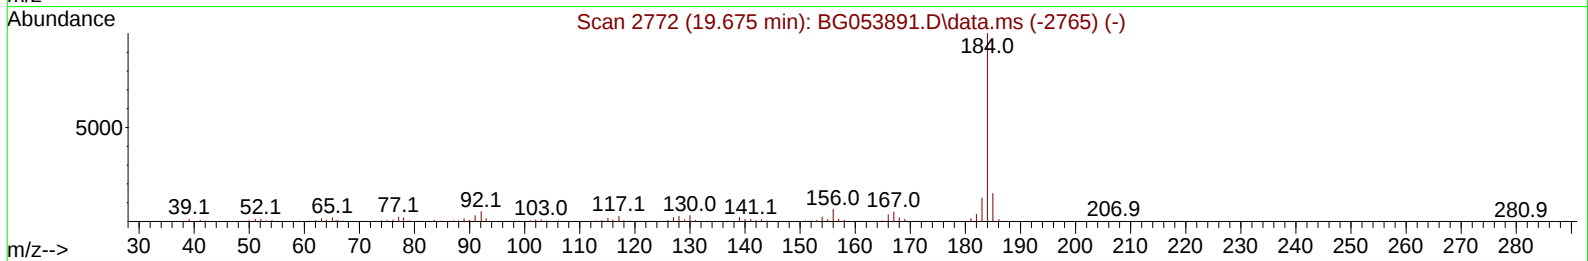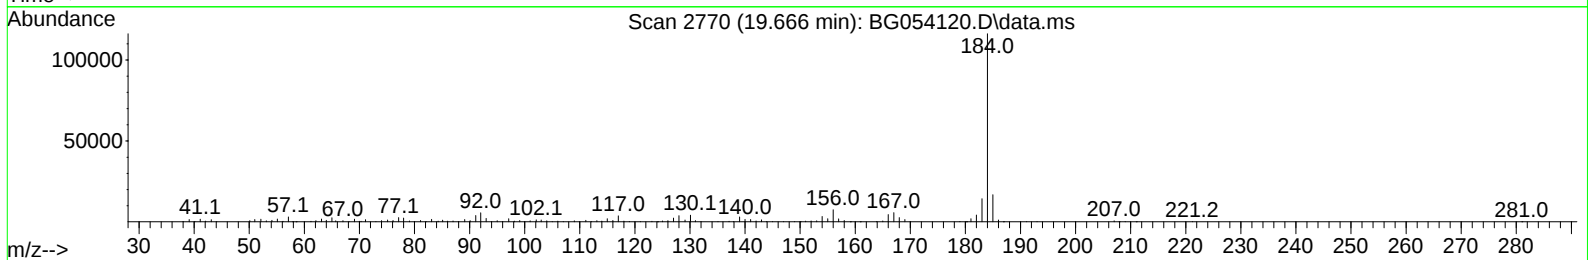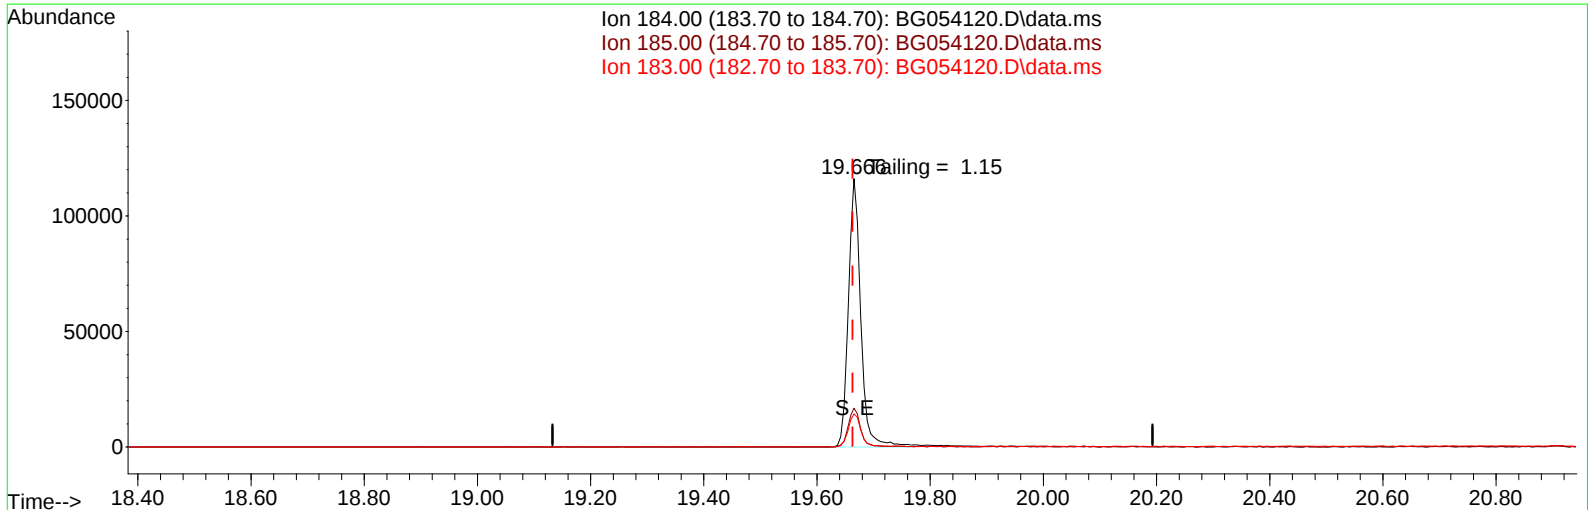

TIC: BG054120.D\data.ms

(77) Benzidine

19.666min (+ 0.003) 140548.41 ng




response 177547

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.52
183.00	11.10	12.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062822\
Data File : BG054120.D
Acq On : 28 Jun 2022 16:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jun 28 16:44:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

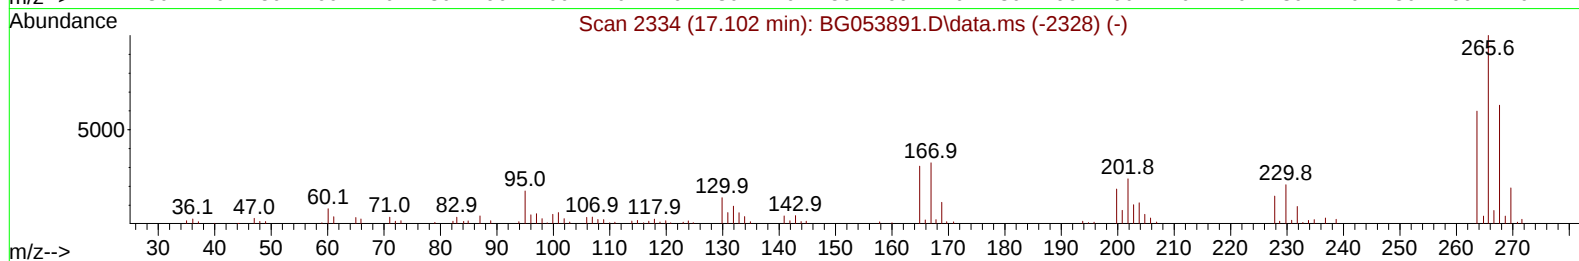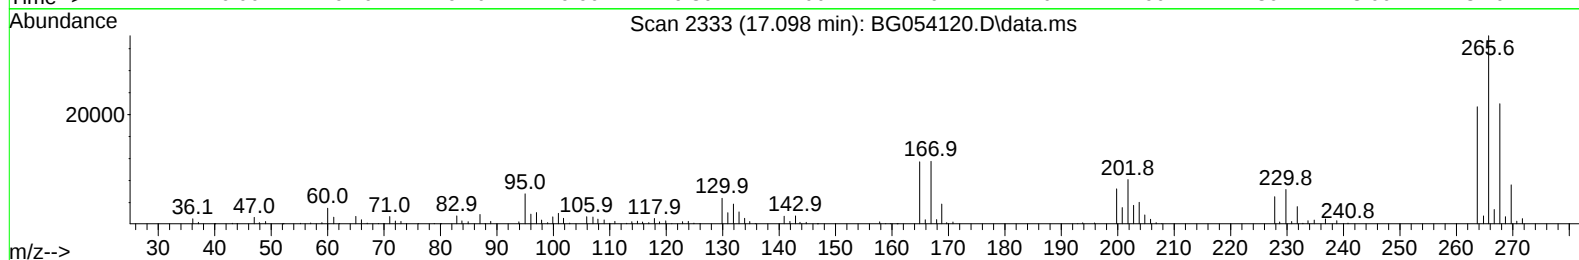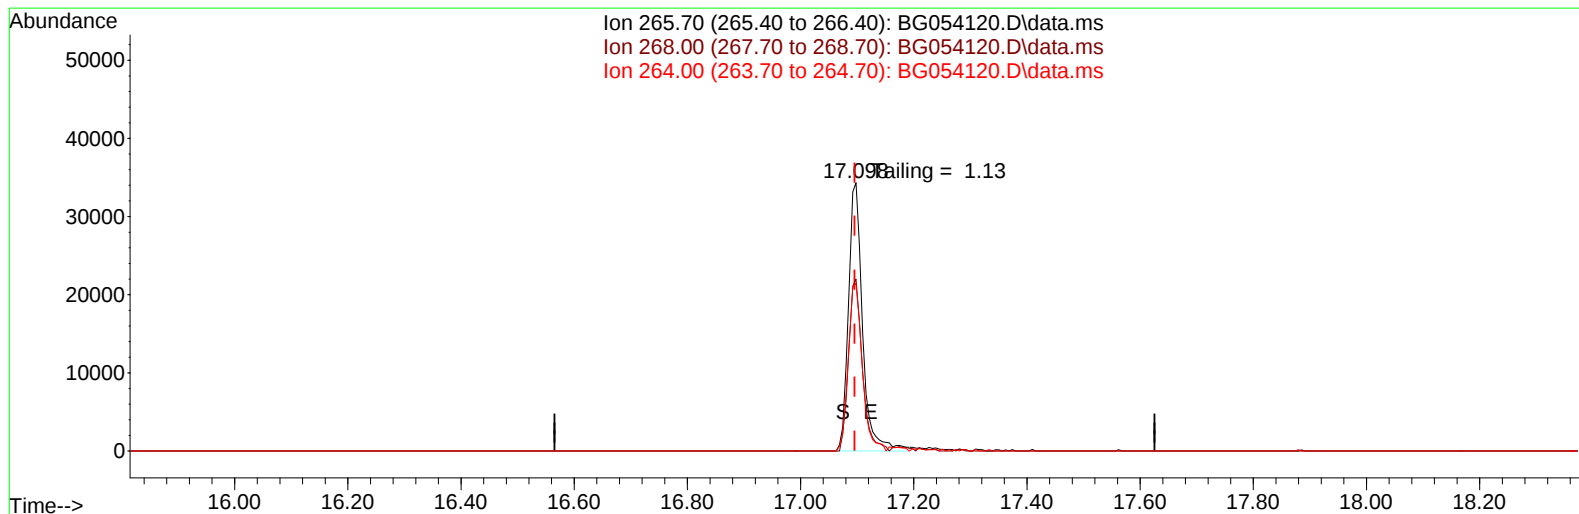

TIC: BG054120.D\data.ms

(70) Pentachlorophenol (C)

17.098min (+ 0.003) 42335.01 ng

response 59000

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	68.17
264.00	66.20	62.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/28/2022	BNA_G	BG054120.D
Compound Name	Response	Retention Time
DDT	155965	20.905
DDD	6347	20.465
DDE	1278	19.953
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7625	163590	4.66

Instrument :
BNA_G
ClientSampleId :
DFTPP