
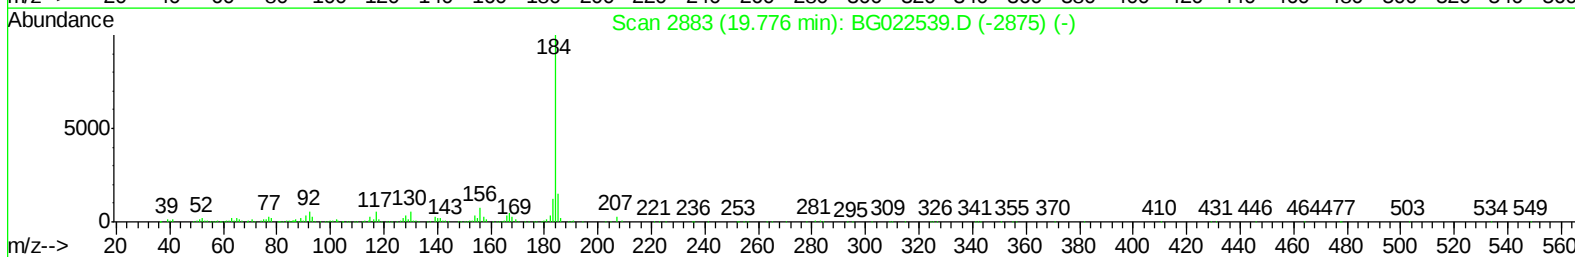
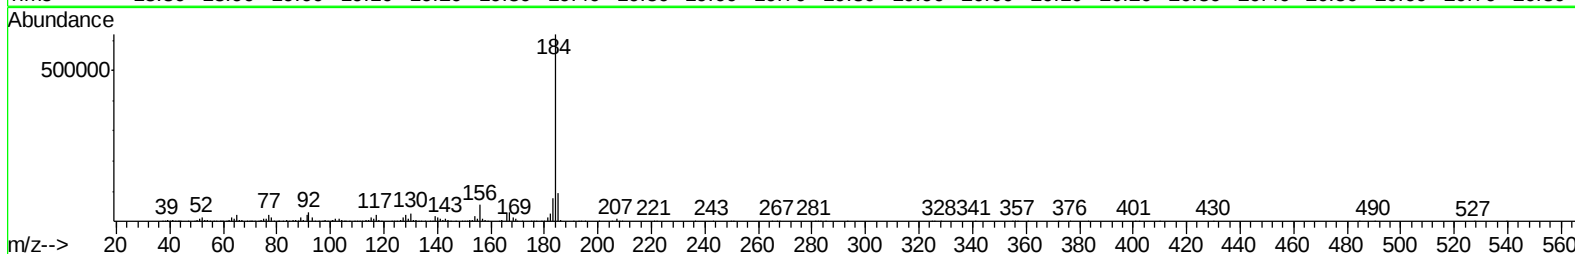


Data Path : Z:\HPCHEM1\BNA G\Data\BG062916\
Data File : BG022698.D
Acq On : 29 Jun 2016 18:00
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 08:11:16 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

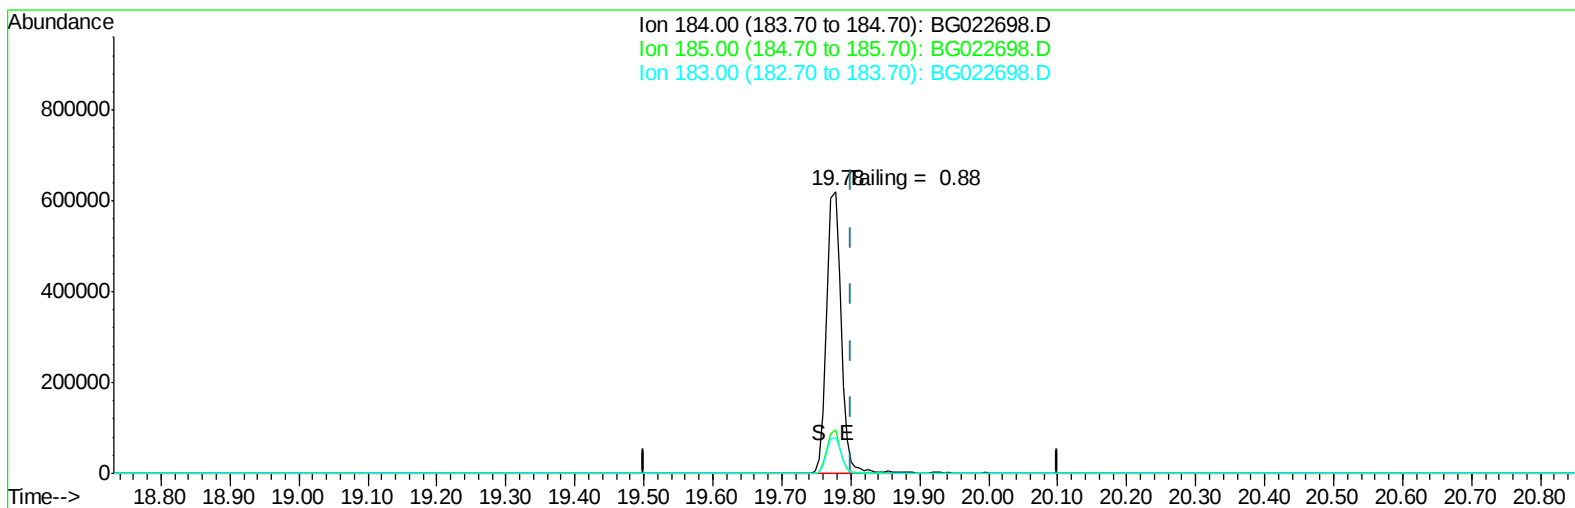

TIC: BG022698.D

(76) Benzidine




19.777min (-0.023) 792405.95ng

response 894266

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	15.43
183.00	13.40	12.65
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG062916\
Data File : BG022698.D
Acq On : 29 Jun 2016 18:00
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 08:11:16 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

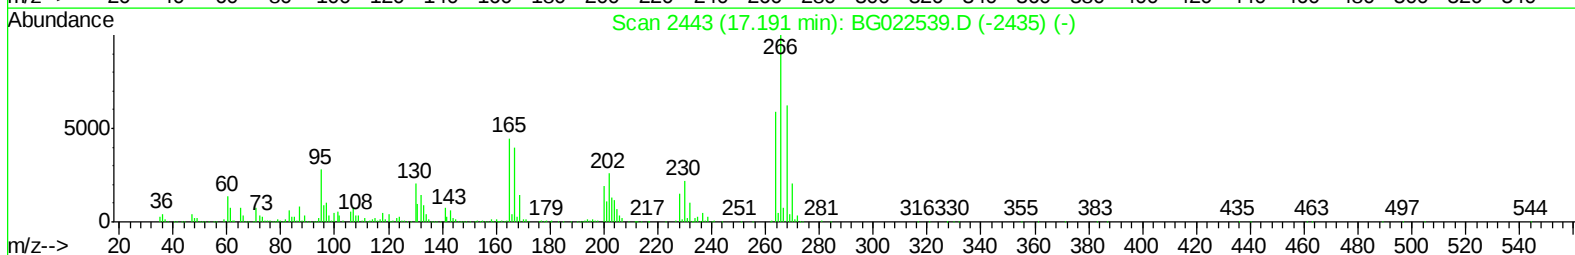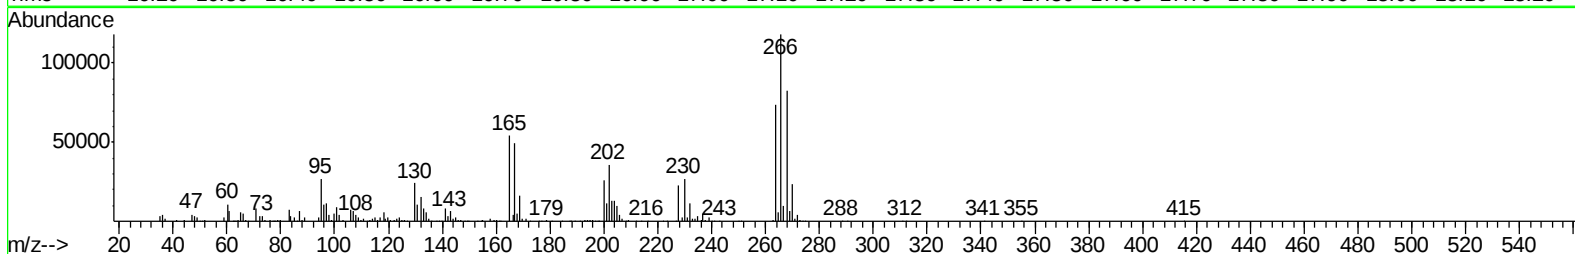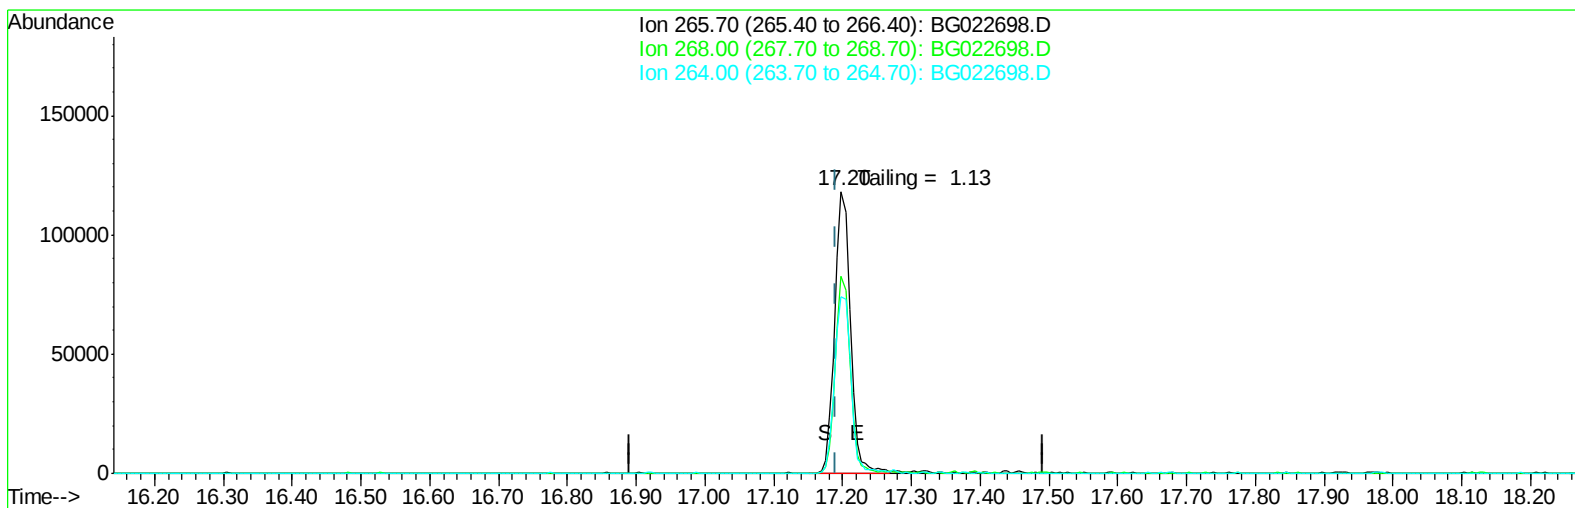

TIC: BG022698.D

(69) Pentachlorophenol (C)

17.198min (+0.006) 360098.37ng

response 186965

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	70.04
264.00	63.20	62.69
0.00	0.00	0.00