
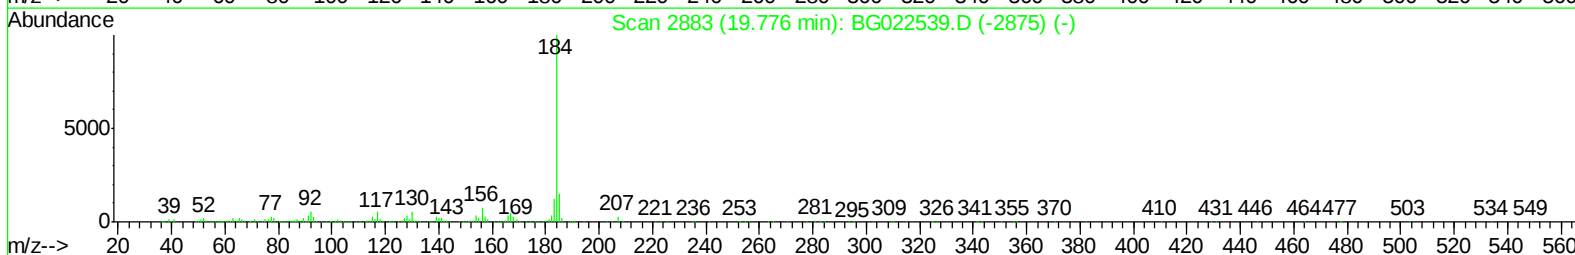
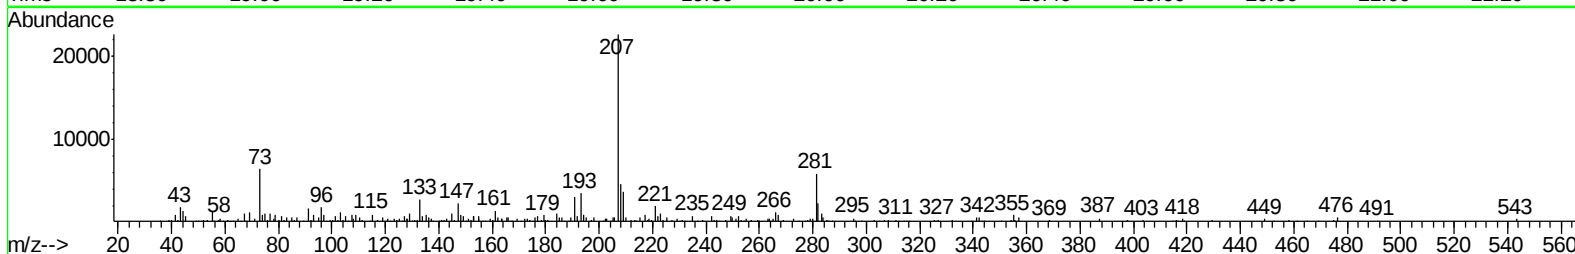


Data Path : Z:\HPCHEM1\BNA G\Data\BG062916\
Data File : BG022715.D
Acq On : 30 Jun 2016 5:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 08:13:18 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

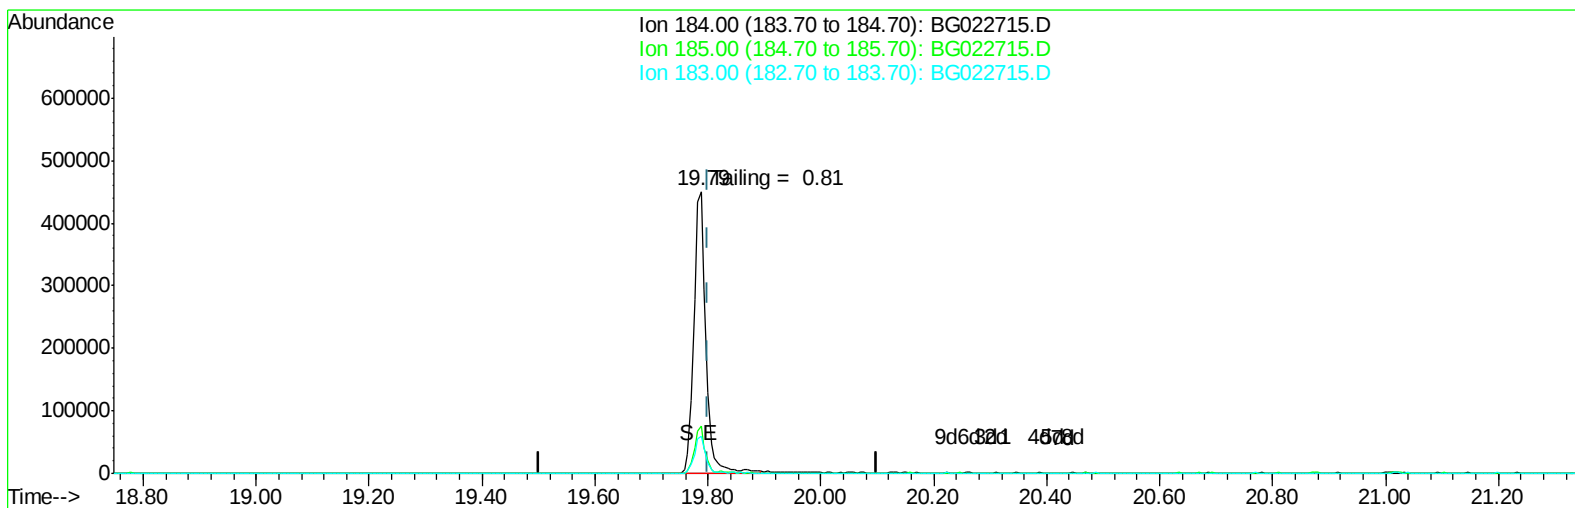

TIC: BG022715.D

(76) Benzidine




20.328min (+0.528) 375.70ng

response 416

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	63.06#
183.00	13.40	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG062916\
Data File : BG022715.D
Acq On : 30 Jun 2016 5:18
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 08:13:18 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 24 20:14:59 2016
Response via : Initial Calibration

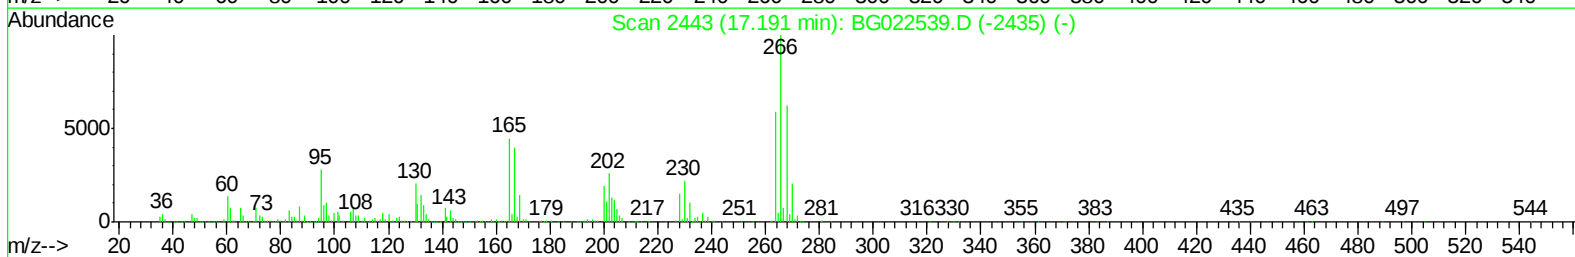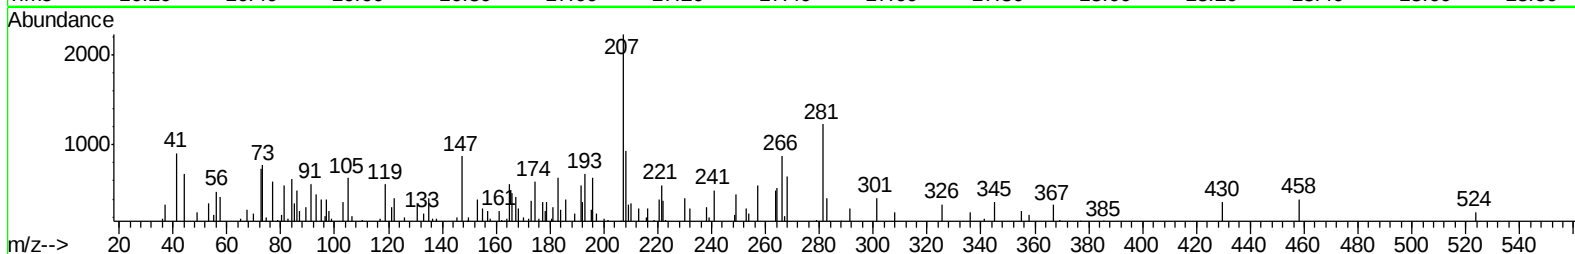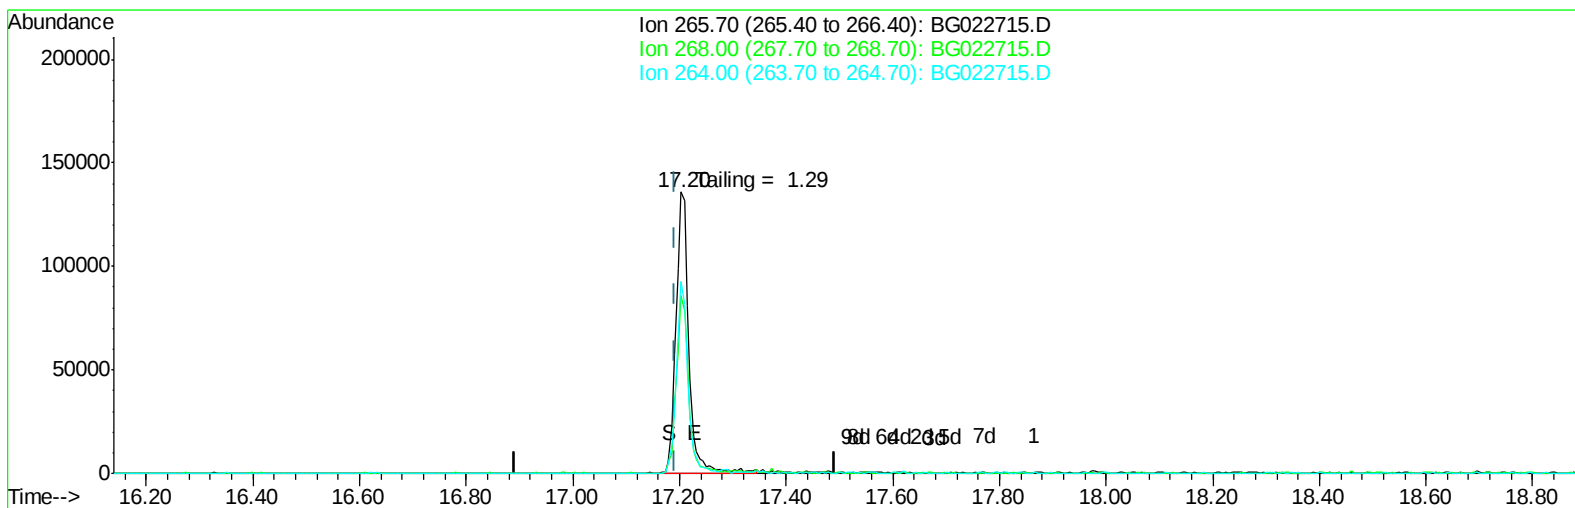

TIC: BG022715.D

(69) Pentachlorophenol (C)

17.867min (+0.675) 324.45ng

response 634

Ion	Exp%	Act%
265.70	100	100
268.00	64.90	74.00
264.00	63.20	59.52
0.00	0.00	0.00