


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062916\
 Data File : BG022698.D
 Acq On : 29 Jun 2016 18:00
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 20:14:59 2016

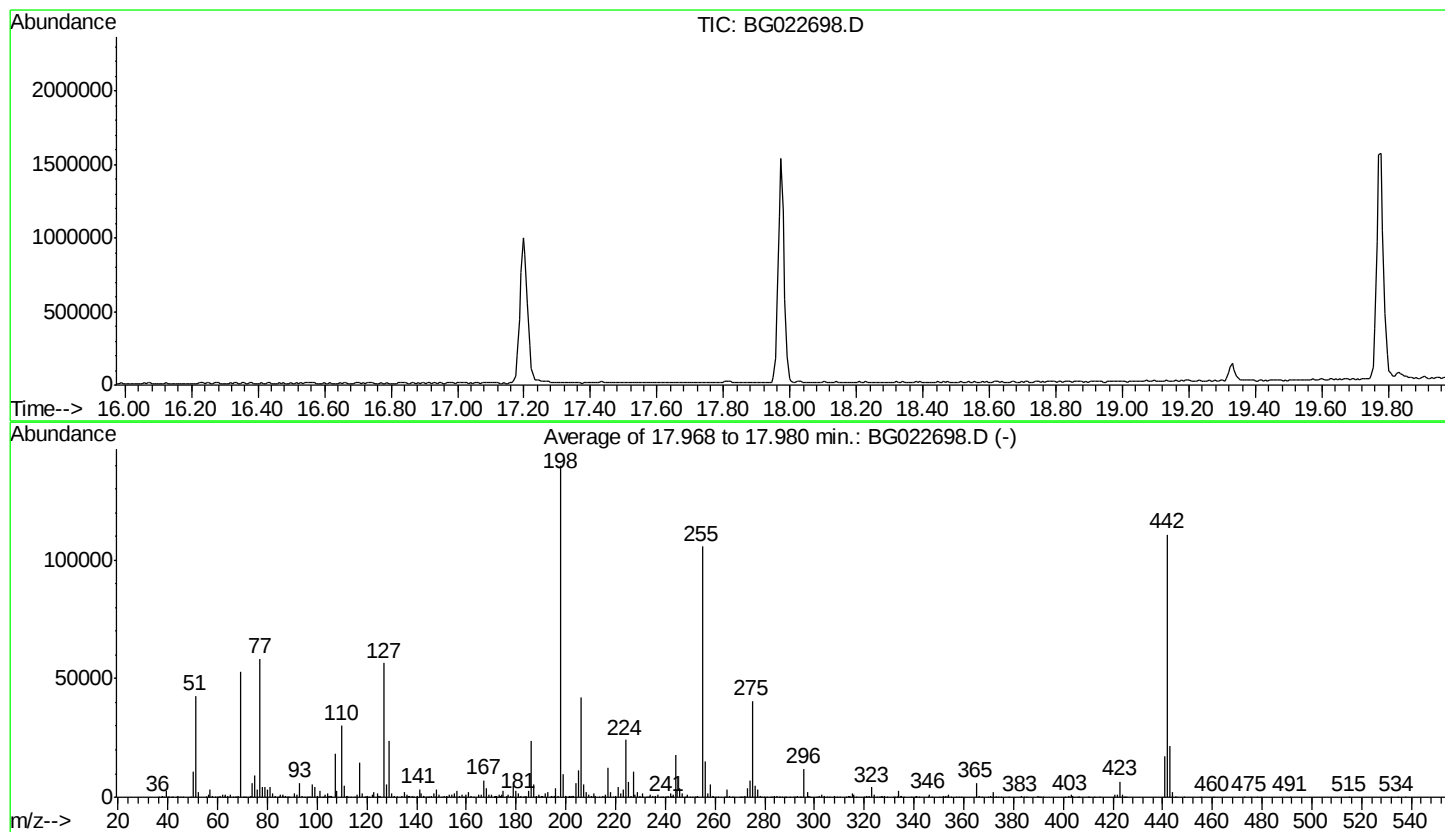

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	42778	PASS
68	69	0.00	2	0.7	373	PASS
69	198	0.00	100	37.9	53066	PASS
70	69	0.00	2	0.2	113	PASS
127	198	10	80	40.4	56568	PASS
197	198	0.00	2	0.3	482	PASS
198	198	100	100	100.0	139920	PASS
199	198	5	9	6.9	9647	PASS
275	198	10	60	29.0	40541	PASS
365	198	1	100	4.3	6055	PASS
441	442	0.01	24	15.7	17339	PASS
442	198	50	100	79.2	110762	PASS
443	442	15	24	19.6	21671	PASS