


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062916\
 Data File : BG022715.D
 Acq On : 30 Jun 2016 5:18
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 24 20:14:59 2016

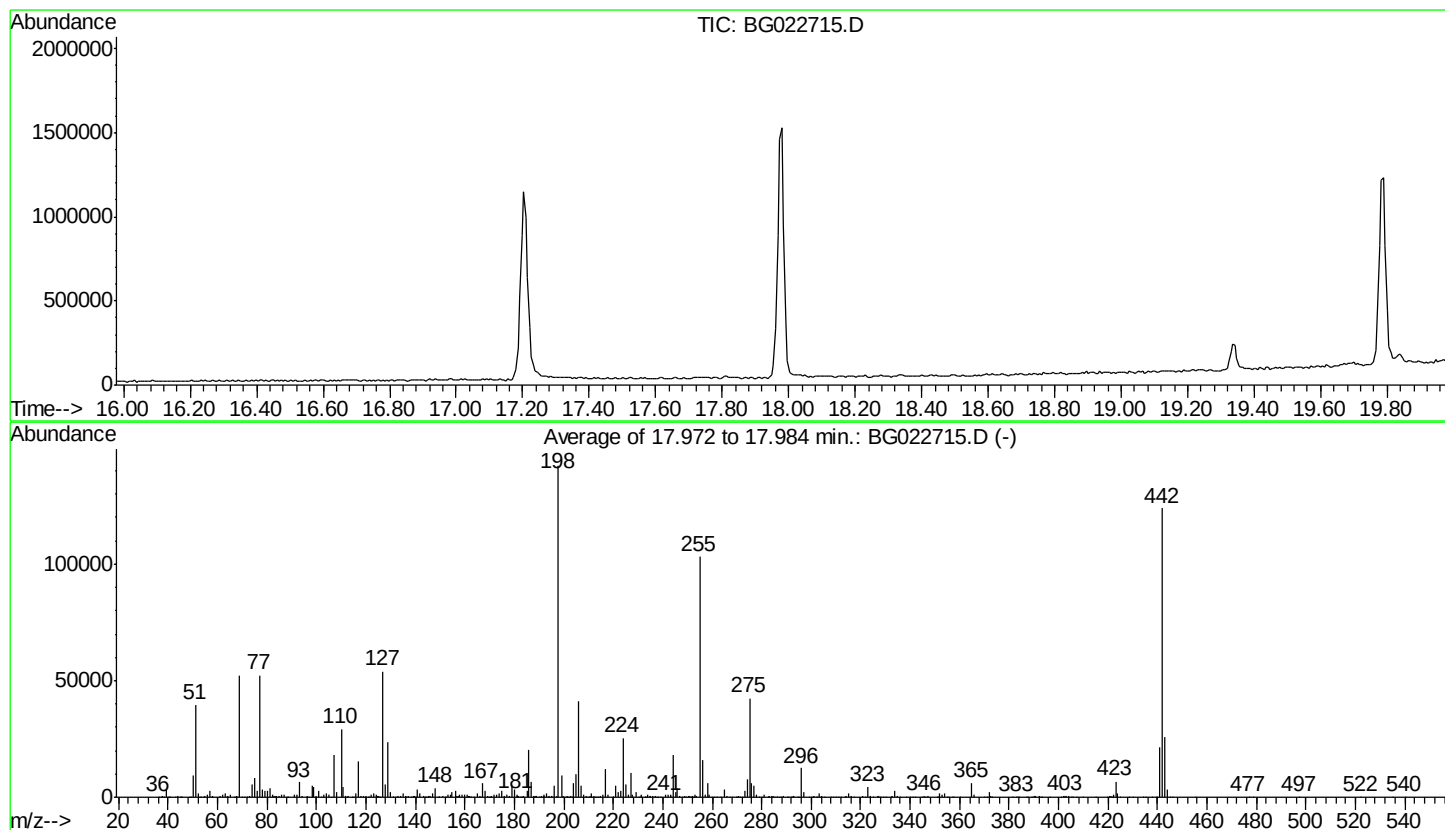

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	39658	PASS
68	69	0.00	2	1.1	576	PASS
69	198	0.00	100	36.6	52015	PASS
70	69	0.00	2	0.3	173	PASS
127	198	10	80	37.9	53861	PASS
197	198	0.00	2	0.5	657	PASS
198	198	100	100	100.0	142216	PASS
199	198	5	9	6.6	9316	PASS
275	198	10	60	29.8	42402	PASS
365	198	1	100	4.3	6045	PASS
441	442	0.01	24	17.2	21288	PASS
442	198	50	100	87.2	124016	PASS
443	442	15	24	20.8	25765	PASS