
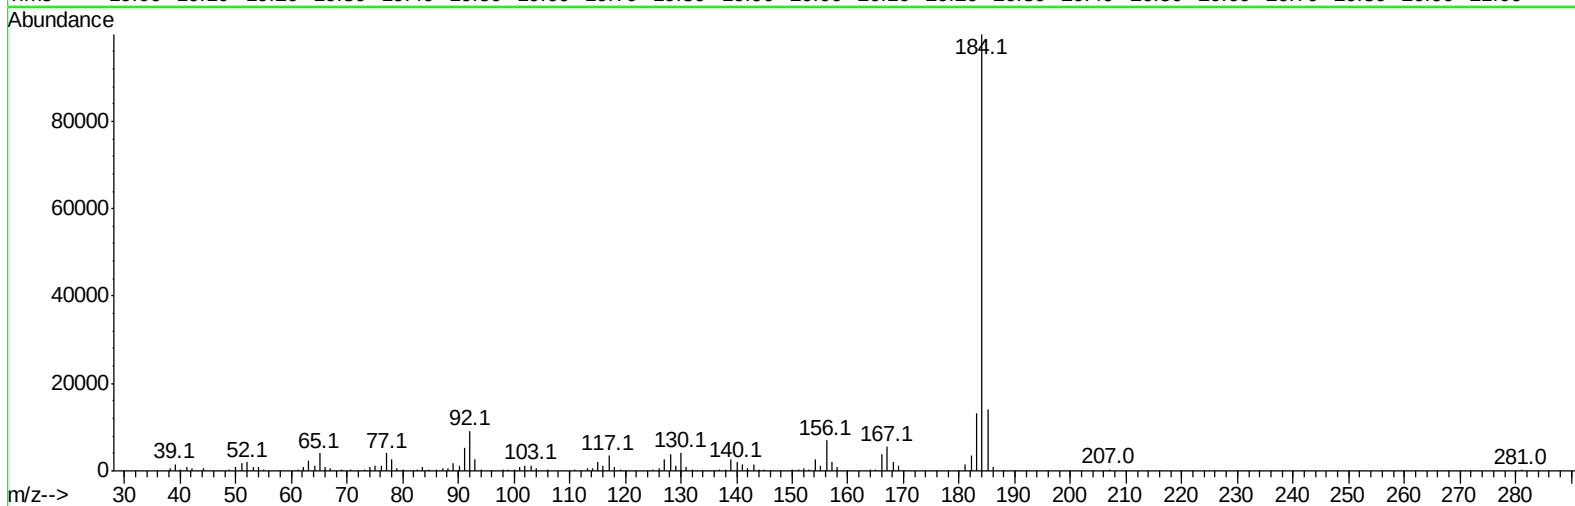


Data Path : Z:\HPCHEM1\BNA G\DATA\BG062917\
Data File : BG027741.D
Acq On : 29 Jun 2017 15:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 06:44:32 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 19:26:37 2017
Response via : Initial Calibration

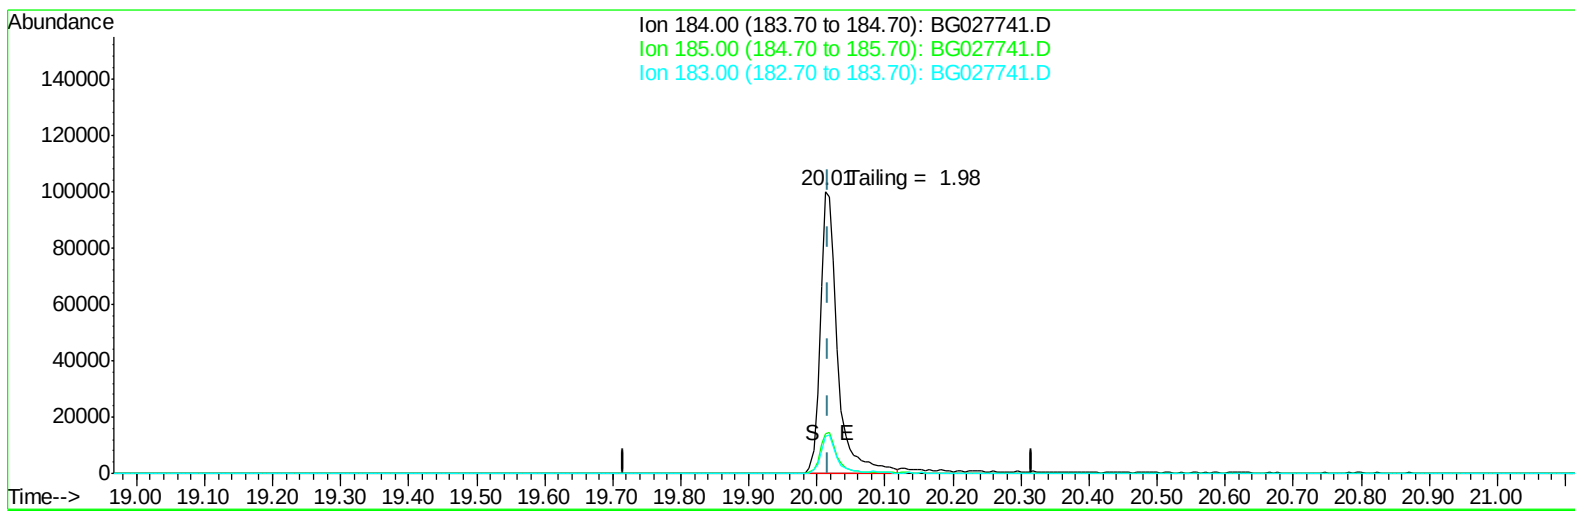

TIC: BG027741.D

(76) Benzidine



20.012min (-0.005) 0.00ng

response 178835

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.01
183.00	13.80	13.34
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062917\
Data File : BG027741.D
Acq On : 29 Jun 2017 15:10
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 06:44:32 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 19:26:37 2017
Response via : Initial Calibration

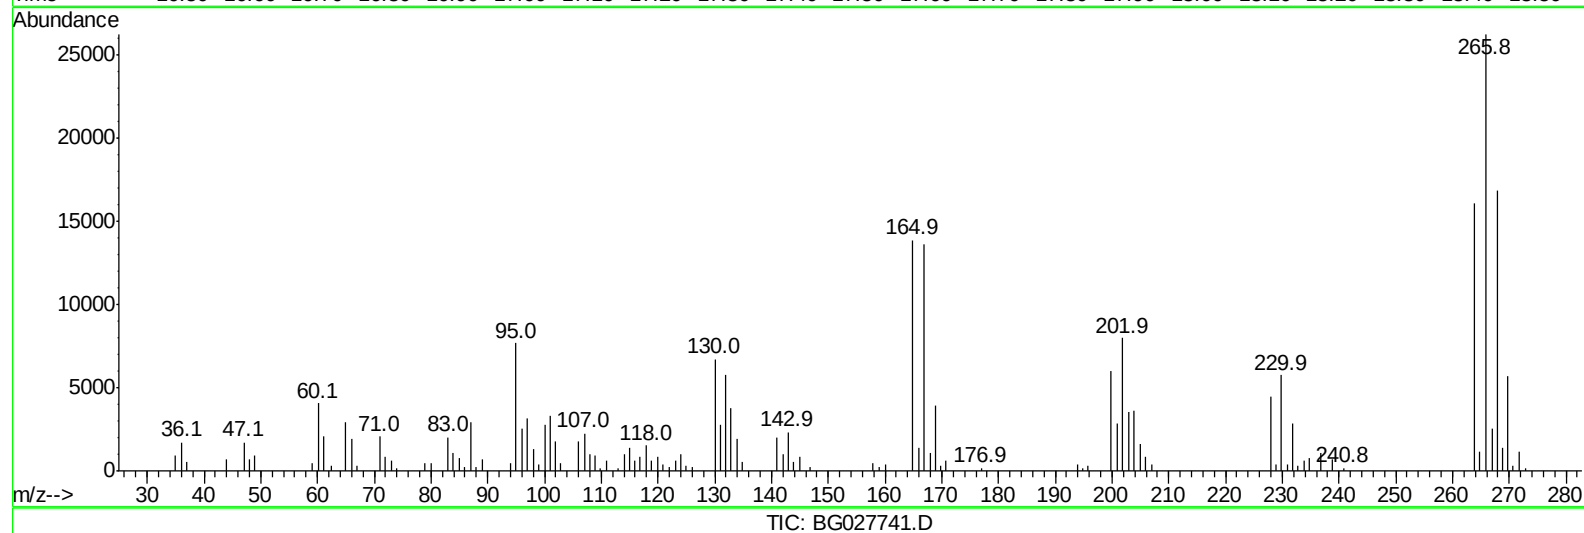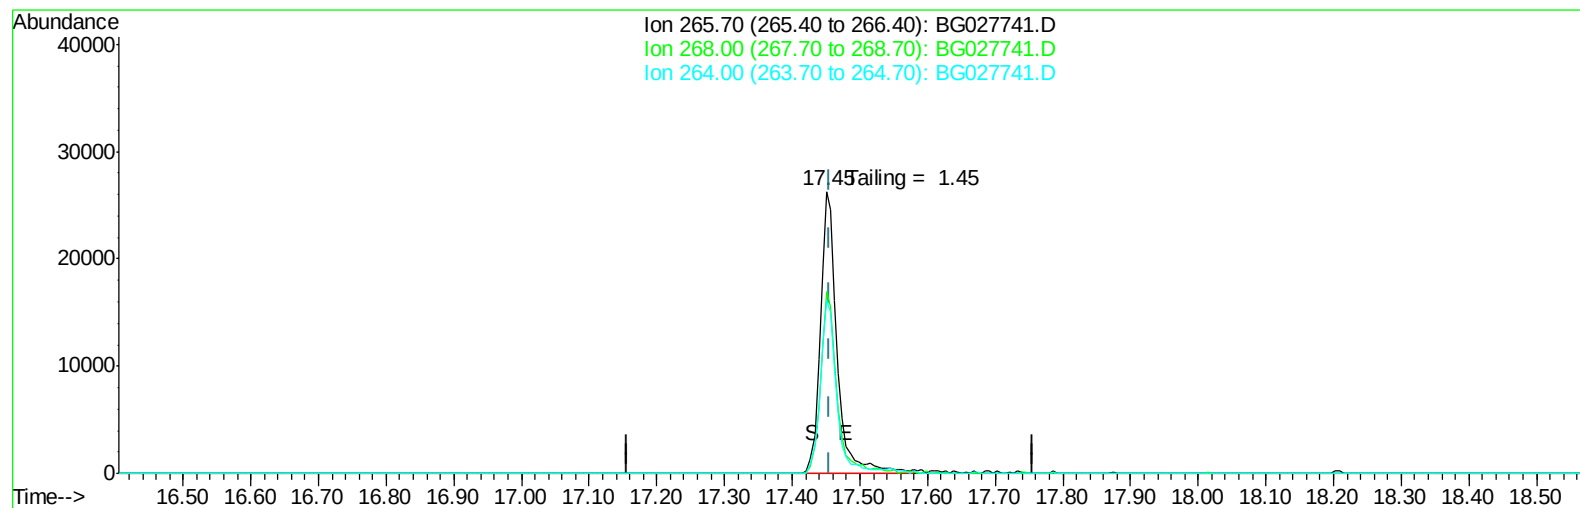

(69) Pentachlorophenol (C)

17.451min (-0.005) 0.00ng

response 45671

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	64.36
264.00	62.60	61.36
0.00	0.00	0.00