

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062917\
 Data File : BG027749.D
 Acq On : 29 Jun 2017 20:32
 Operator : SJ/JU
 Sample : I3905-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CAN-SB-05-11-50

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.609	286	293	302	rBV	84905	142568	7.17%	1.268%
2	6.056	362	369	382	rBV	456065	772204	38.84%	6.870%
3	7.613	626	634	647	rBV	458835	849381	42.72%	7.556%
4	8.006	693	701	712	rBV	439410	805568	40.52%	7.167%
5	8.477	774	781	791	rVB	103228	187733	9.44%	1.670%
6	8.800	828	836	847	rVB	287477	531664	26.74%	4.730%
7	9.640	971	979	988	rBV	262595	491069	24.70%	4.369%
8	11.291	1252	1260	1268	rBV	163360	304099	15.30%	2.705%
9	13.682	1658	1667	1678	rBV	695194	1094746	55.06%	9.739%
10	14.493	1798	1805	1812	rBV	303058	448630	22.57%	3.991%
11	15.063	1894	1902	1909	rBV2	248663	425613	21.41%	3.786%
12	16.544	2147	2154	2171	rBV	661290	1027263	51.67%	9.139%
13	16.720	2179	2184	2192	rBV2	15629	26699	1.34%	0.238%
14	17.807	2363	2369	2375	rBV2	353538	591270	29.74%	5.260%
15	17.848	2375	2376	2381	rVB	25484	29753	1.50%	0.265%
16	18.653	2507	2513	2521	rBV7	11223	26512	1.33%	0.236%
17	19.846	2711	2716	2721	rVB	29886	43944	2.21%	0.391%
18	20.204	2773	2777	2783	rVB	26999	40743	2.05%	0.362%
19	20.386	2802	2808	2815	rBV	1482973	1988130	100.00%	17.687%
20	22.172	3103	3112	3118	rBV	387035	733976	36.92%	6.530%
21	25.780	3713	3726	3738	rBV3	199014	679022	34.15%	6.041%


Sum of corrected areas: 11240587

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062917\
Data File : BG027749.D
Acq On : 29 Jun 2017 20:32
Operator : SJ/JU
Sample : I3905-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CAN-SB-05-11-50

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

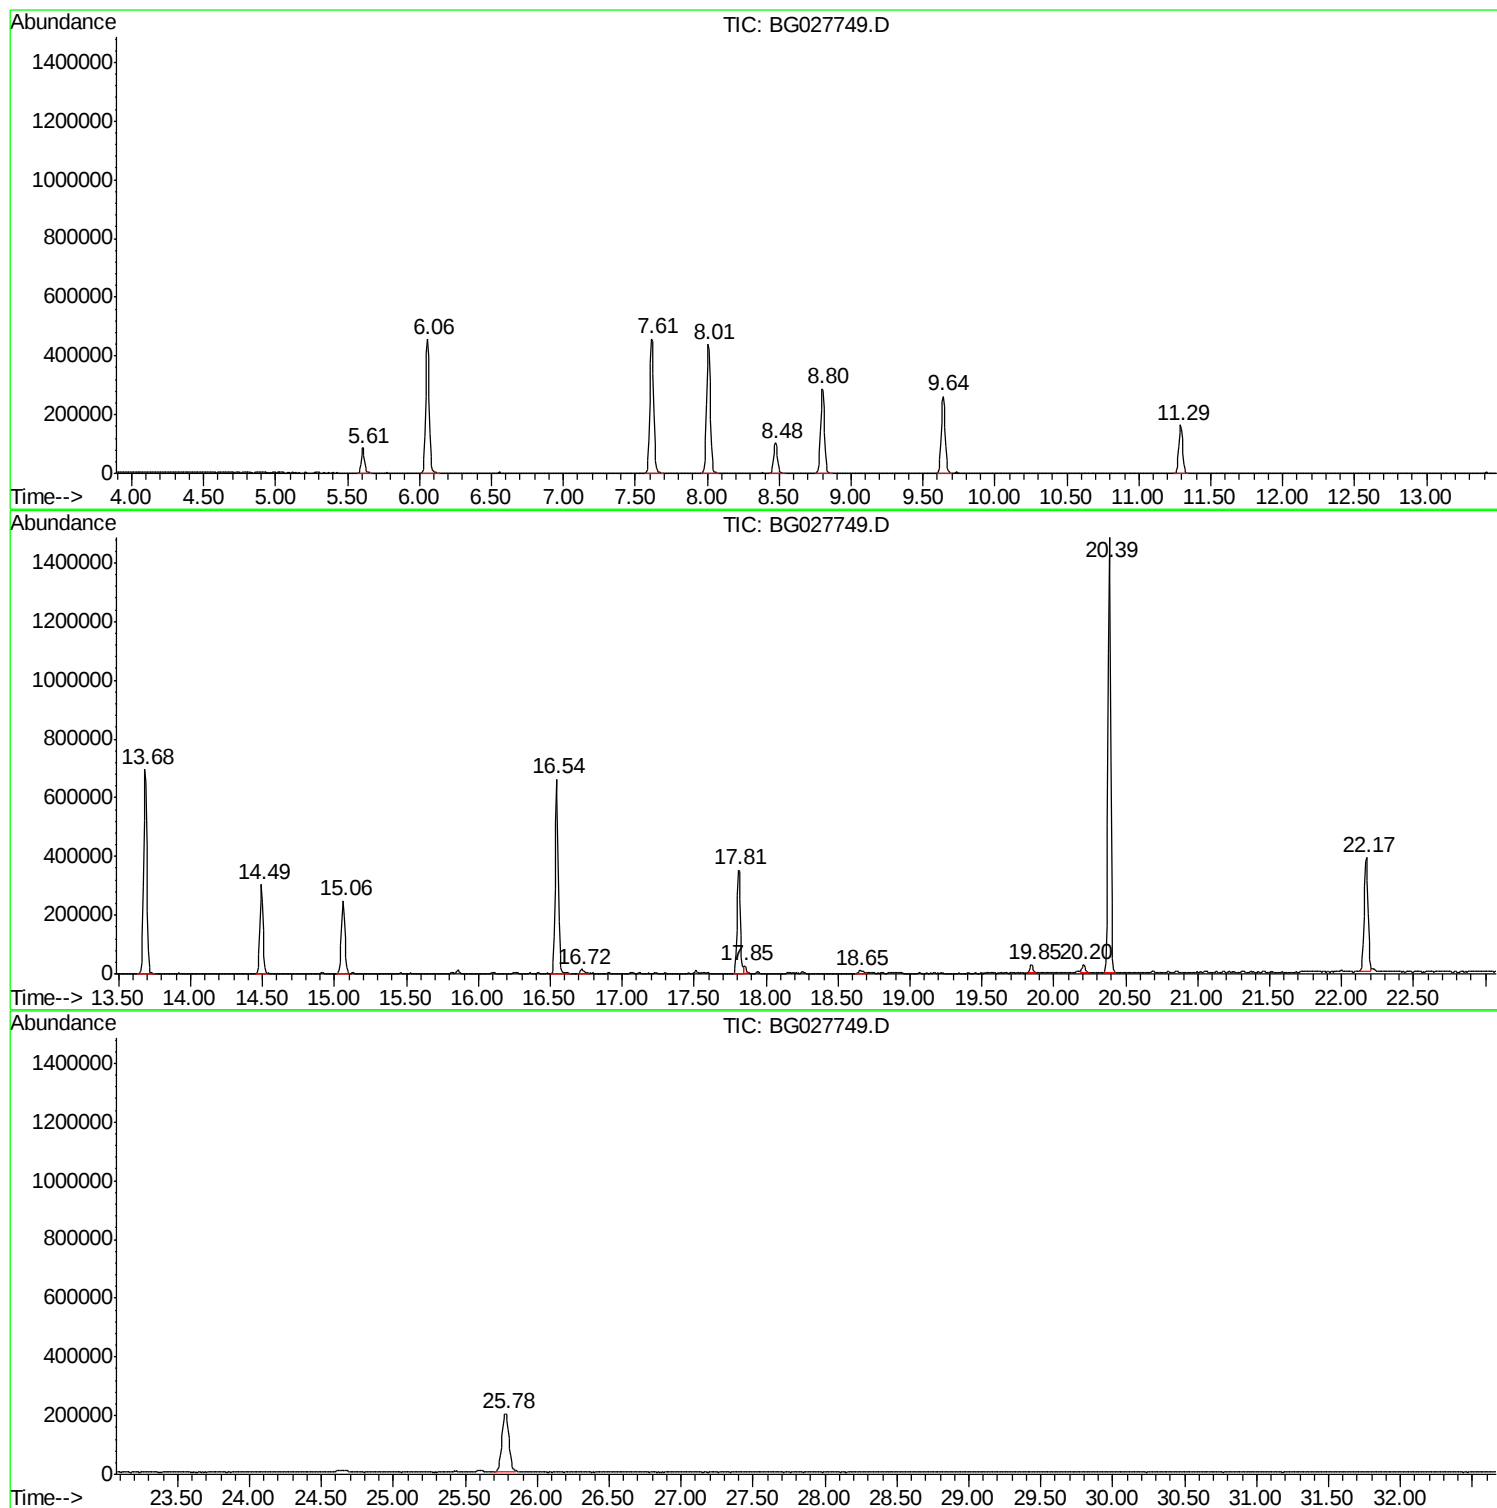

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062917\
Data File : BG027749.D
Acq On : 29 Jun 2017 20:32
Operator : SJ/JU
Sample : I3905-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CAN-SB-05-11-50










Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.61	15.19 ng	142568	1,4-Dichlorobenzene-d4	8.48

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2		3-Pentanol, 2-methyl-	102	C6H14O	000565-67-3	33
3		3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
4		Acetic acid, cyano-, 1,1-dimethyl-	141	C7H11NO2	001116-98-9	23
5		Pentane, 2-methoxy-	102	C6H14O	006795-88-6	9

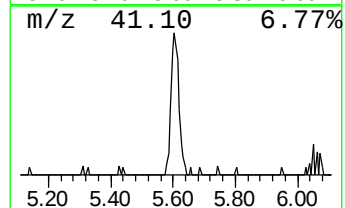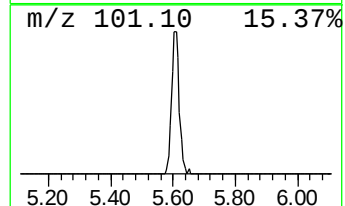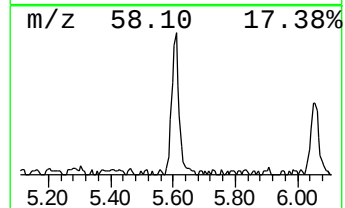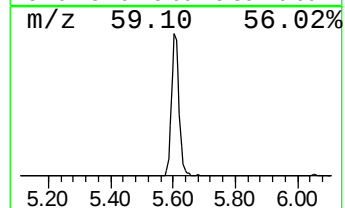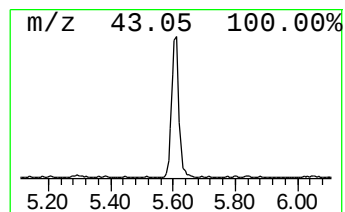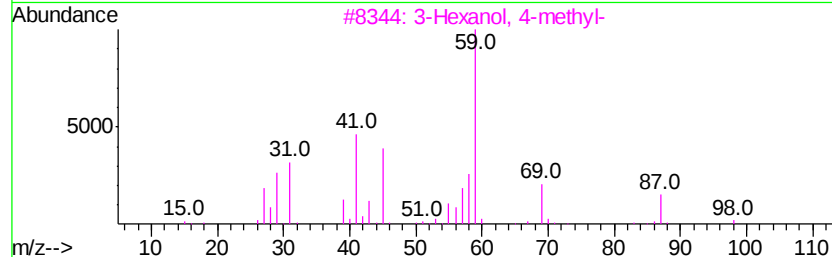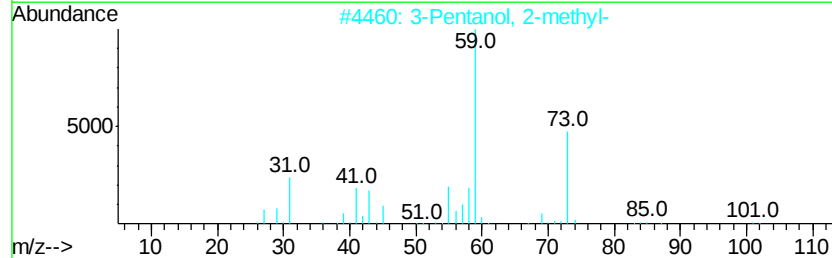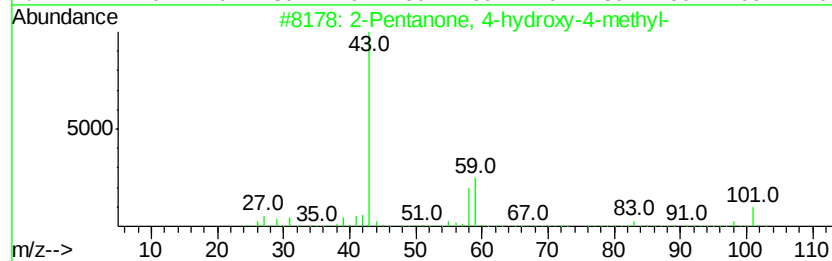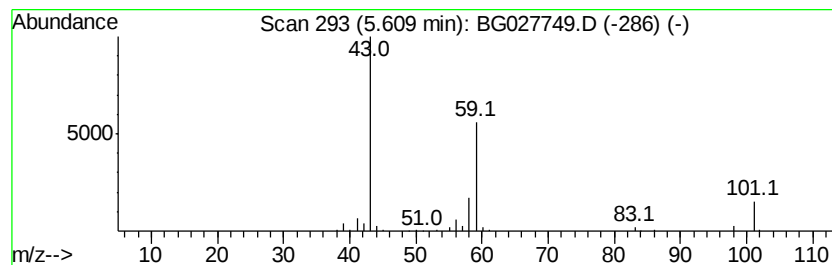

Data Path : Z:\HPCHEM1\BNA G\DATA\BG062917\
Data File : BG027749.D
Acq On : 29 Jun 2017 20:32
Operator : SJ/JU
Sample : I3905-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CAN-SB-05-11-50








Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown8.01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.01	85.82 ng	805568	1,4-Dichlorobenzene-d4	8.48

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

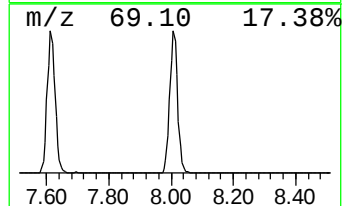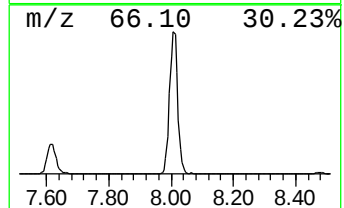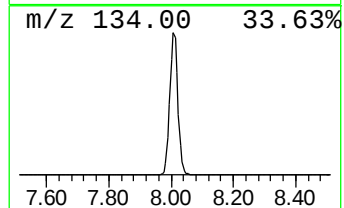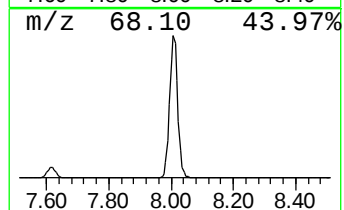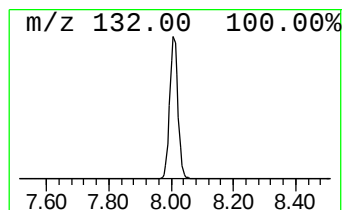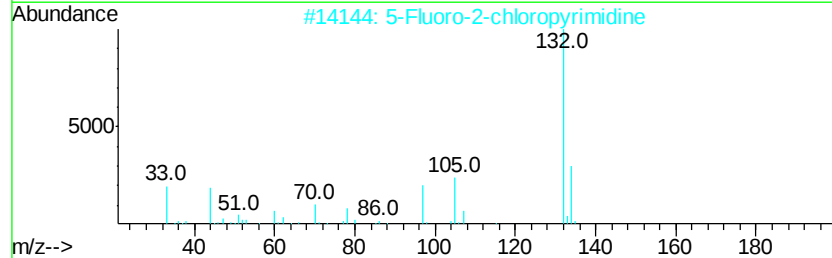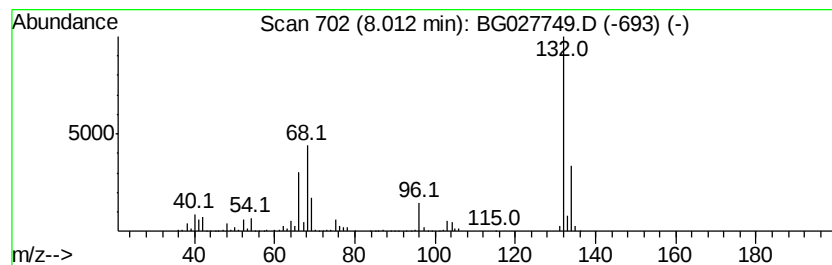

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG062917\
Data File : BG027749.D
Acq On : 29 Jun 2017 20:32
Operator : SJ/JU
Sample : I3905-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CAN-SB-05-11-50

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.61	15.2	ng	142568	1	8.48	187733	20.0
unknown8.01	8.01	85.8	ng	805568	1	8.48	187733	20.0