
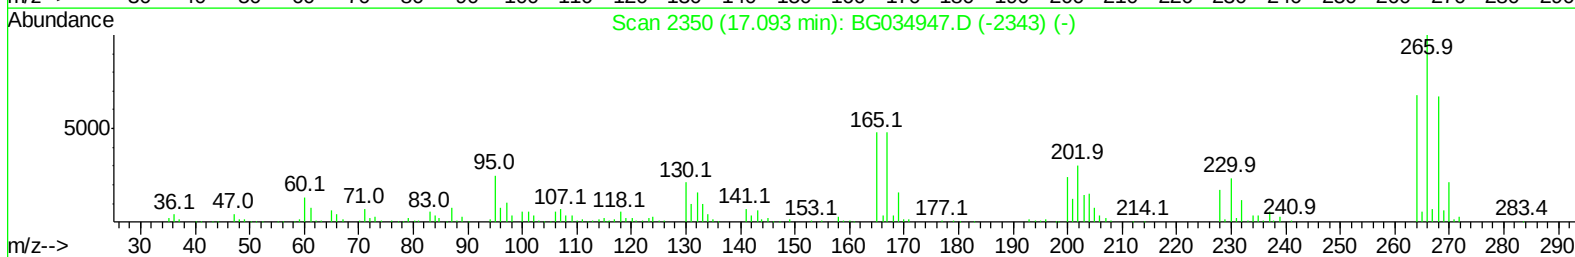
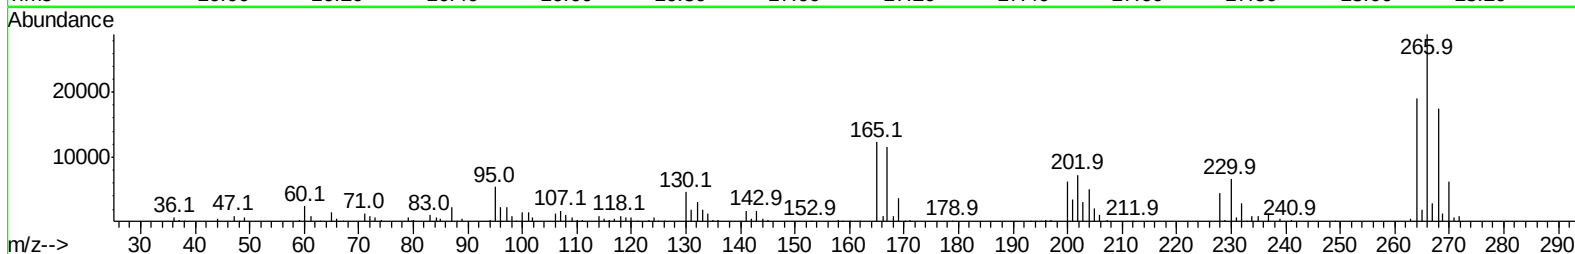


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062918\
Data File : BG035515.D
Acq On : 29 Jun 2018 21:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 08:29:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

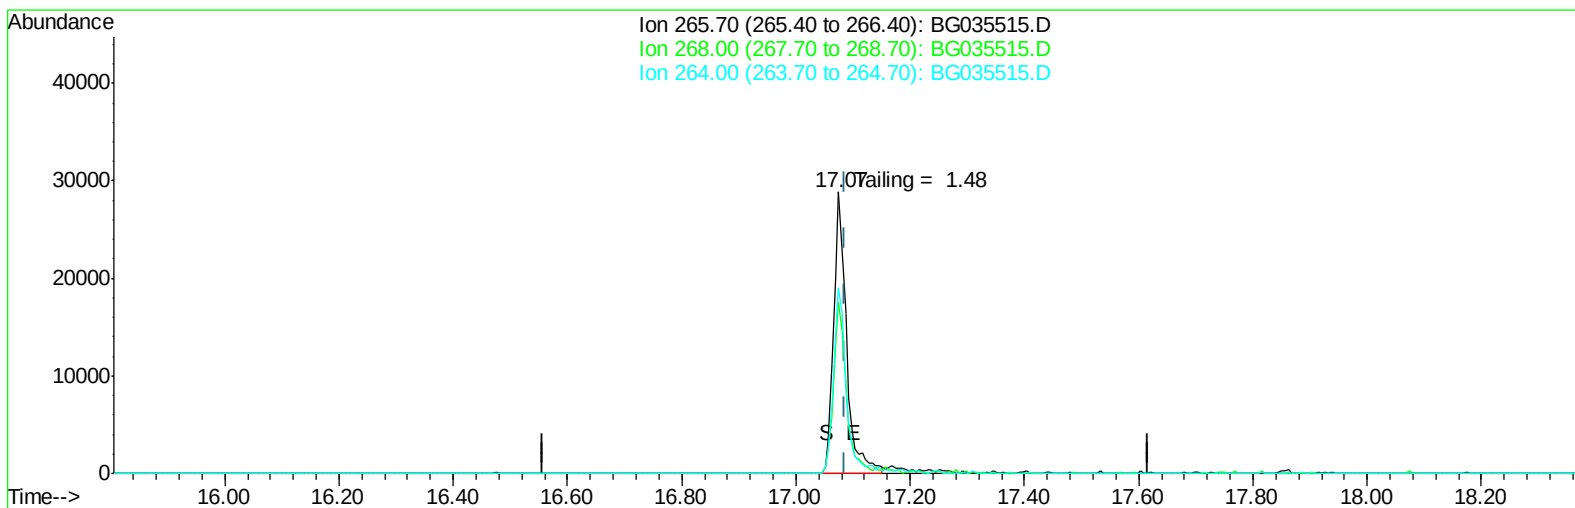

TIC: BG035515.D

(69) Pentachlorophenol (C)




17.075min (-0.013) 9917.78ng

response 45204

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.75
264.00	62.00	66.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG062918\
Data File : BG035515.D
Acq On : 29 Jun 2018 21:24
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 08:29:03 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG060718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 08 17:16:28 2018
Response via : Initial Calibration

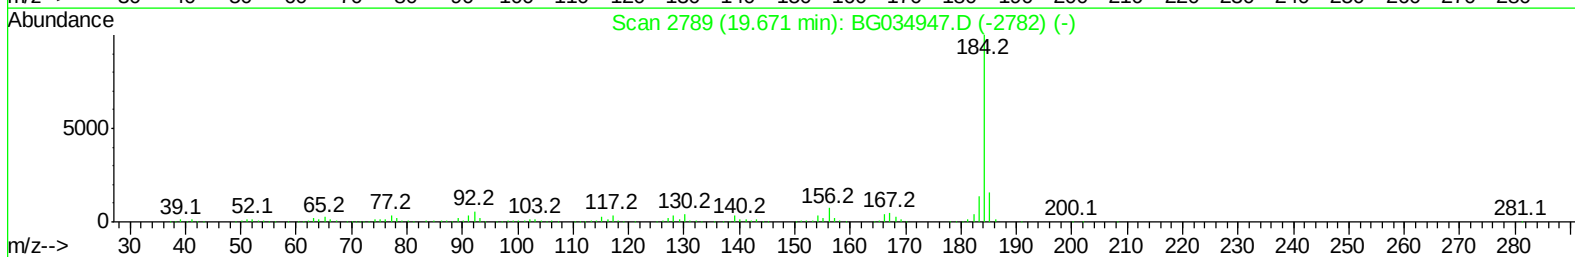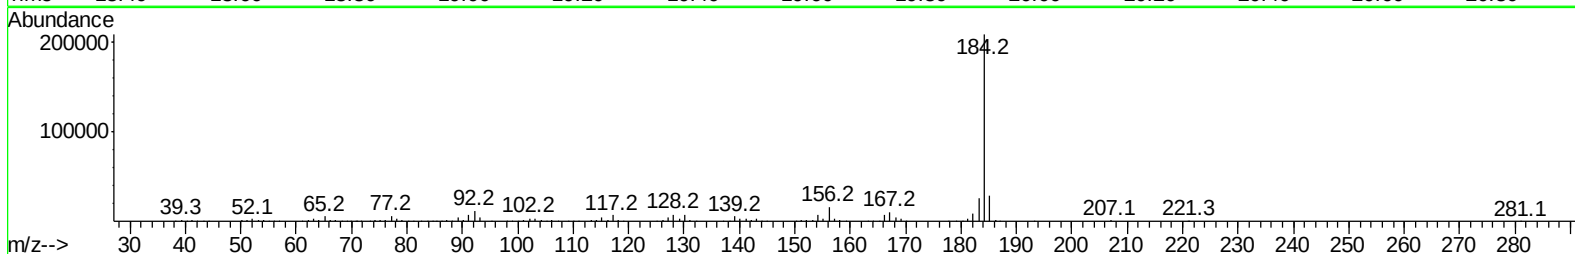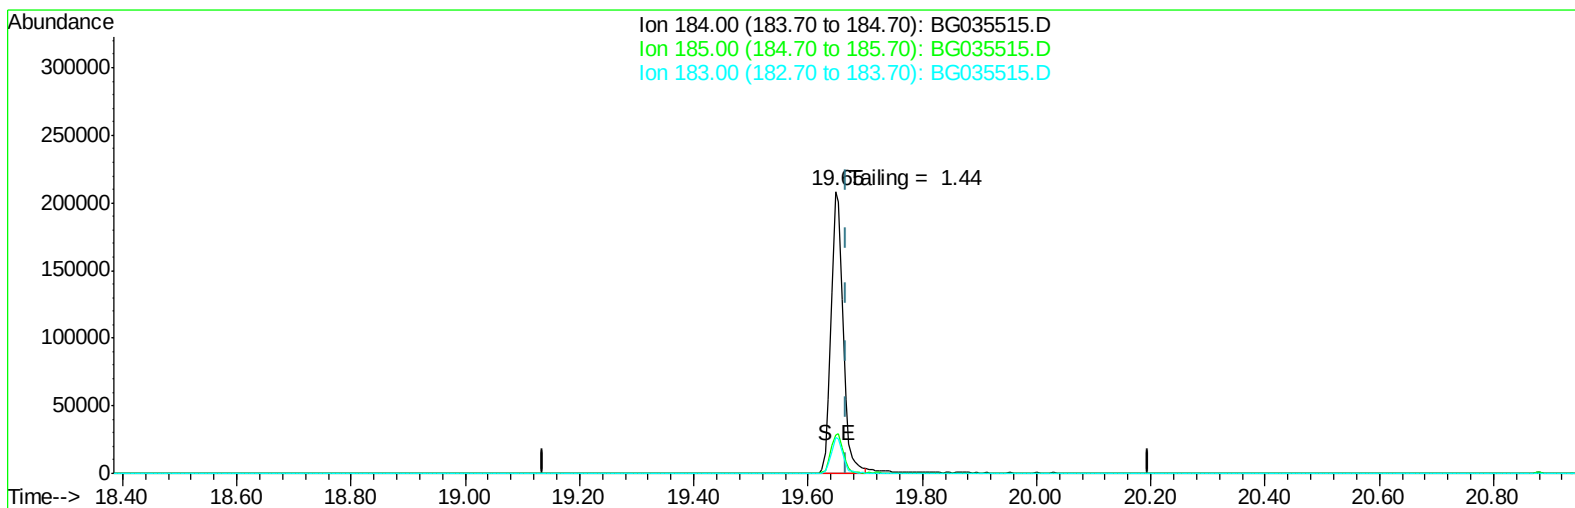

TIC: BG035515.D

(76) Benzidine

19.648min (-0.019) 0.00ng

response 308261

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.83
183.00	13.30	12.62
0.00	0.00	0.00