


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062918\
 Data File : BG035506.D
 Acq On : 29 Jun 2018 9:46
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG060718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 08 17:16:28 2018

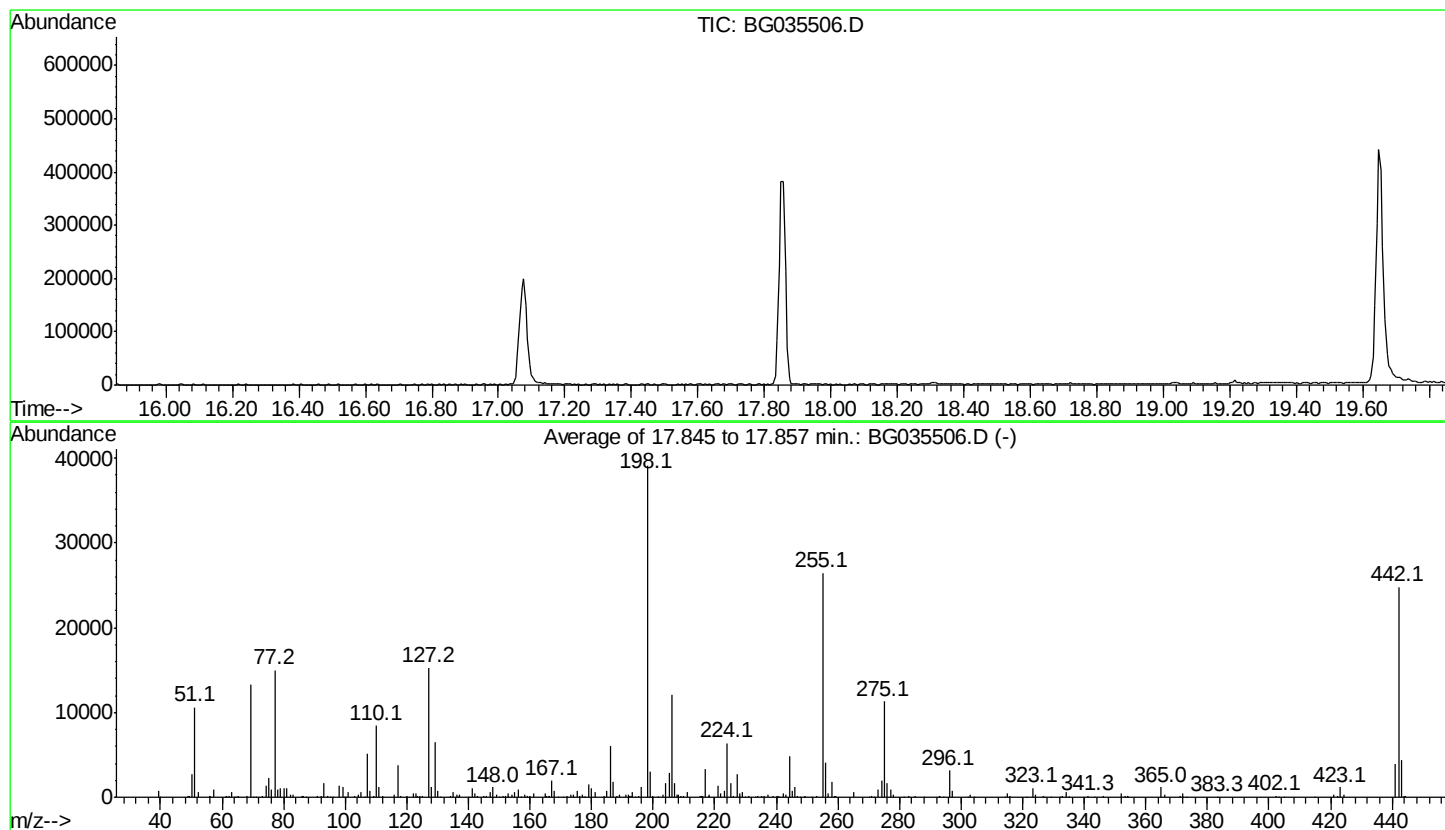

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	10576	PASS
68	69	0.00	2	1.1	149	PASS
69	198	0.00	100	34.2	13367	PASS
70	69	0.00	2	0.4	60	PASS
127	198	10	80	39.1	15284	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39125	PASS
199	198	5	9	7.8	3055	PASS
275	198	10	60	28.8	11268	PASS
365	198	1	100	3.0	1185	PASS
441	443	0.01	100	89.1	3877	PASS
442	198	50	100	63.5	24825	PASS
443	442	15	24	17.5	4352	PASS