
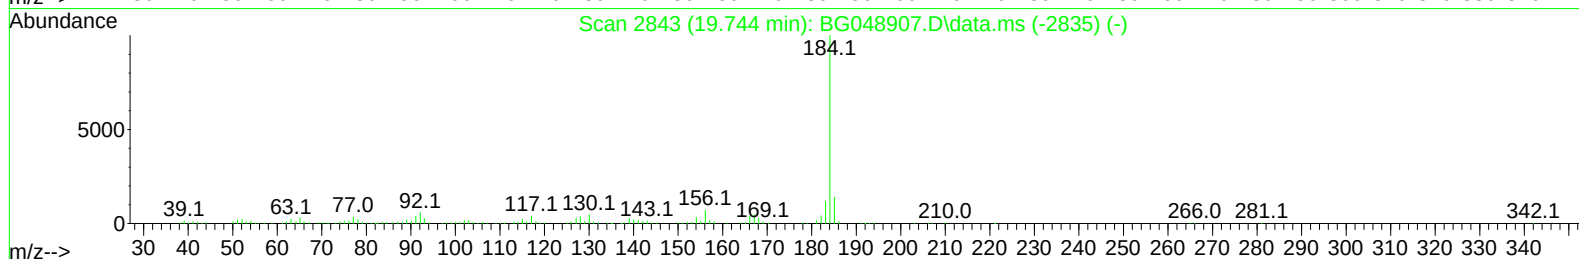
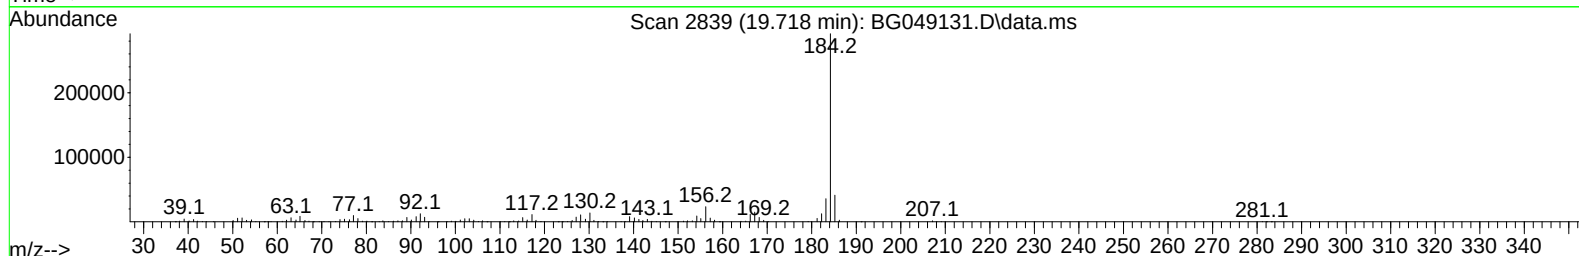


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062921\
Data File : BG049131.D
Acq On : 29 Jun 2021 11:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 12:45:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

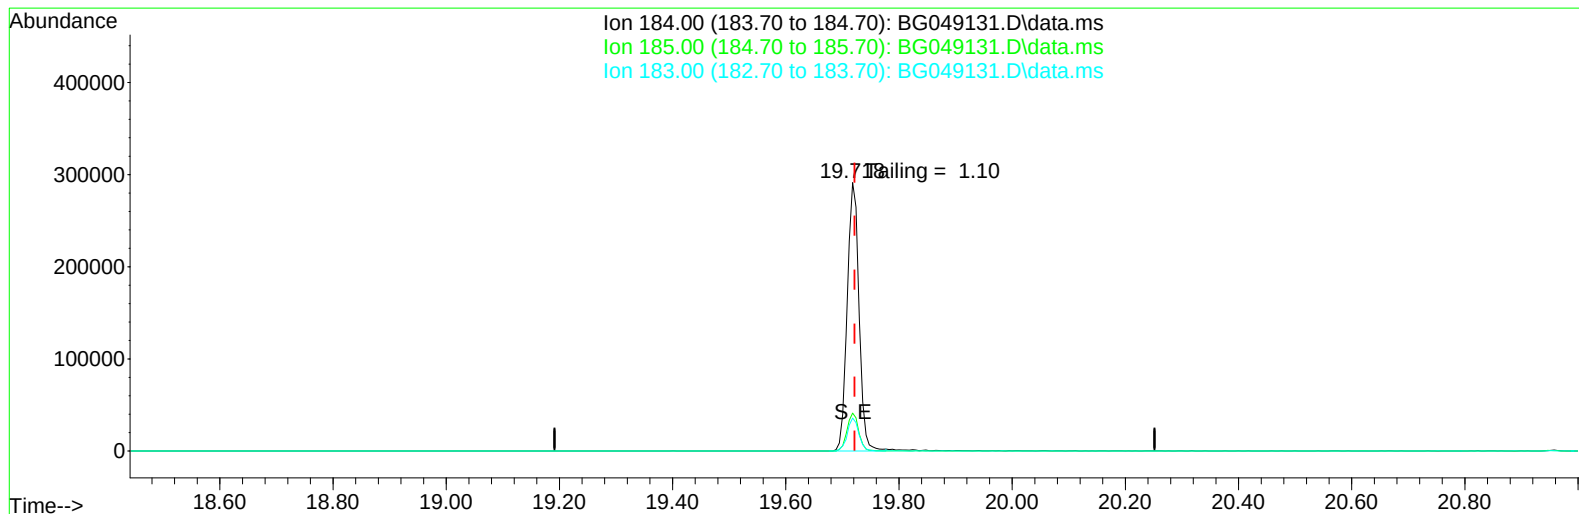

TIC: BG049131.D\data.ms

(77) Benzidine




19.718min (-0.003) 5844.45 ng m

response 423850

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.16
183.00	11.70	12.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062921\
Data File : BG049131.D
Acq On : 29 Jun 2021 11:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 29 12:45:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 24 11:02:36 2021
Response via : Initial Calibration

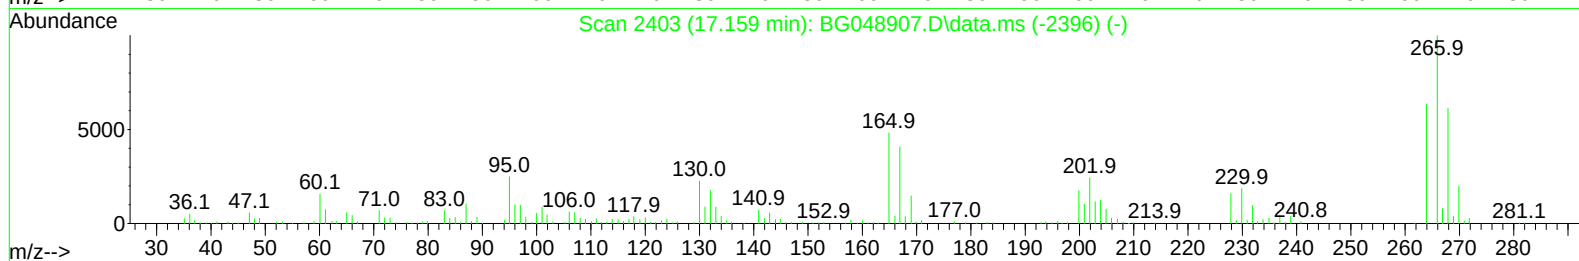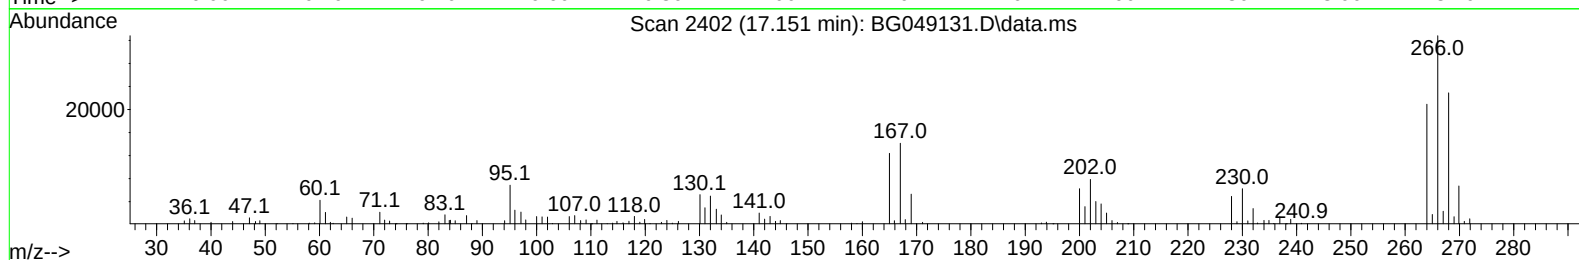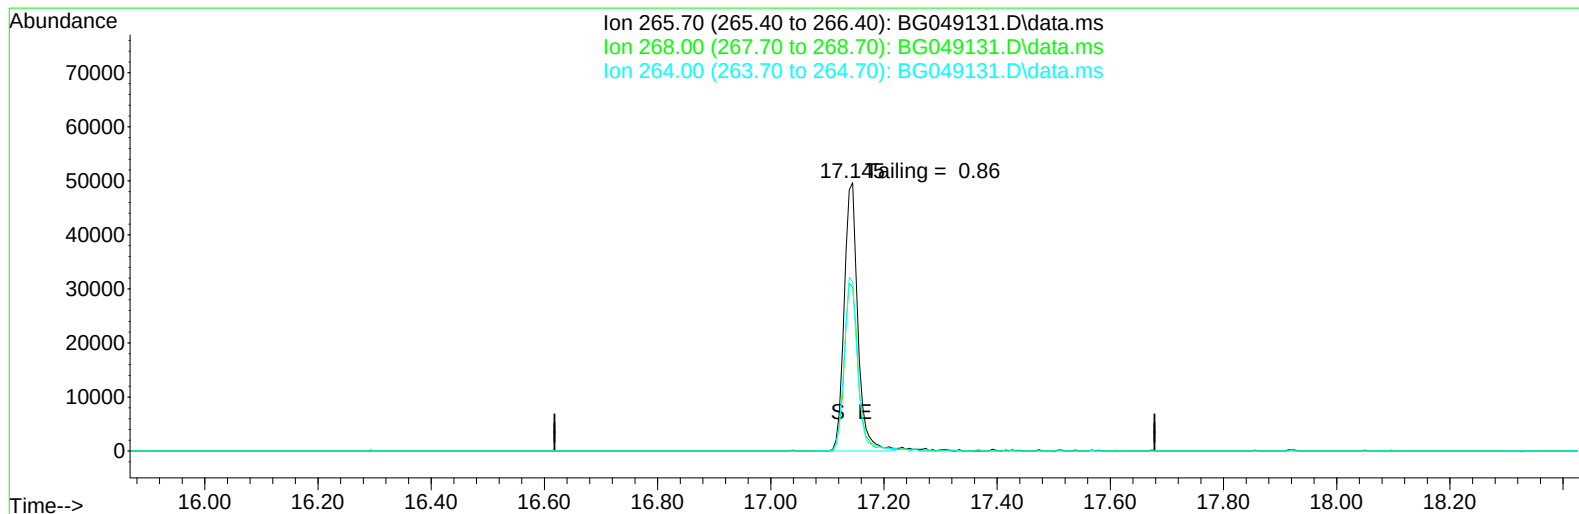

TIC: BG049131.D\data.ms

(70) Pentachlorophenol (C)

17.148min (-17.148) 0.00 ng

response 0

Ion	Exp%	Act%
265.70	100.00	0.00
268.00	61.20	0.00#
264.00	61.30	0.00#
0.00	0.00	0.00