


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062921\
 Data File : BG049131.D
 Acq On : 29 Jun 2021 11:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 24 11:02:36 2021

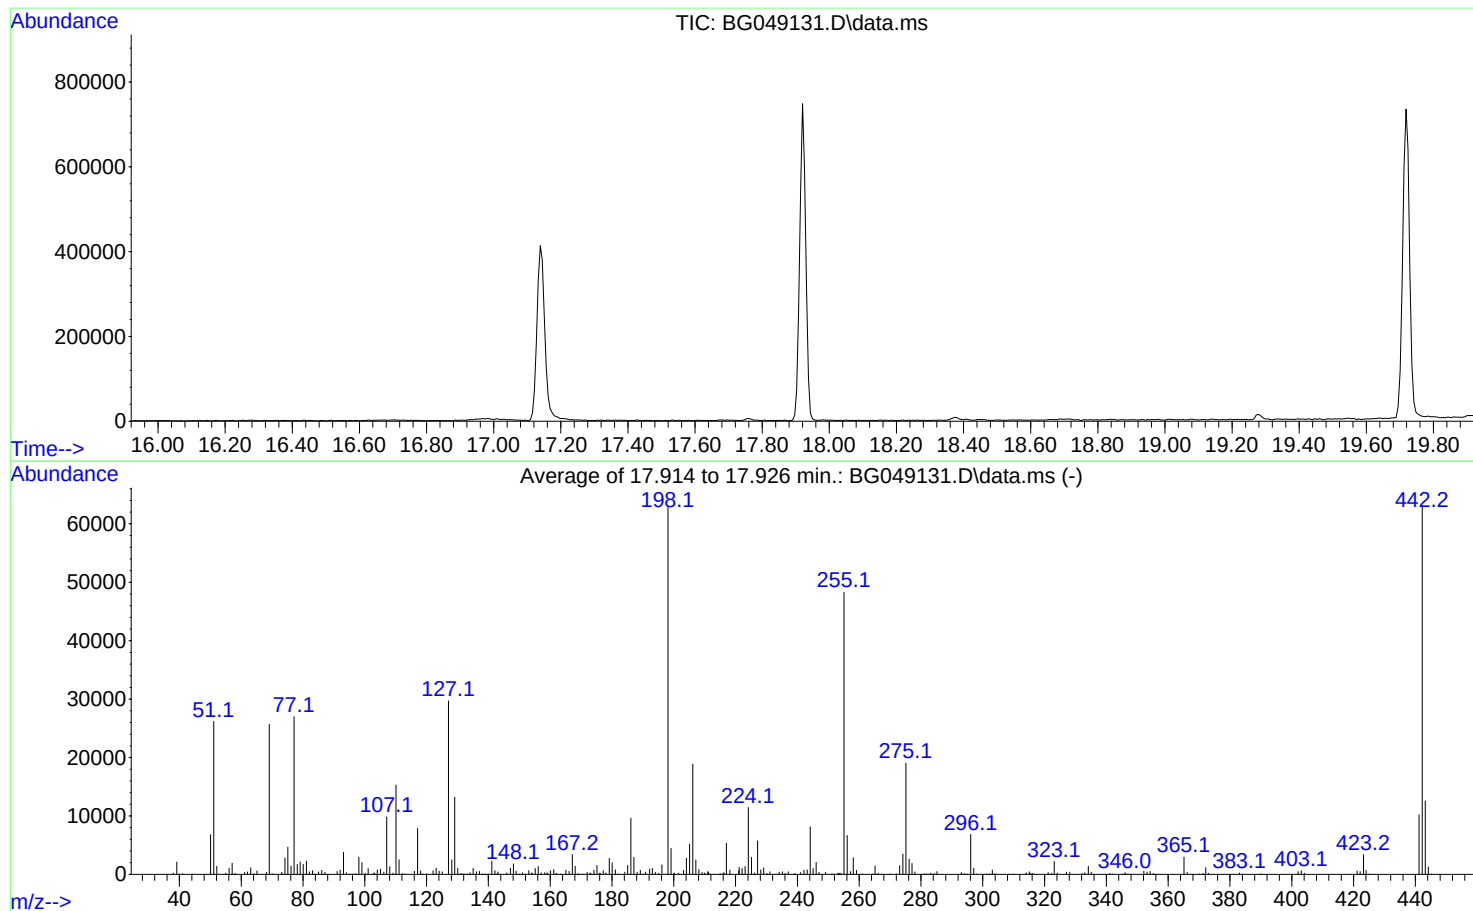




AutoFind: Scans 2532, 2533, 2534; Background Corrected with Scan 2525

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	26187	PASS
68	69	0.00	2	1.4	352	PASS
69	198	0.00	100	40.8	25677	PASS
70	69	0.00	2	0.3	67	PASS
127	198	10	80	47.2	29704	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62973	PASS
199	198	5	9	7.1	4449	PASS
275	198	10	60	30.2	19023	PASS
365	198	1	100	4.7	2971	PASS
441	198	0.01	100	16.2	10181	PASS
442	442	100	100	100.0	62891	PASS
443	442	15	24	20.0	12583	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062921\
 Data File : BG049131.D
 Acq On : 29 Jun 2021 11:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 29 12:45:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 24 11:02:36 2021
 Response via : Initial Calibration

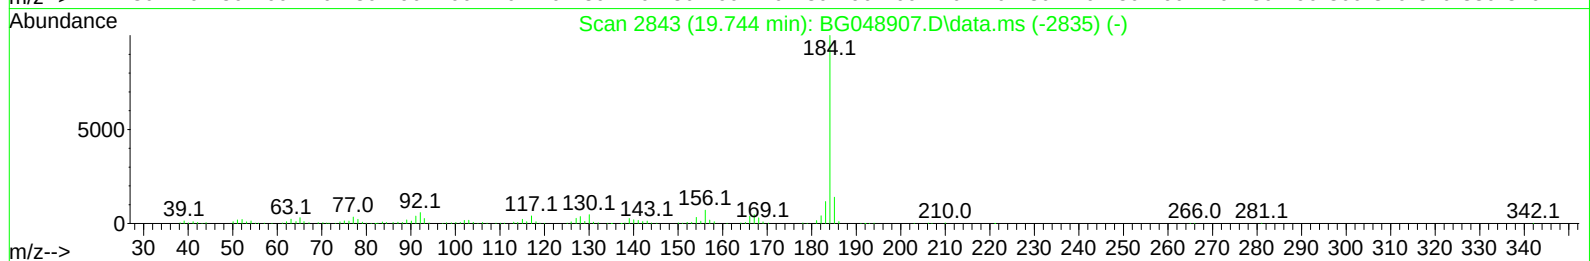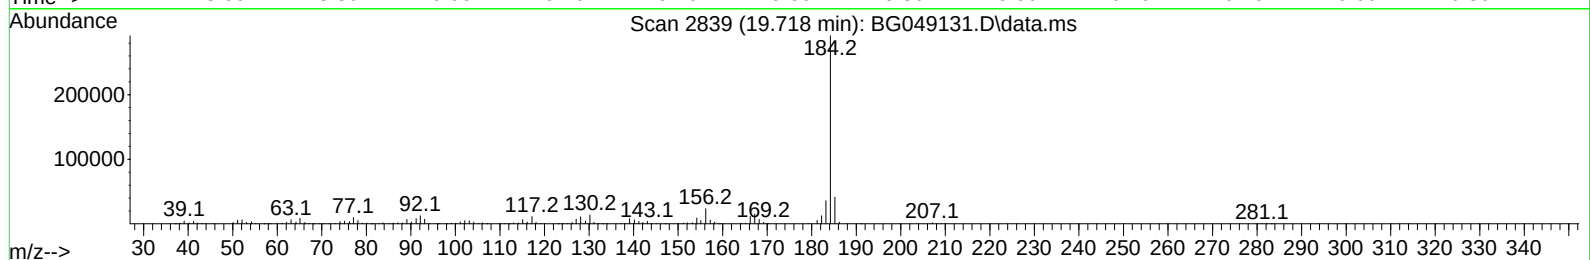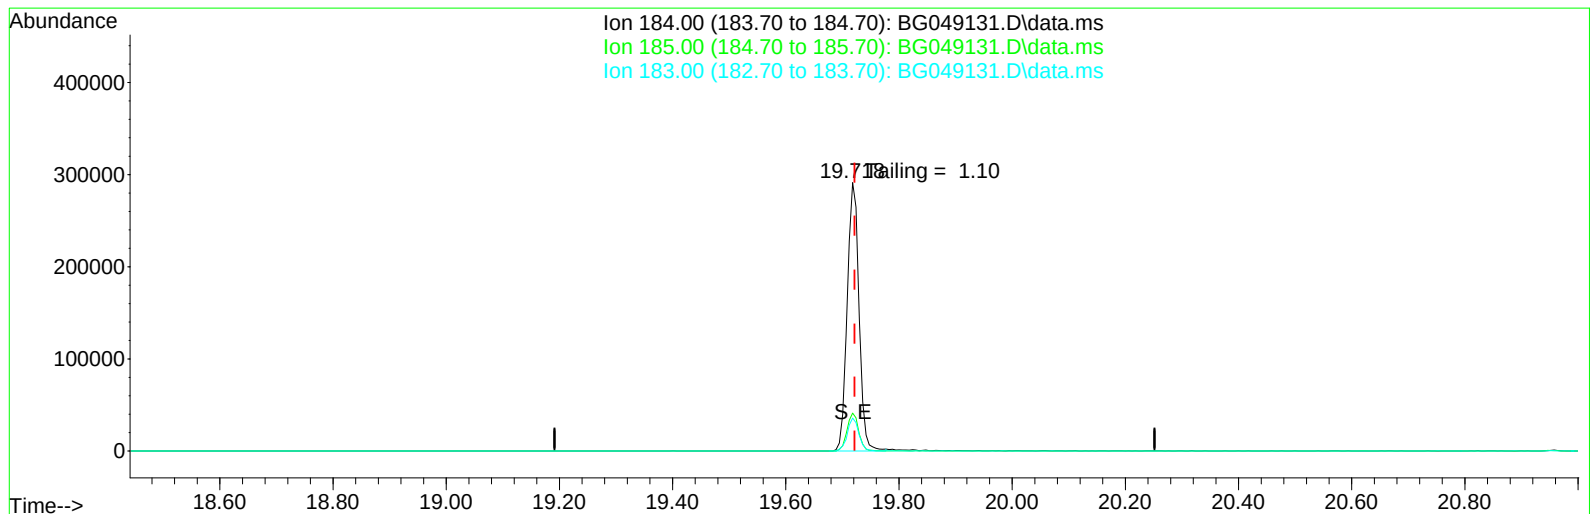

TIC: BG049131.D\data.ms

(77) Benzidine

19.718min (-0.003) 5844.45 ng m




response 423850

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.16
183.00	11.70	12.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG062921\
 Data File : BG049131.D
 Acq On : 29 Jun 2021 11:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 29 12:45:29 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG061121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 24 11:02:36 2021
 Response via : Initial Calibration

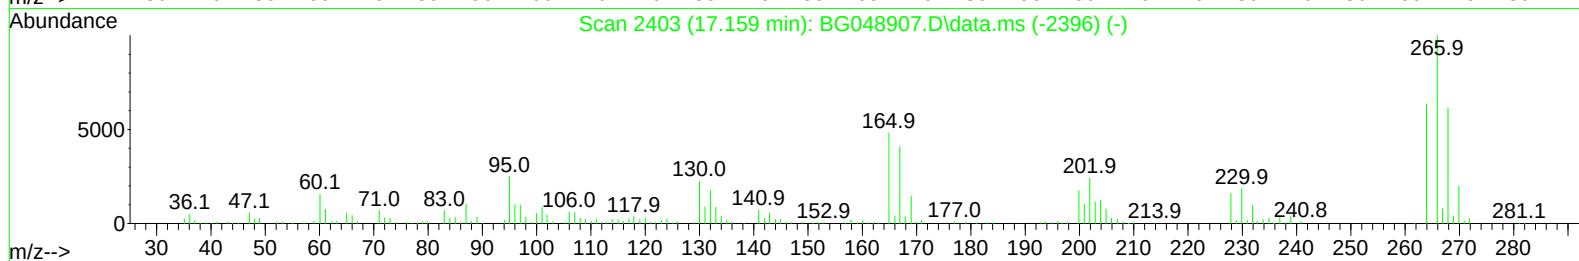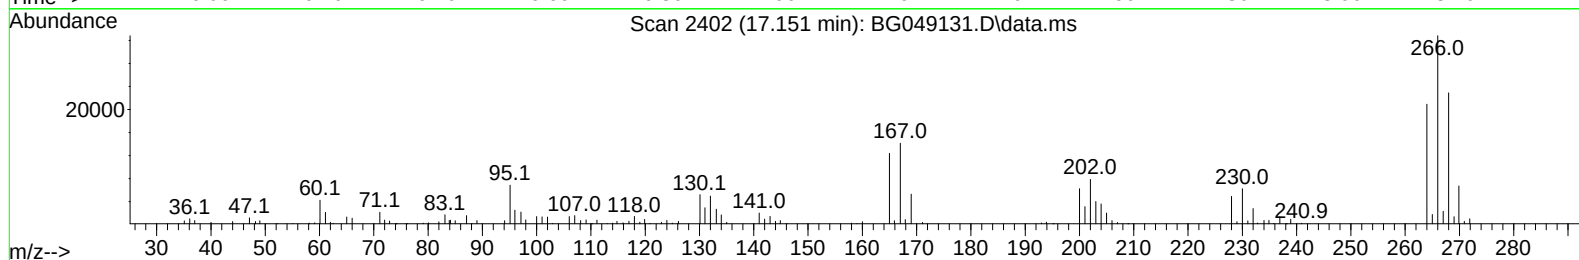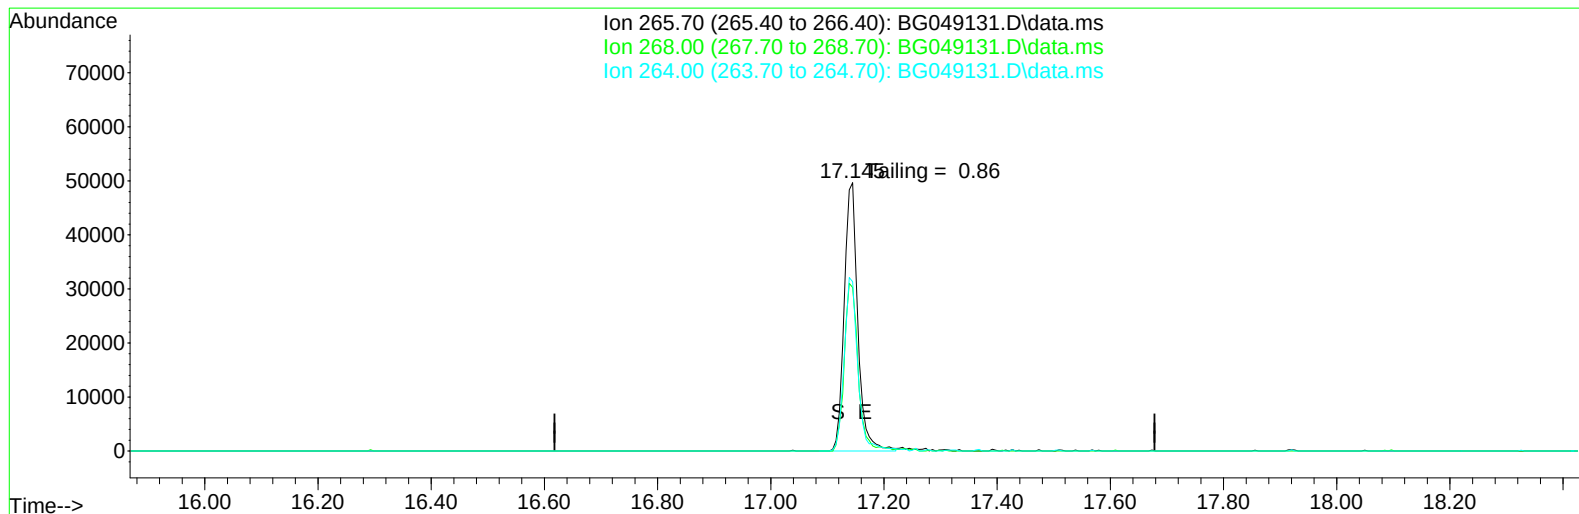

TIC: BG049131.D\data.ms

(70) Pentachlorophenol (C)

17.148min (-17.148) 0.00 ng

response 0

Ion	Exp%	Act%
265.70	100.00	0.00
268.00	61.20	0.00#
264.00	61.30	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/29/2021	BNA_G	BG049131.D
Compound Name	Response	Retention Time
DDT	228990	20.95
DDD	1238	20.5
DDE	508	20.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1746	230736	0.76

Instrument :
BNA_G
ClientSampleId :
DFTPP