

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG063016\
 Data File : BG022743.D
 Acq On : 1 Jul 2016 1:40
 Operator : UM/SJ
 Sample : H3759-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHP6

Quant Time: Jul 01 03:38:53 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 01 03:35:17 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	115883	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	524166	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	412494	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	1023462	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1152910	20.00	ng/ul	0.00
83) Perylene-d12	25.22	264	1158629	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	6567	3.17	ng/uL	0.00
5) Phenol-d5	7.31	99	401115	32.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	251001	36.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	269867	33.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	329201	34.77	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	142597	34.12	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	176930	35.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	346680	32.88	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	433583	48.57	ng/ul	0.00
43) Dimethylphthalate-d6	14.20	166	1251910	37.36	ng/ul	0.00
46) Acenaphthylene-d8	14.50	160	1387331	36.12	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	176101	33.47	ng/ul	0.00
57) Fluorene-d10	15.79	176	1164860	36.69	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	206020	31.30	ng/ul	0.00
70) Anthracene-d10	17.66	188	1687144	35.47	ng/ul	0.00
76) Pyrene-d10	19.94	212	1988492	36.10	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	2017984	36.66	ng/ul	0.00

Target Compounds


						Qvalue
6) Phenol	7.33	94	13198	1.06	ng/ul#	23
44) Dimethylphthalate	14.24	163	325383	9.51	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG063016\
Data File : BG022743.D
Acq On : 1 Jul 2016 1:40
Operator : UM/SJ
Sample : H3759-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHP6

Quant Time: Jul 01 03:38:53 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 01 03:35:17 2016
Response via : Initial Calibration

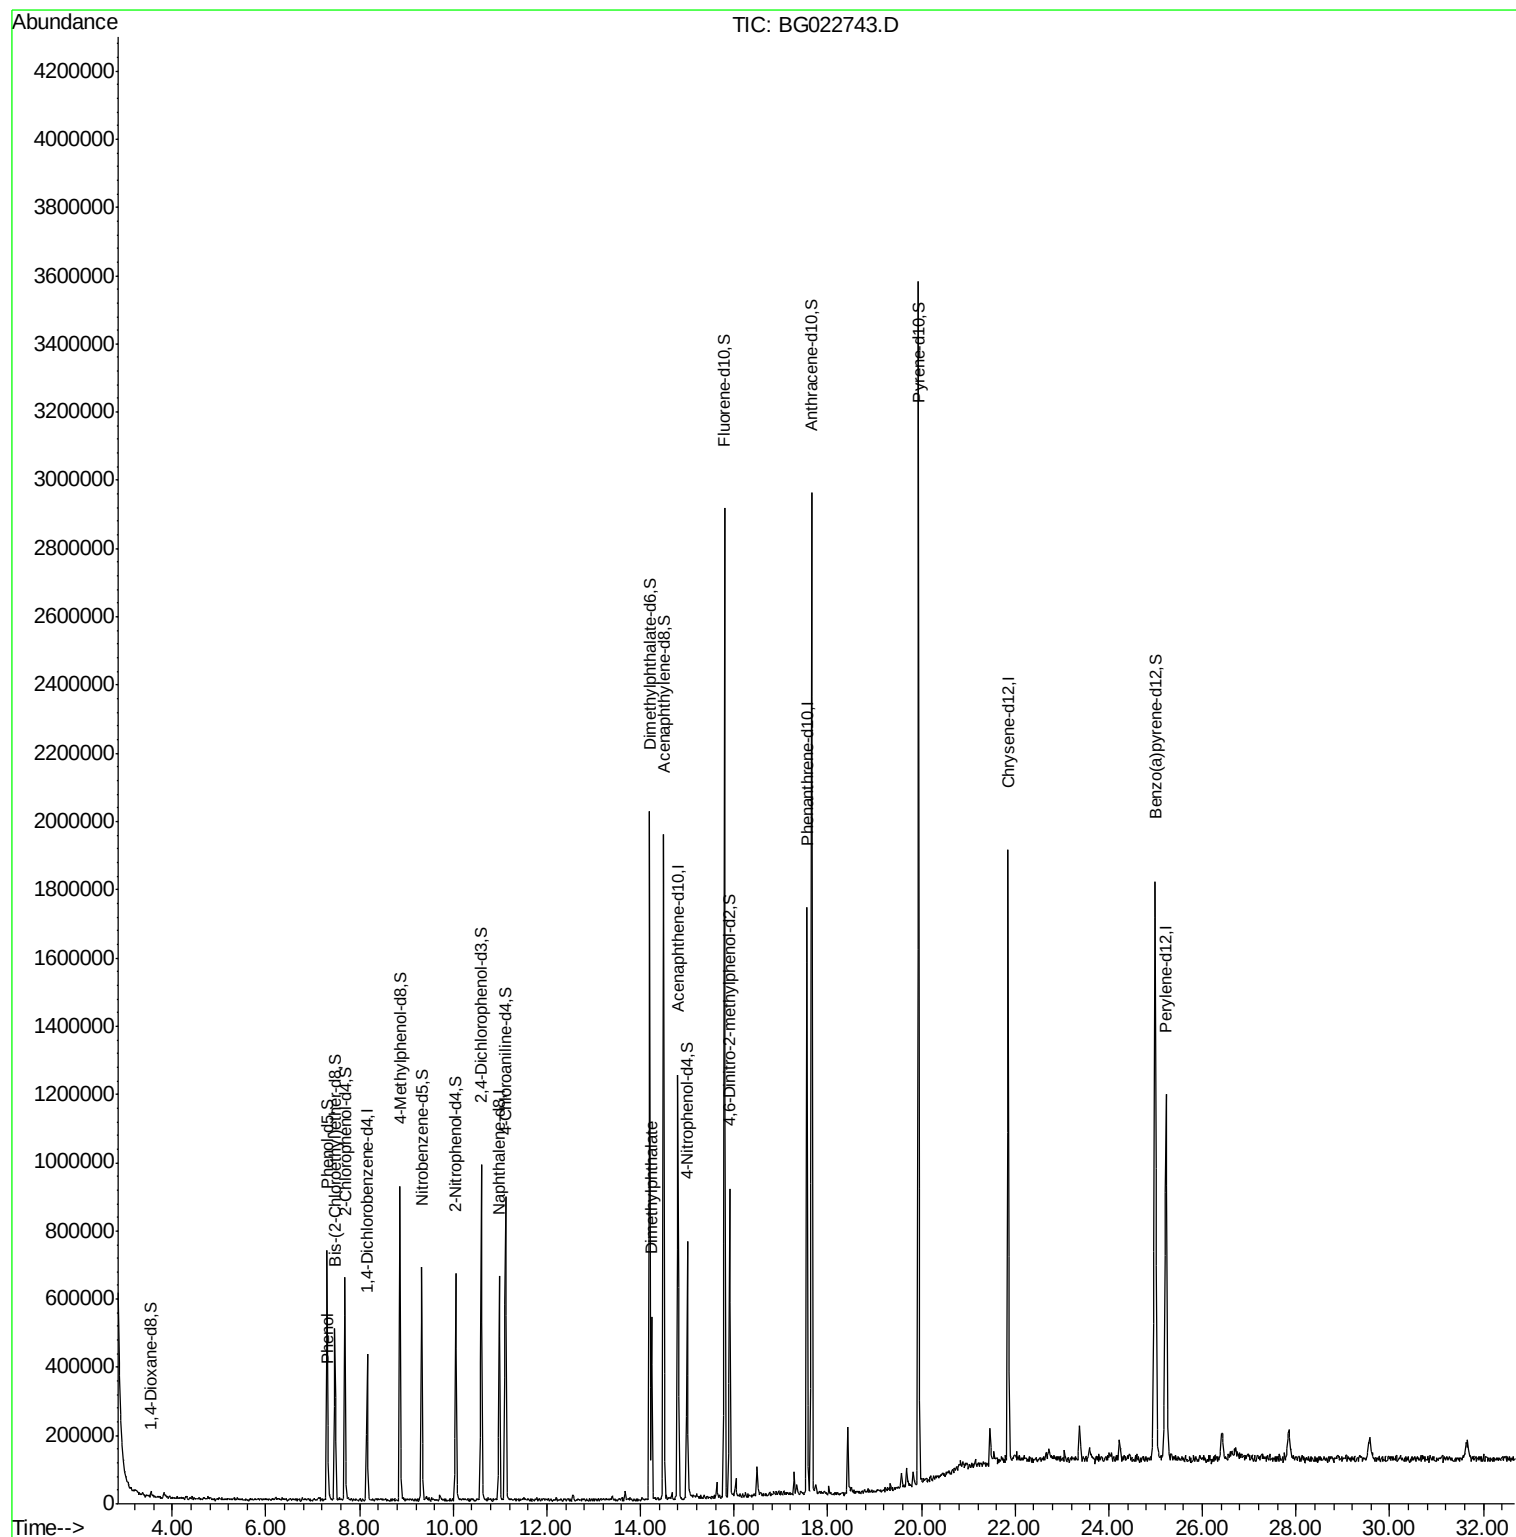

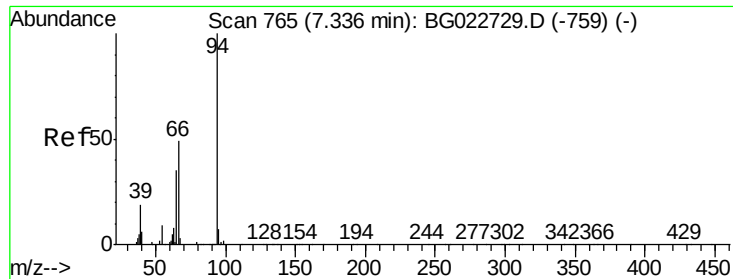

#6

Phenol

Concen: 1.06 ng/ul

RT: 7.33 min Scan# 765

Delta R.T. -0.00 min

Lab File: BG022743.D

Acq: 1 Jul 2016 1:40

Instrument :

BNA_G

ClientSampleId :

BDHP6


Tgt Ion: 94 Resp: 13198

Ion Ratio Lower Upper




94 100

65 45.3 16.8 25.2#

66 79.1 22.6 33.8#

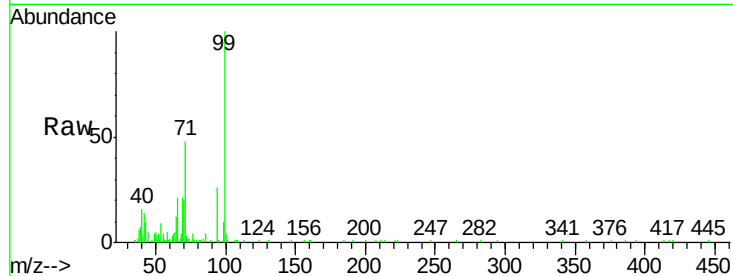

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

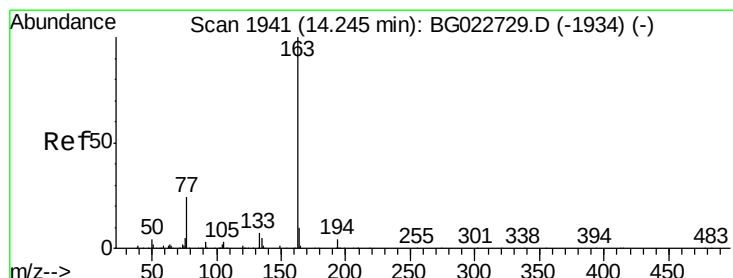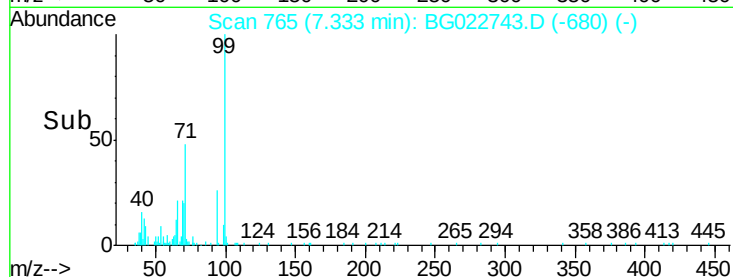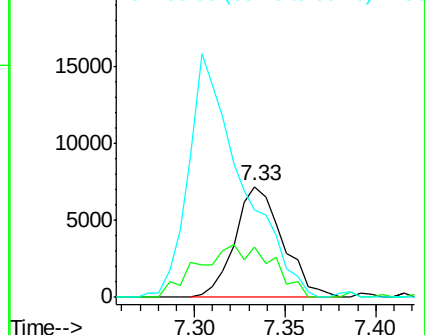

#44

Dimethylphthalate

Concen: 9.51 ng/ul

RT: 14.24 min Scan# 1941

Delta R.T. -0.00 min

Lab File: BG022743.D

Acq: 1 Jul 2016 1:40


Tgt Ion:163 Resp: 325383

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 10.3 8.8 13.2

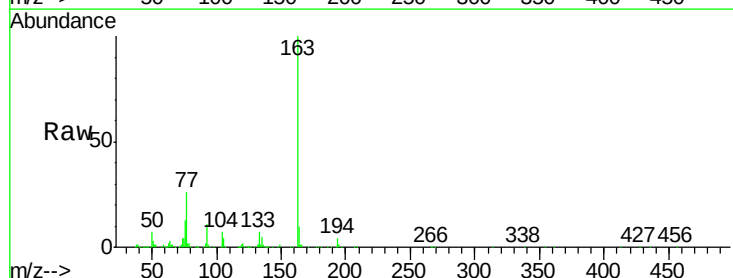

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

