

Data Path : Z:\HPCHEM1\BNA G\DATA\BG063016\
 Data File : BG022731.D
 Acq On : 30 Jun 2016 17:41
 Operator : UM/SJ
 Sample : H3759-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHM4

Manual Integrations

sohil
 7/1/2016 7:04:49 PM

Quant Time: Jul 01 04:08:38 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 01 03:35:17 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	104463	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	493719	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	386867	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	983682m	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1100802	20.00	ng/ul	0.00
83) Perylene-d12	25.22	264	1033252	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	1504	0.80	ng/uL	0.00
5) Phenol-d5	7.31	99	103420	9.41	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	242227	39.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	224930	30.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	181465	21.26	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	149003	37.85	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	183450	38.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	340039	34.24	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	21514	2.56	ng/ul	0.00
43) Dimethylphthalate-d6	14.19	166	1259300	40.07	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	1370433	38.05	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	47781m	9.68	ng/ul	0.00
57) Fluorene-d10	15.79	176	1185151	39.80	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	238136m	37.64	ng/ul	0.00
70) Anthracene-d10	17.66	188	1820893m	39.83	ng/ul	0.00
76) Pyrene-d10	19.94	212	2114022	40.20	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	2117925	43.14	ng/ul	0.00

Target Compounds					Ovalue
73) Di-n-butylphthalate	18.51	149	99489m	2.03	ng/ul

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG063016\
Data File : BG022731.D
Acq On : 30 Jun 2016 17:41
Operator : UM/SJ
Sample : H3759-01
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDHM4

Manual Integrations

sohil
7/1/2016 7:04:49 PM

Quant Time: Jul 01 04:08:38 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 01 03:35:17 2016
Response via : Initial Calibration

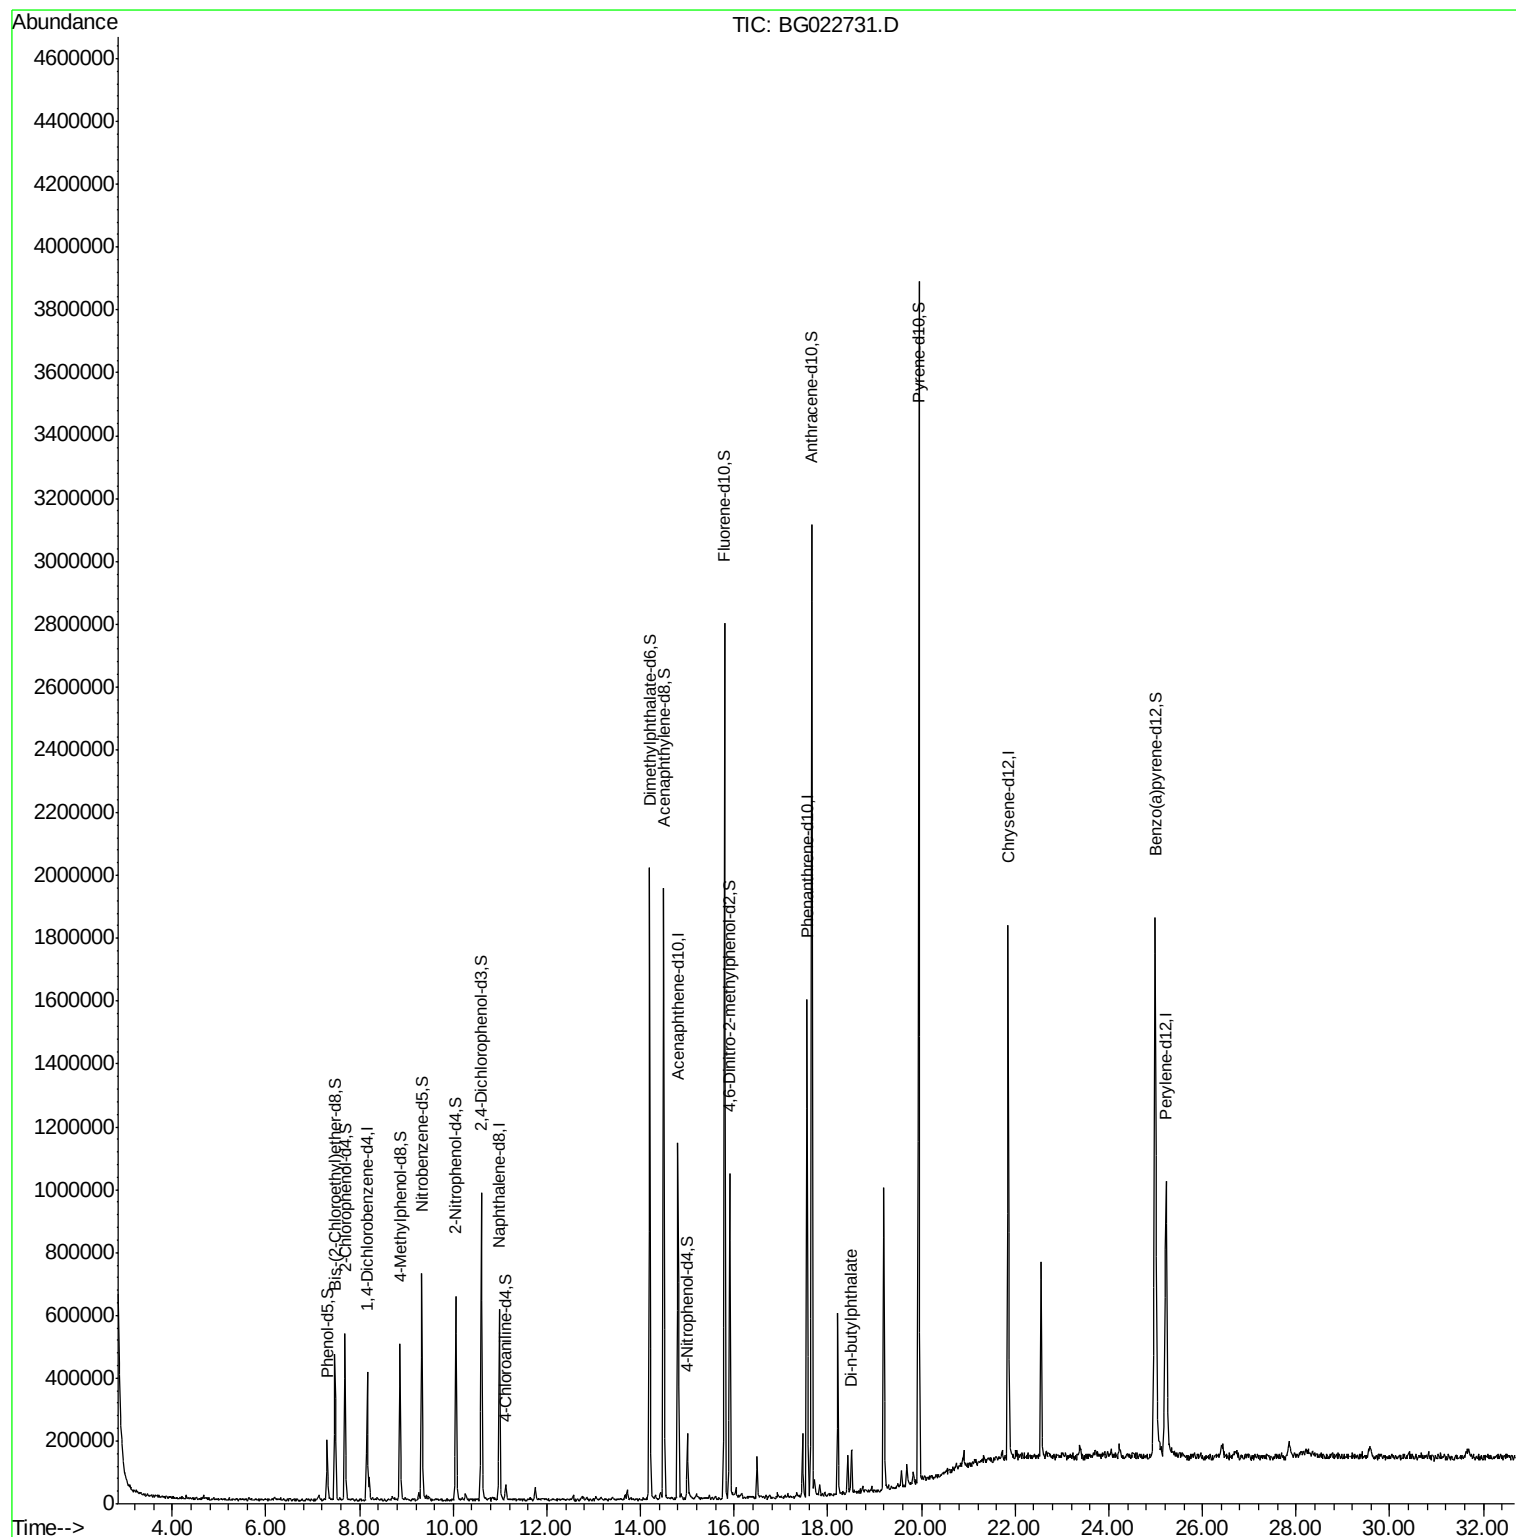

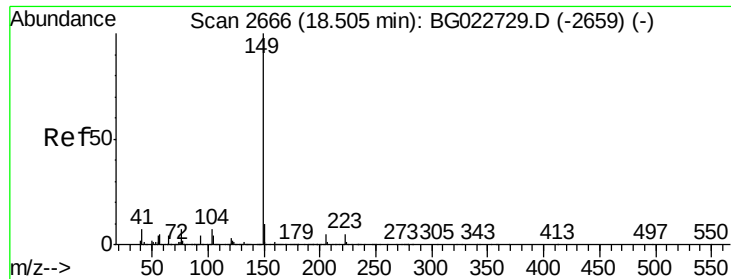

#73
 Di-n-butylphthalate
 Concen: 2.03 ng/ul m
 RT: 18.51 min Scan# 2667
 Delta R.T. 0.00 min
 Lab File: BG022731.D
 Acq: 30 Jun 2016 17:41

Instrument :
 BNA_G
 ClientSampleId :
 BDHM4

Tot Ion	Ratio	Lower	Upper
149	100		
150	9.8	7.1	10.7
104	5.8	3.3	4.9

Manual Integrations

sohil
 7/1/2016 7:04:49 PM

