

Data Path : Z:\HPCHEM1\BNA G\DATA\BG063016\
 Data File : BG022736.D
 Acq On : 30 Jun 2016 21:00
 Operator : UM/SJ
 Sample : H3759-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHN8

Manual Integrations

sohil
 7/1/2016 7:05:03 PM

Quant Time: Jul 01 04:27:19 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 01 03:35:17 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	103196	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	477580	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	368349	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	926531	20.00	ng/ul	0.00
75) Chrysene-d12	21.86	240	1045583	20.00	ng/ul	0.00
83) Perylene-d12	25.22	264	1079171	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	7839	4.24	ng/uL	0.00
5) Phenol-d5	7.31	99	444628	40.96	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	259735	42.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.68	132	293647	40.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	338897	40.19	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	156224	41.02	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	188860	41.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	367893	38.30	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	448985	55.20	ng/ul	0.00
43) Dimethylphthalate-d6	14.19	166	1284630	42.93	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	1435535	41.86	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	191438m	40.74	ng/ul	0.00
57) Fluorene-d10	15.79	176	1209325	42.65	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	219662	36.86	ng/ul	0.00
70) Anthracene-d10	17.66	188	1793319	41.64	ng/ul	0.00
76) Pyrene-d10	19.93	212	2075026	41.54	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	2140122m	41.74	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	14.24	163	290756	9.52 ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG063016\
Data File : BG022736.D
Acq On : 30 Jun 2016 21:00
Operator : UM/SJ
Sample : H3759-08
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDHN8

Manual Integrations

sohil
7/1/2016 7:05:03 PM

Quant Time: Jul 01 04:27:19 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 01 03:35:17 2016
Response via : Initial Calibration

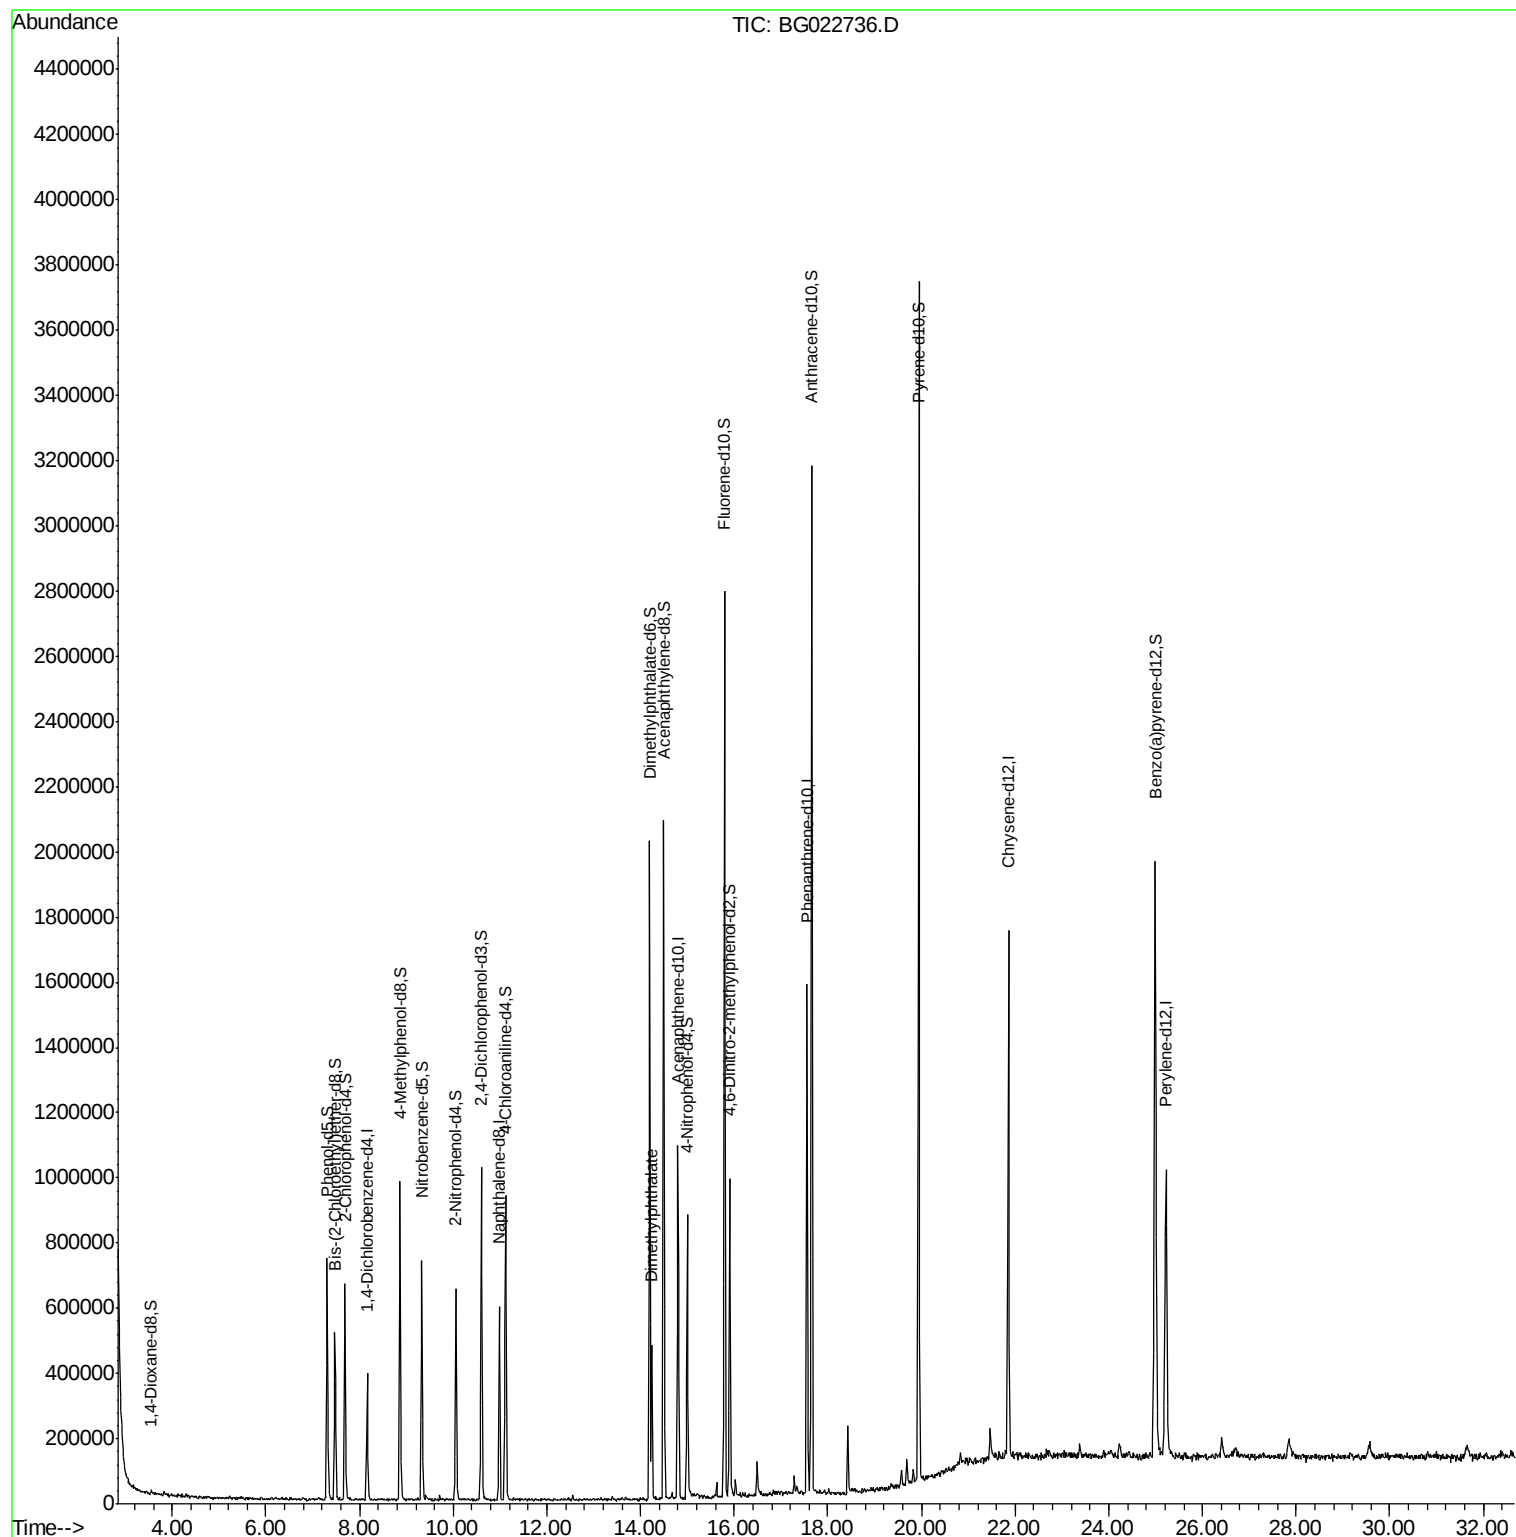

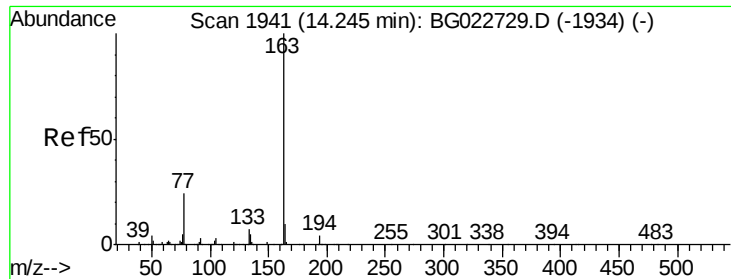

#44
 Dimethylphthalate
 Concen: 9.52 ng/ul
 RT: 14.24 min Scan# 1941
 Delta R.T. -0.00 min
 Lab File: BG022736.D
 Acq: 30 Jun 2016 21:00

Instrument :
 BNA_G
 ClientSampleId :
 BDHN8

Tot Ion	Ratio	Resp	Lower	Upper
163	100	290756		
194	4.5		3.4	5.2
164	8.4		8.8	13.2#

Manual Integrations

sohil
 7/1/2016 7:05:03 PM

