

Data Path : Z:\HPCHEM1\BNA G\DATA\BG063016\
 Data File : BG022743.D
 Acq On : 1 Jul 2016 1:40
 Operator : UM/SJ
 Sample : H3759-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHP6

Quant Time: Jul 01 05:00:43 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 01 03:35:17 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	115883	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	524166	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	412494	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	1023462	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1152910	20.00	ng/ul	0.00
83) Perylene-d12	25.22	264	1158629	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	6567	3.17	ng/uL	0.00
5) Phenol-d5	7.31	99	401115	32.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	251001	36.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	269867	33.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	329201	34.77	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	142597	34.12	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	176930	35.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	346680	32.88	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	433583	48.57	ng/ul	0.00
43) Dimethylphthalate-d6	14.20	166	1251910	37.36	ng/ul	0.00
46) Acenaphthylene-d8	14.50	160	1387331	36.12	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	176101	33.47	ng/ul	0.00
57) Fluorene-d10	15.79	176	1164860	36.69	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	206020	31.30	ng/ul	0.00
70) Anthracene-d10	17.66	188	1687144	35.47	ng/ul	0.00
76) Pyrene-d10	19.94	212	1988492	36.10	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	2017984	36.66	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.24	163	325383	9.51	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG063016\
Data File : BG022743.D
Acq On : 1 Jul 2016 1:40
Operator : UM/SJ
Sample : H3759-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHP6

Quant Time: Jul 01 05:00:43 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 01 03:35:17 2016
Response via : Initial Calibration

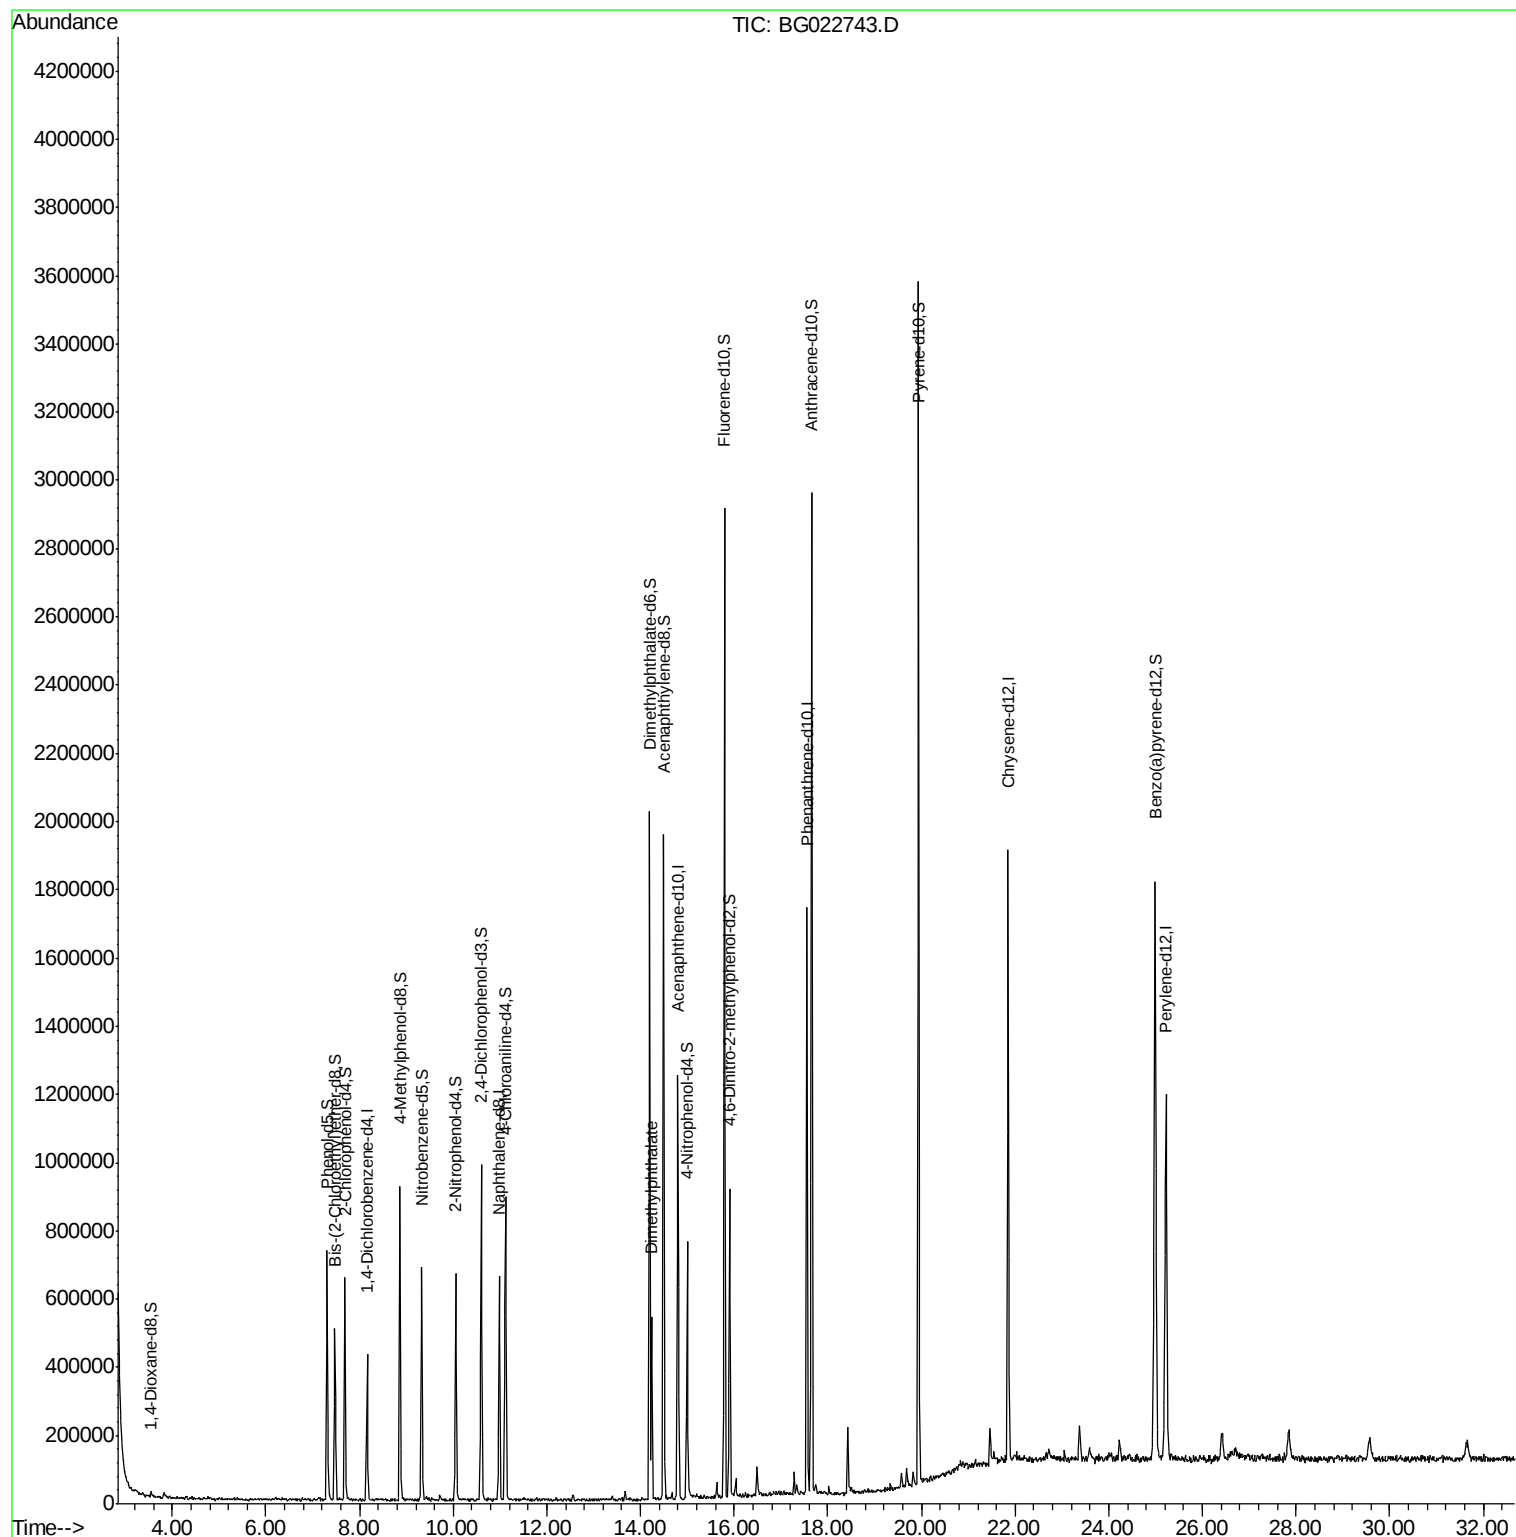


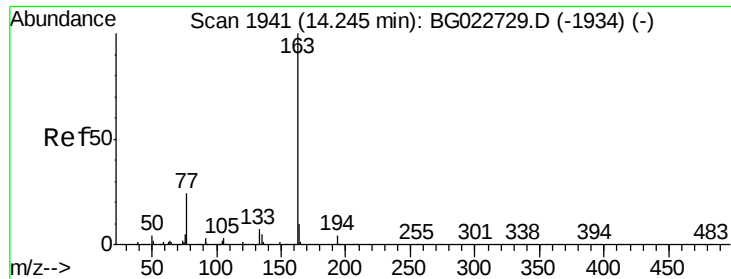

#44
 Dimethylphthalate
 Concen: 9.51 ng/ul
 RT: 14.24 min Scan# 1941
 Delta R.T. -0.00 min
 Lab File: BG022743.D
 Acq: 1 Jul 2016 1:40

Instrument :
 BNA_G
 ClientSampleId :
 BDHP6

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.2
164	10.3	8.8	13.2

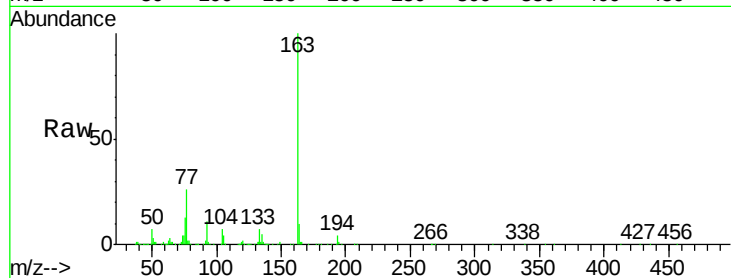

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

