

Data Path : Z:\HPCHEM1\BNA G\DATA\BG063017\
 Data File : BG027757.D
 Acq On : 30 Jun 2017 17:08
 Operator : SJ/JU
 Sample : PB100337BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB100337BL

Quant Time: Jul 01 00:49:09 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 19:26:37 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.48	152	31204	20.00	ng	0.00
21) Naphthalene-d8	11.29	136	157700	20.00	ng	0.00
38) Acenaphthene-d10	15.07	164	96070	20.00	ng	0.00
63) Phenanthrene-d10	17.82	188	254167	20.00	ng	0.00
75) Chrysene-d12	22.18	240	265063	20.00	ng	0.00
86) Perylene-d12	25.79	264	257012	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.06	112	268729	132.62	ng	0.00
7) Phenol-d6	7.62	99	370322	119.63	ng	0.00
23) Nitrobenzene-d5	9.64	82	218544	77.25	ng	0.00
41) 2,4,6-Tribromophenol	16.56	330	178842	135.72	ng	0.00
44) 2-Fluorobiphenyl	13.69	172	564615	83.94	ng	0.00
78) Terphenyl-d14	20.40	244	1018657	90.10	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG063017\
Data File : BG027757.D
Acq On : 30 Jun 2017 17:08
Operator : SJ/JU
Sample : PB100337BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB100337BL

Quant Time: Jul 01 00:49:09 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 19:26:37 2017
Response via : Initial Calibration

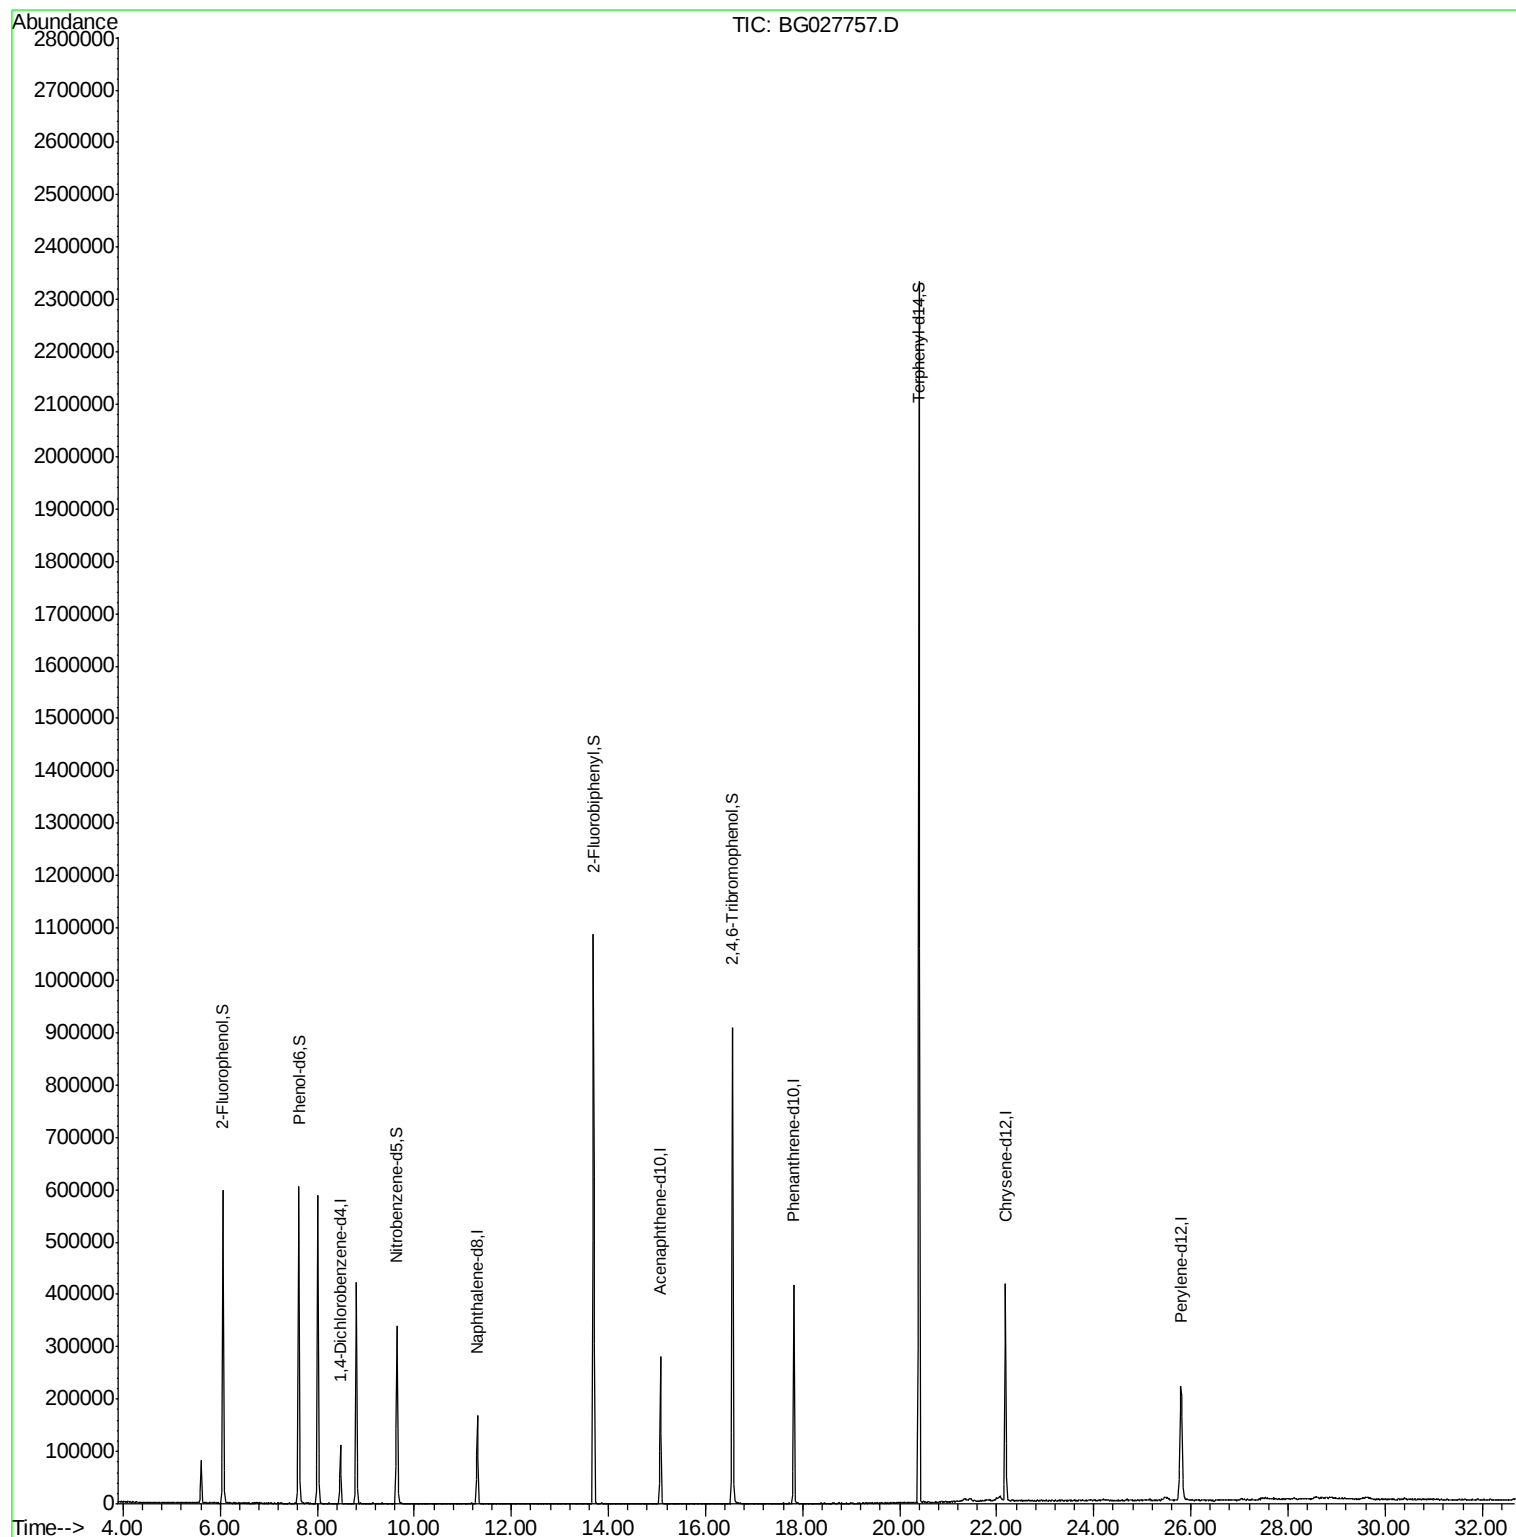

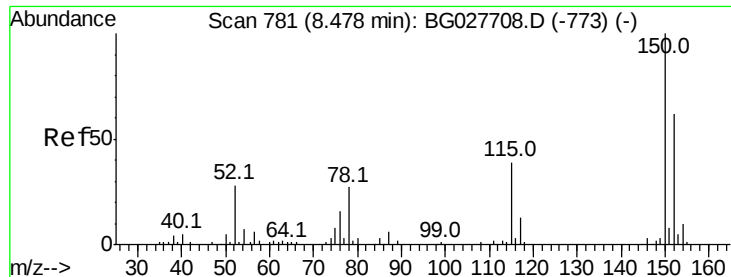

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.48 min Scan# 781

Delta R.T. 0.00 min

Lab File: BG027757.D

Acq: 30 Jun 2017 17:08

Instrument :

BNA_G

ClientSampleId :

PB100337BL


Tot Ion:152 Resp: 31204

Ion Ratio Lower Upper

152 100

150 164.6 114.0 171.0




115 68.9 48.1 72.1

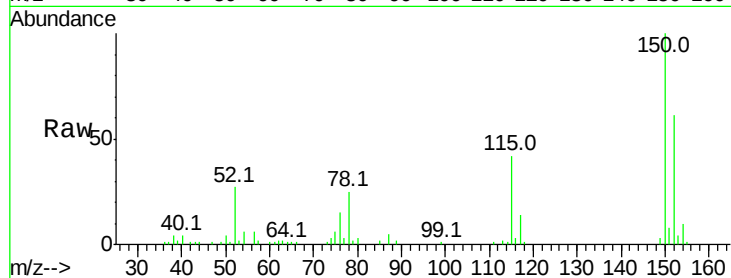

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

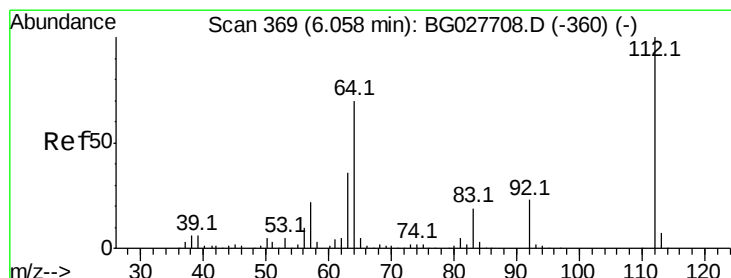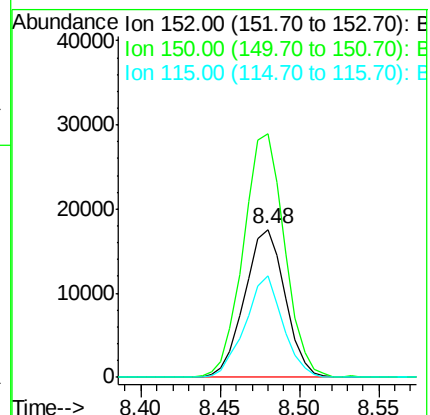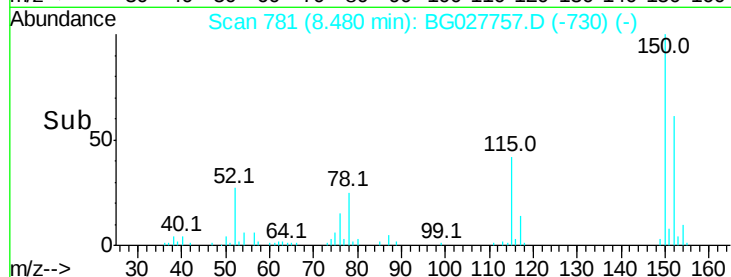

#5

2-Fluorophenol

Concen: 132.62 ng

RT: 6.06 min Scan# 369

Delta R.T. 0.00 min

Lab File: BG027757.D

Acq: 30 Jun 2017 17:08


Tgt Ion:112 Resp: 268729

Ion Ratio Lower Upper

112 100

64 70.7 61.8 92.6



63 36.3 37.2 55.8#

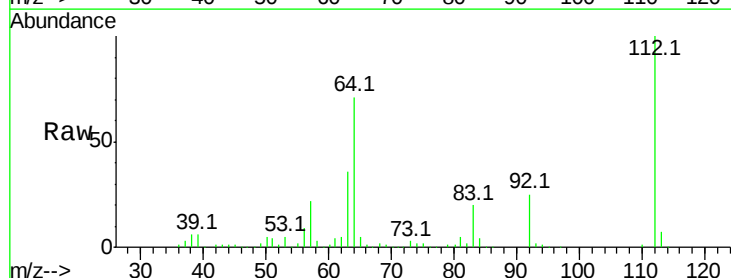

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

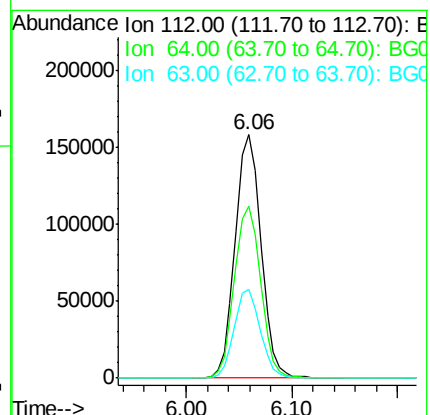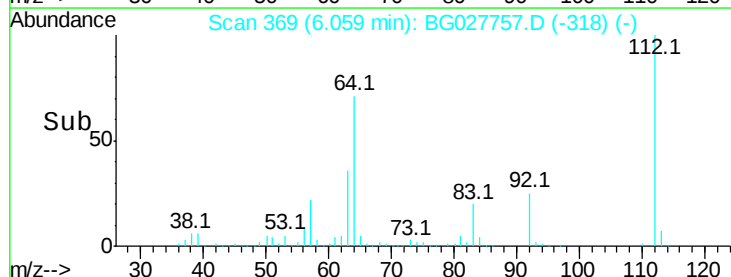



#7

Phenol-d6

Concen: 119.63 ng

RT: 7.62 min Scan# 634

Delta R.T. 0.00 min

Lab File: BG027757.D

Acq: 30 Jun 2017 17:08

Instrument :

BNA_G

ClientSampled :

PB100337BL


Tot Ion: 99 Resp: 370322

Ion Ratio Lower Upper




99 100

42 19.4 20.5 30.7#

71 32.7 37.6 56.4#

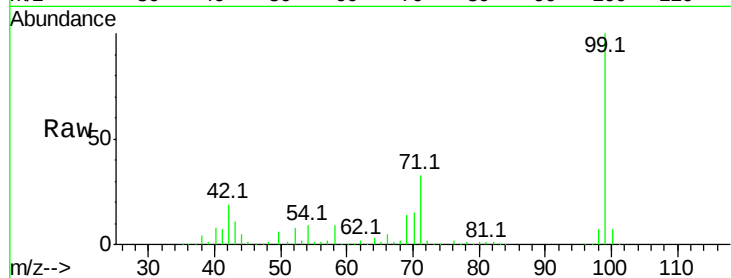

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

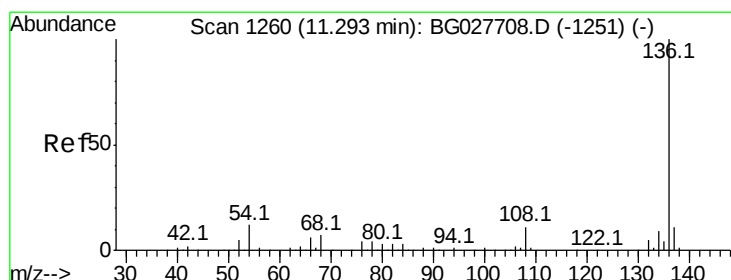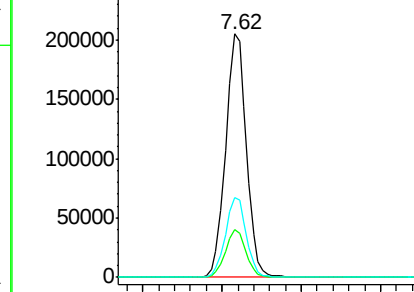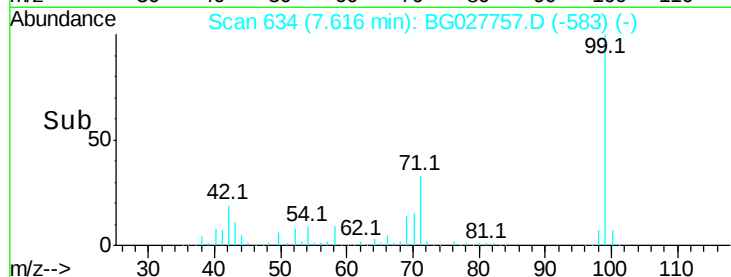

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.29 min Scan# 1260

Delta R.T. 0.00 min

Lab File: BG027757.D

Acq: 30 Jun 2017 17:08

Tgt Ion: 136 Resp: 157700


Ion Ratio Lower Upper

136 100



137 10.2 8.9 13.3


54 12.6 9.3 13.9

68 7.1 5.1 7.7

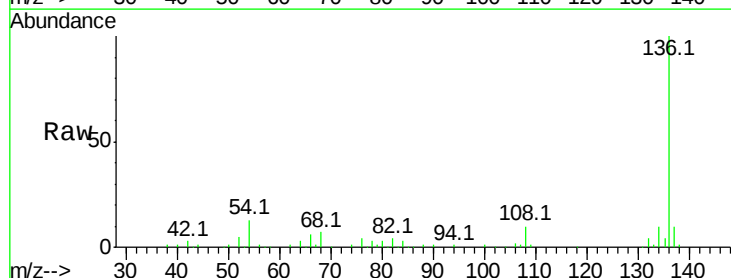

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

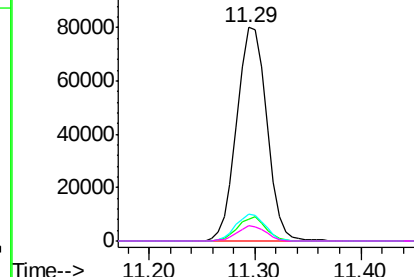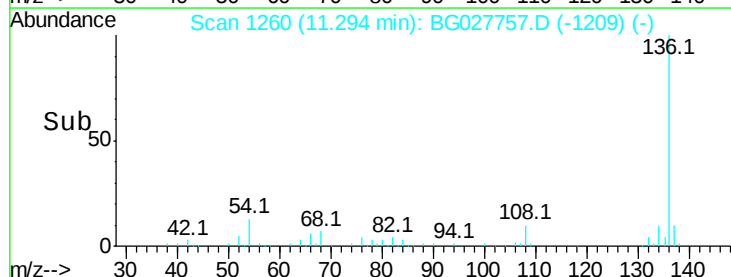


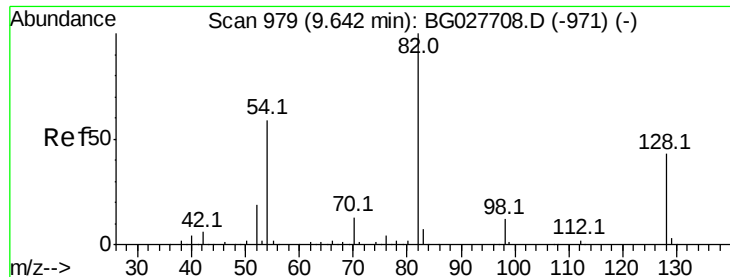




#23
Nitrobenzene-d5
Concen: 77.25 ng
RT: 9.64 min Scan# 979
Delta R.T. 0.00 min
Lab File: BG027757.D
Acq: 30 Jun 2017 17:08

Instrument :
BNA_G
ClientSampleId :
PB100337BL

Tot Ion	82	Resp	218544
Ion Ratio	Lower	Upper	
82	100		
128	43.3	26.4	39.6#
54	58.4	49.4	74.2

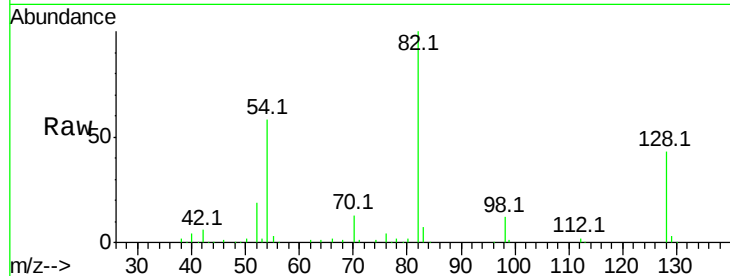


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

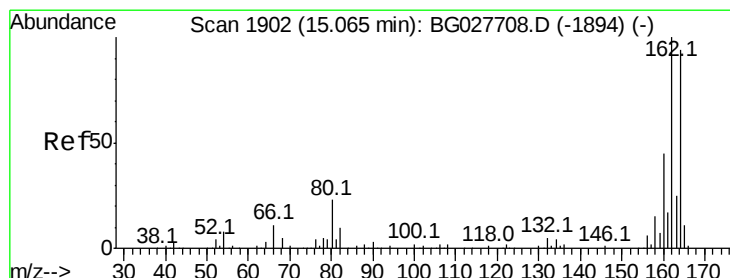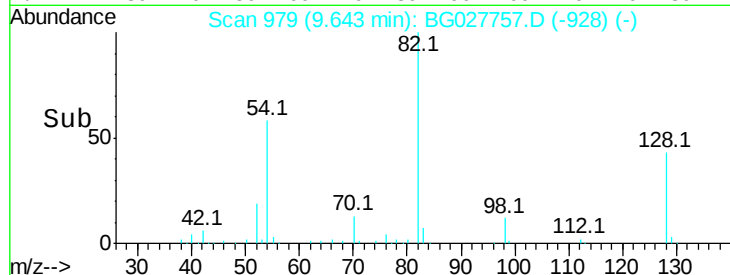
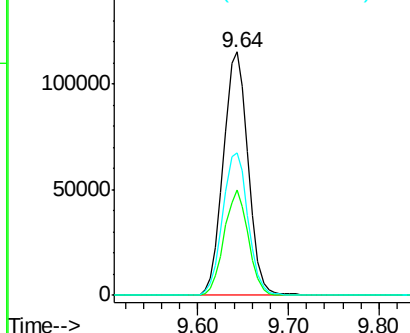



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 15.07 min Scan# 1903
Delta R.T. 0.01 min
Lab File: BG027757.D
Acq: 30 Jun 2017 17:08

Tgt Ion	164	Resp	96070
Ion Ratio	Lower	Upper	
164	100		
162	108.1	85.1	127.7
160	48.4	34.7	52.1

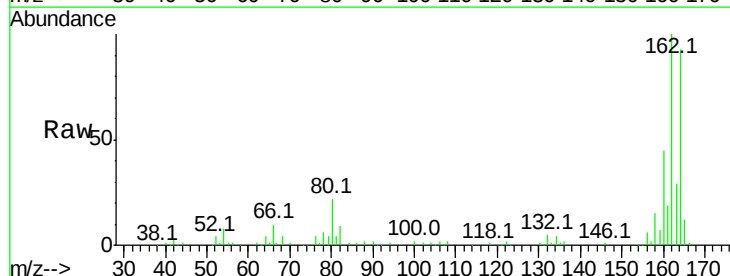

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

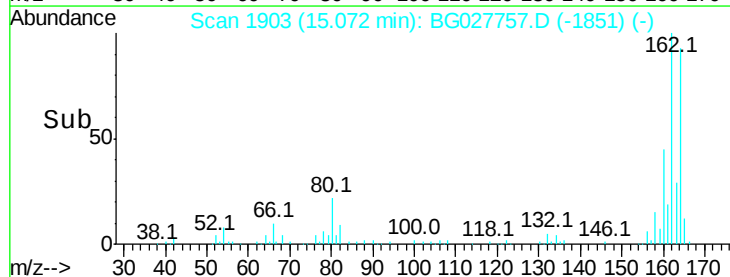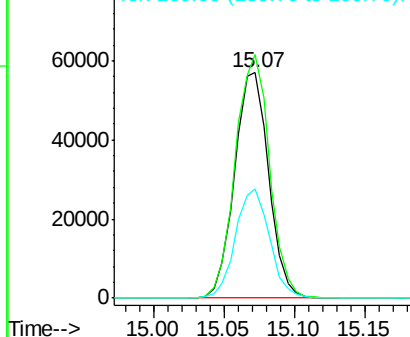


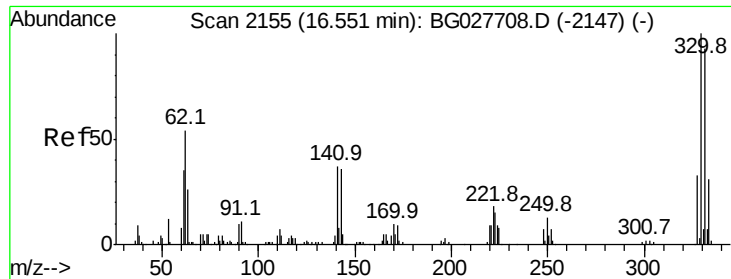




#41
 2,4,6-Tribromophenol
 Concen: 135.72 ng
 RT: 16.56 min Scan# 2156
 Delta R.T. 0.01 min
 Lab File: BG027757.D
 Acq: 30 Jun 2017 17:08

Instrument :
 BNA_G
 ClientSampleId :
 PB100337BL

Tot Ion:330 Resp: 178842
 Ion Ratio Lower Upper
 330 100
 332 94.7 77.3 115.9
 141 37.2 32.1 48.1

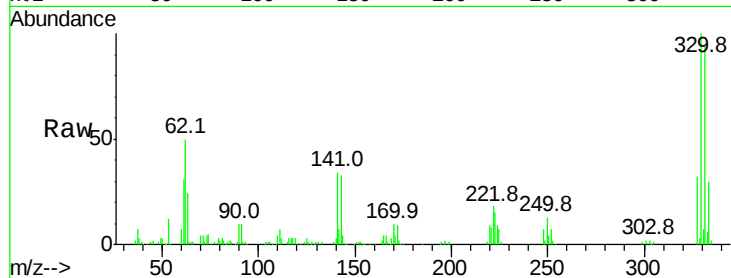


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

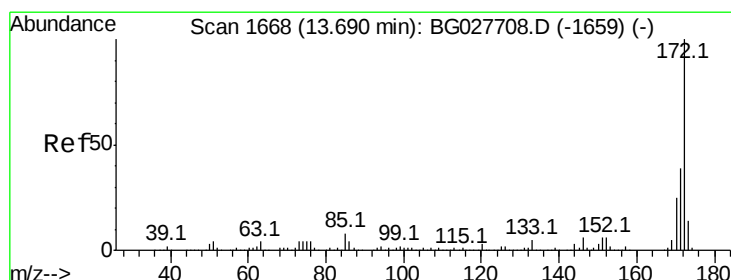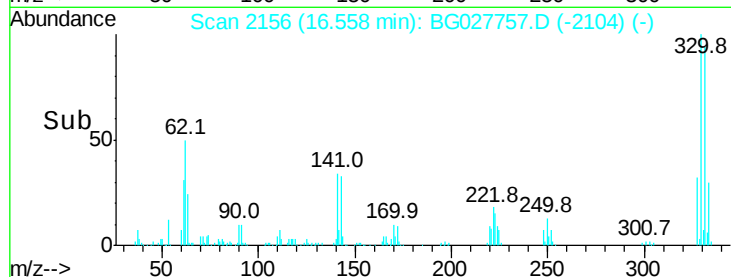
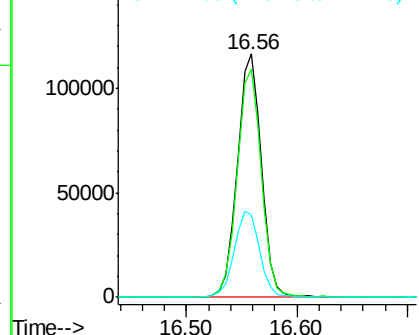



#44
 2-Fluorobiphenyl
 Concen: 83.94 ng
 RT: 13.69 min Scan# 1668
 Delta R.T. 0.00 min
 Lab File: BG027757.D
 Acq: 30 Jun 2017 17:08

Tgt Ion:172 Resp: 564615
 Ion Ratio Lower Upper
 172 100
 171 36.2 32.2 48.2
 170 24.0 21.8 32.6

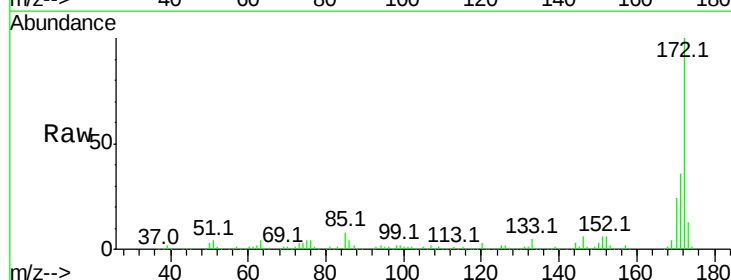

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

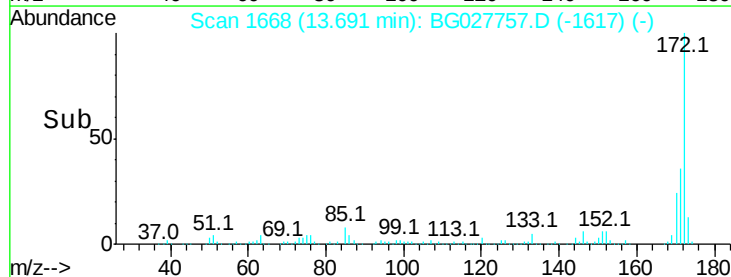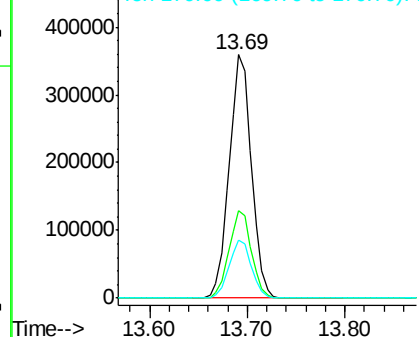

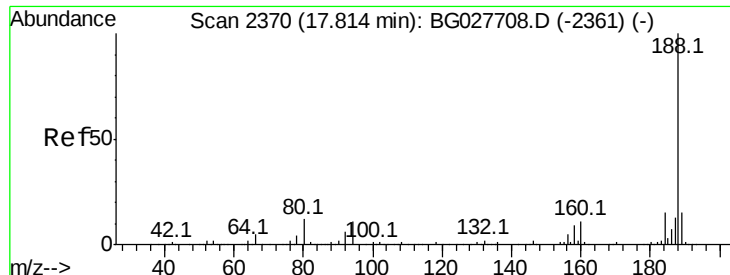

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.82 min Scan# 2370

Delta R.T. 0.00 min

Lab File: BG027757.D

Acq: 30 Jun 2017 17:08

Instrument :

BNA_G

ClientSampleId :

PB100337BL


Tot Ion:188 Resp: 254167

Ion Ratio Lower Upper

188 100

94 10.4 5.8 8.8#




80 12.8 7.5 11.3#

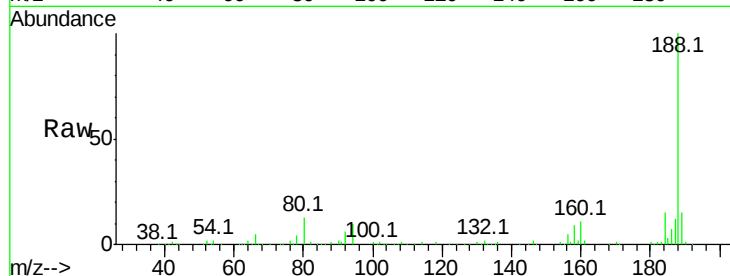

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

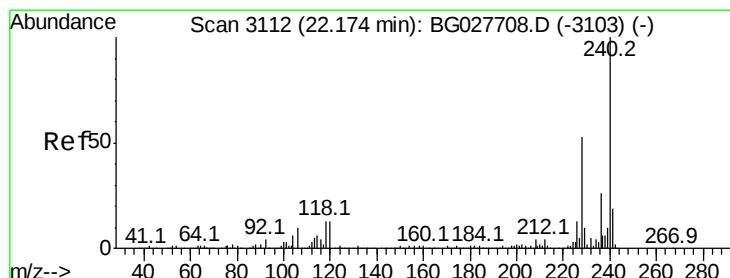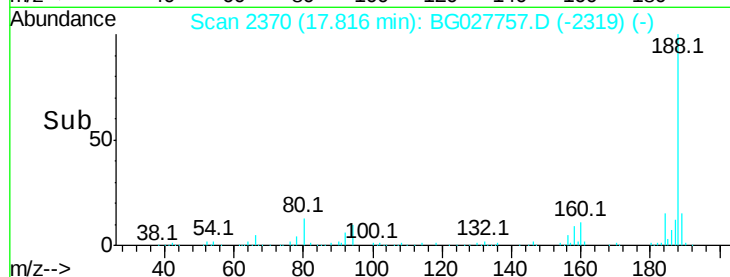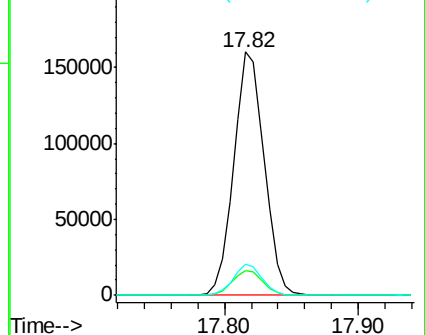

#75

Chrysene-d12

Concen: 20.00 ng

RT: 22.18 min Scan# 3113

Delta R.T. 0.01 min

Lab File: BG027757.D

Acq: 30 Jun 2017 17:08


Tgt Ion:240 Resp: 265063

Ion Ratio Lower Upper

240 100

120 13.1 5.7 8.5#



236 26.0 22.2 33.4

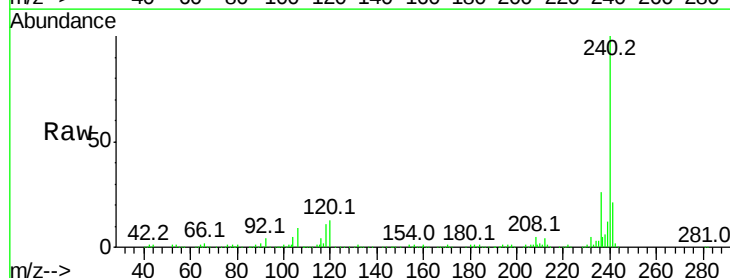


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

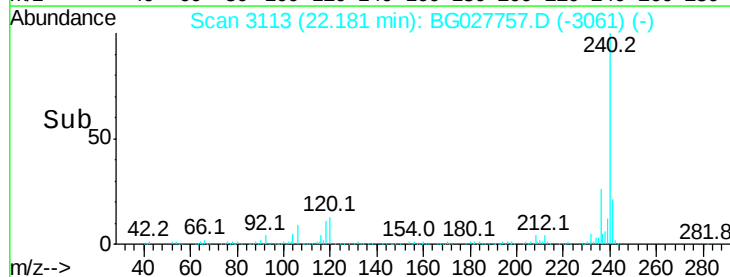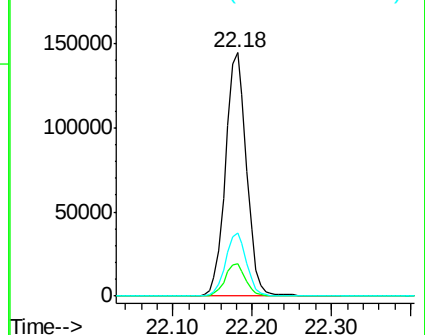

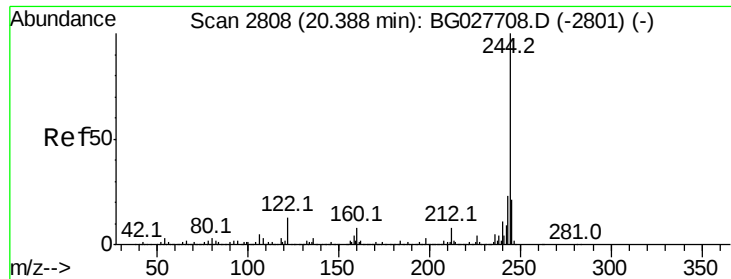

#78

Terphenyl-d14

Concen: 90.10 ng

RT: 20.40 min Scan# 2809

Delta R.T. 0.01 min

Lab File: BG027757.D

Acq: 30 Jun 2017 17:08

Instrument :

BNA_G

ClientSampleId :

PB100337BL


Tot Ion:244 Resp: 1018657

Ion Ratio Lower Upper

244 100

212 7.4 10.0 15.0#




122 12.0 8.6 12.8

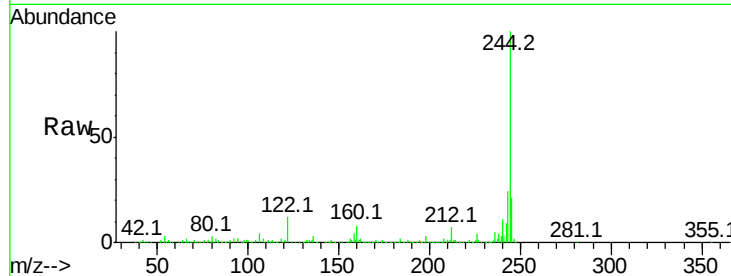

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

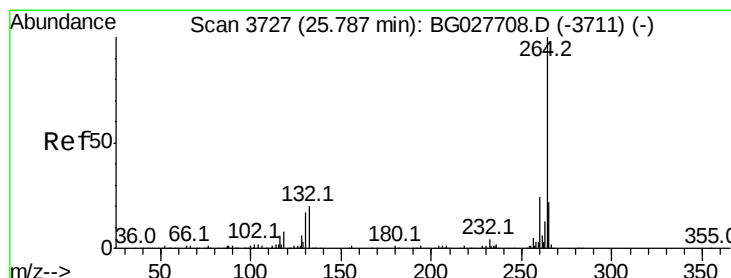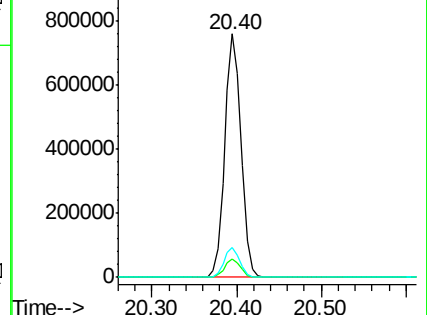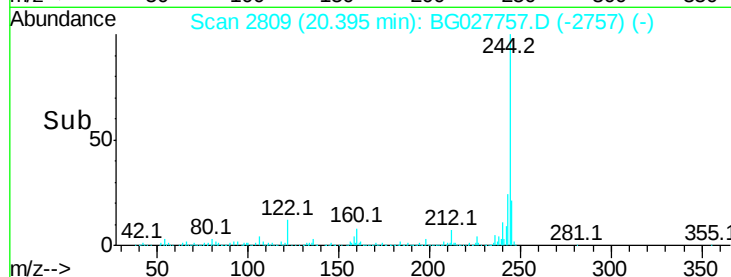

#86

Perylene-d12

Concen: 20.00 ng

RT: 25.79 min Scan# 3728

Delta R.T. 0.01 min

Lab File: BG027757.D

Acq: 30 Jun 2017 17:08


Tgt Ion:264 Resp: 257012

Ion Ratio Lower Upper

264 100

260 23.8 21.8 32.8

265 20.9 18.2 27.4

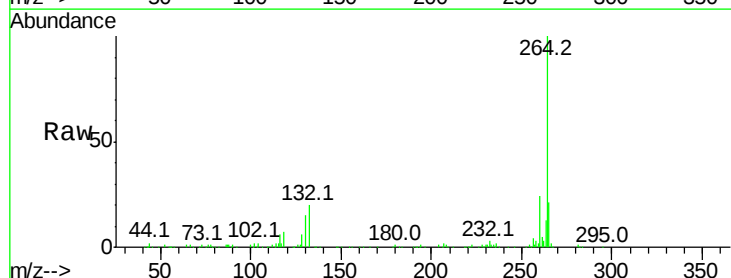

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

