


Data Path : Z:\HPCHEM1\BNA_G\Data\BG063017\
 Data File : BG027755.D
 Acq On : 30 Jun 2017 15:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 19:26:37 2017

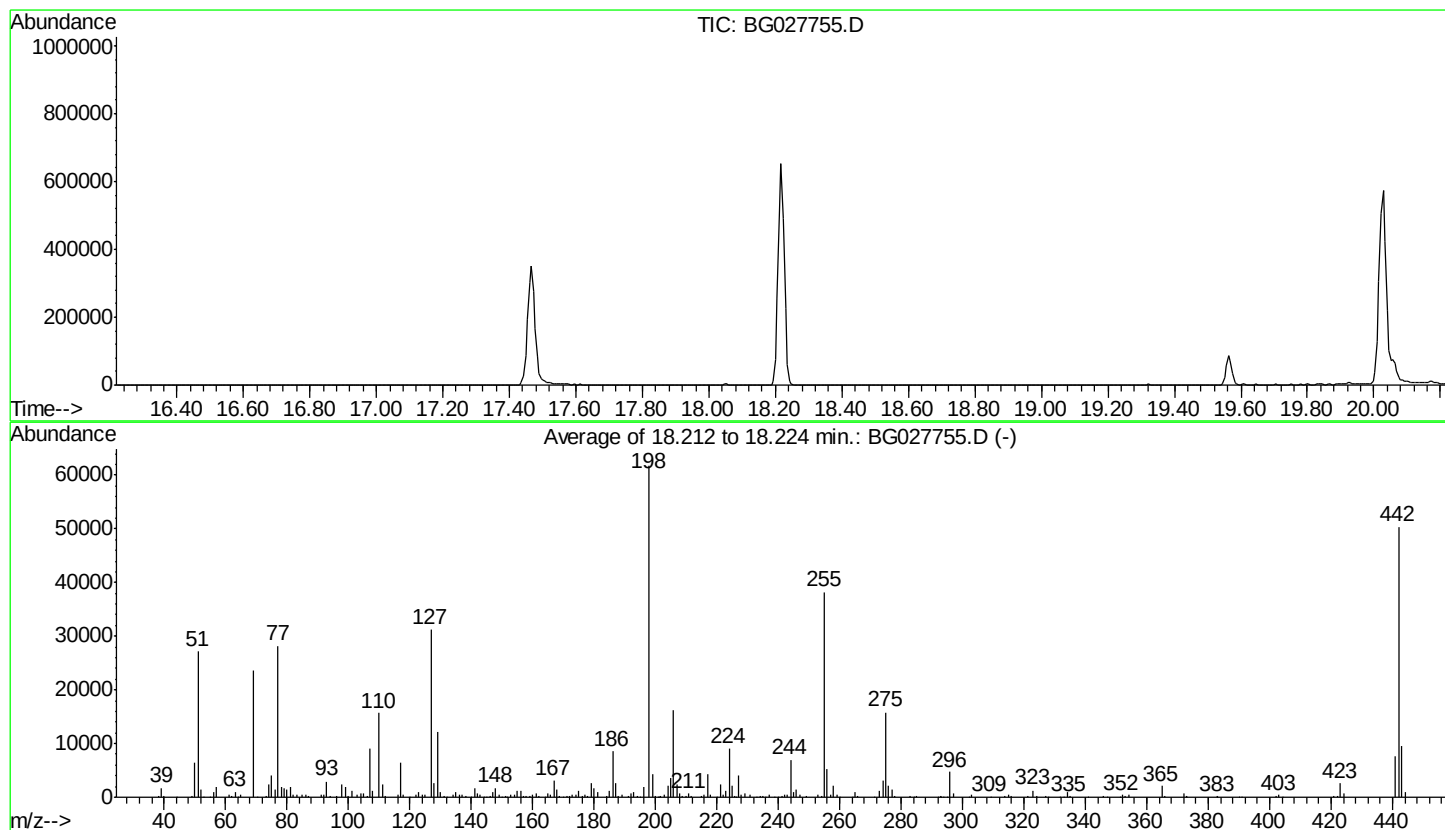

AutoFind: Scans 2438, 2439, 2440; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	27096	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.1	23562	PASS
70	69	0.00	2	0.3	59	PASS
127	198	10	80	50.5	31226	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	61776	PASS
199	198	5	9	6.8	4203	PASS
275	198	10	60	25.6	15835	PASS
365	198	1	100	3.4	2089	PASS
441	442	0.01	24	15.1	7607	PASS
442	198	50	100	81.6	50394	PASS
443	442	15	24	19.0	9584	PASS