
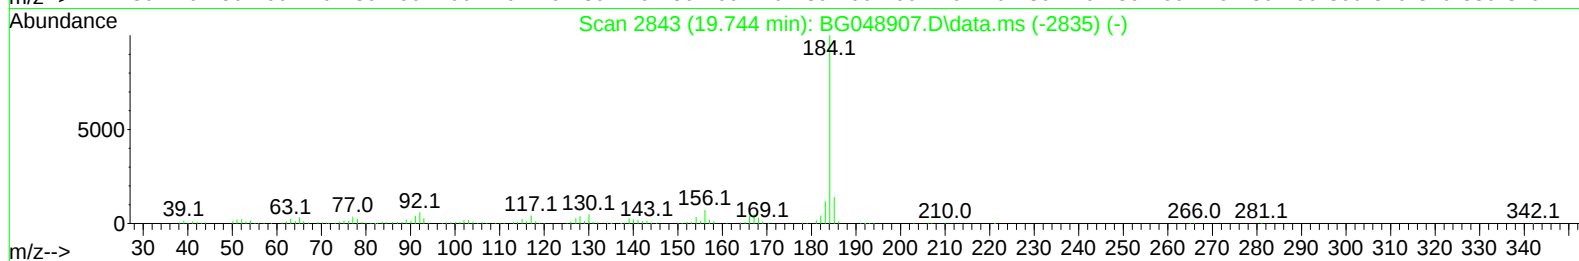
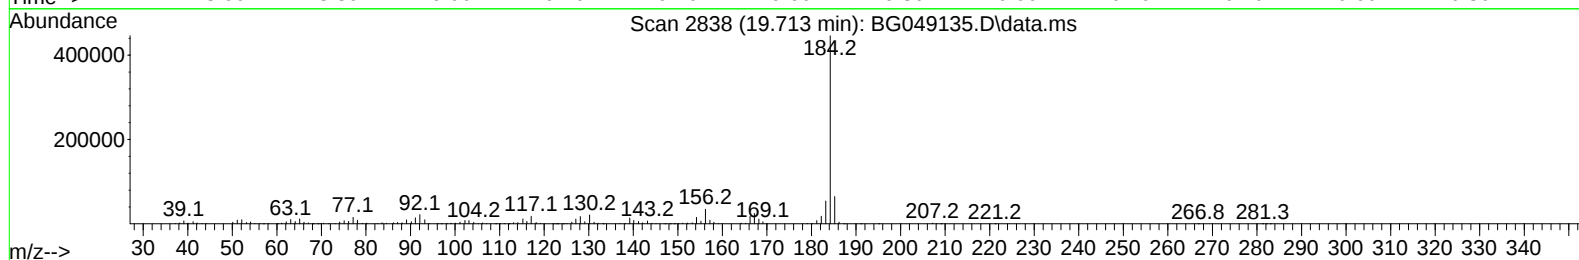


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063021\
Data File : BG049135.D
Acq On : 30 Jun 2021 9:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 10:55:07 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 10:49:10 2021
Response via : Initial Calibration

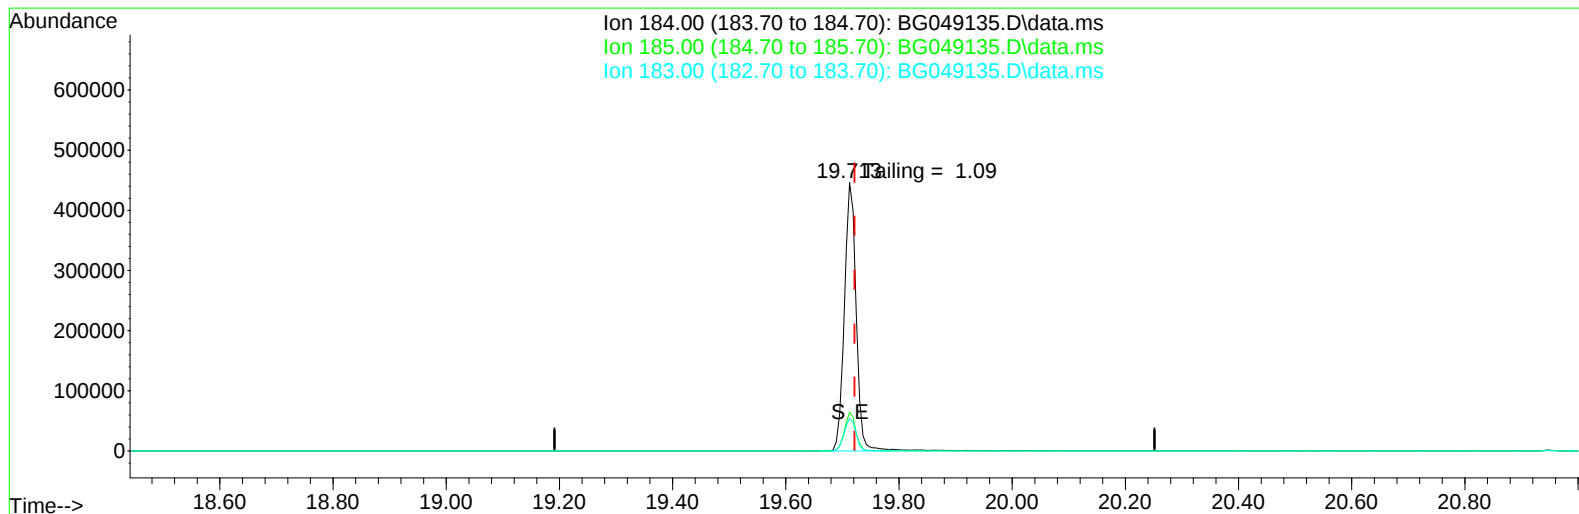




TIC: BG049135.D\data.ms

(77) Benzidine**19.713min (-0.008) 39603.84 ng****response 642243**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.47
183.00	11.70	12.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063021\
Data File : BG049135.D
Acq On : 30 Jun 2021 9:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 30 10:55:07 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 30 10:49:10 2021
Response via : Initial Calibration

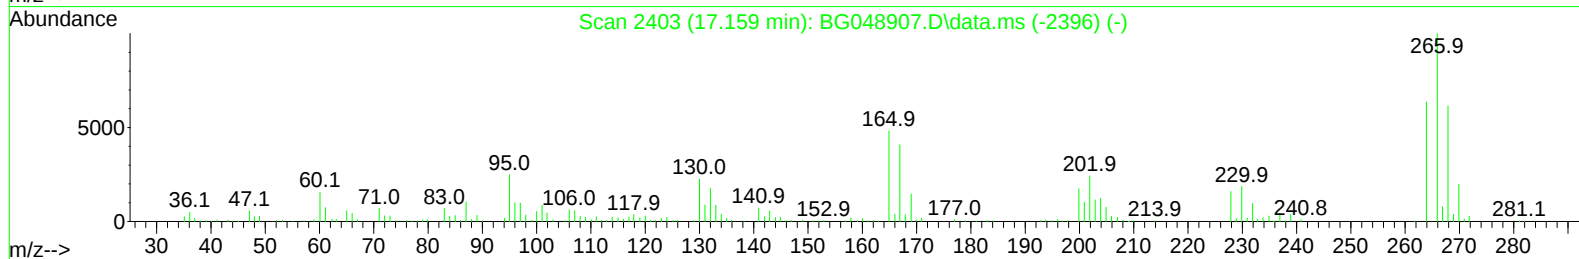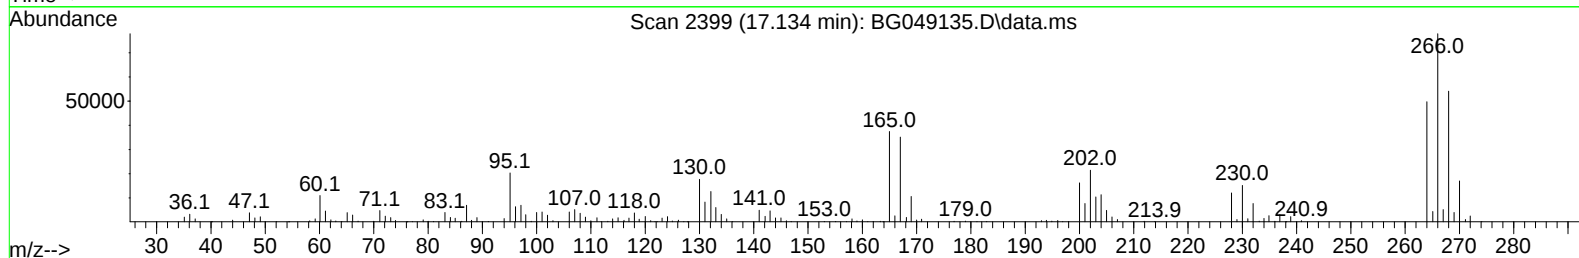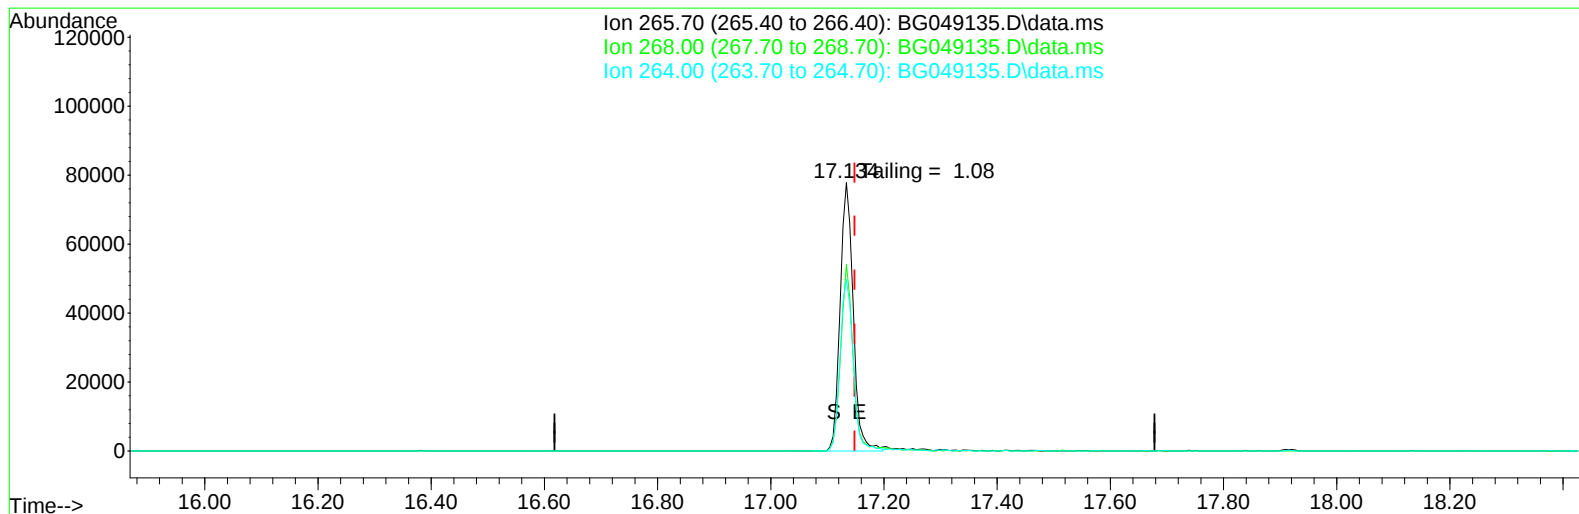

TIC: BG049135.D\data.ms

(70) Pentachlorophenol (C)

17.134min (-0.014) 201789.40 ng

response 126371

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	69.48
264.00	61.30	63.93
0.00	0.00	0.00