
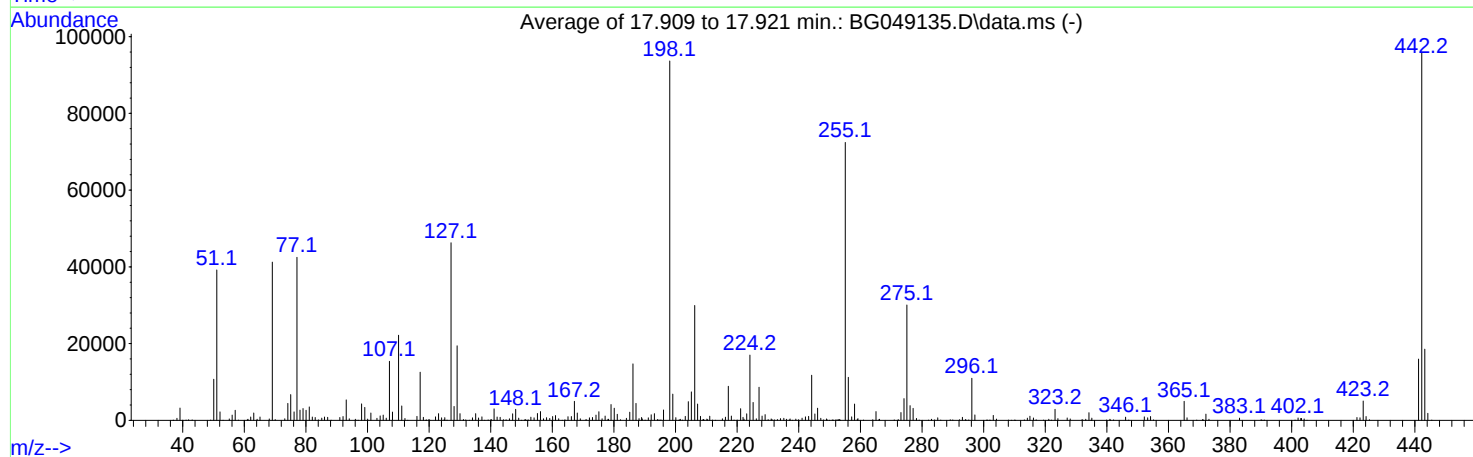


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063021\
 Data File : BG049135.D
 Acq On : 30 Jun 2021 9:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 30 15:39:12 2021

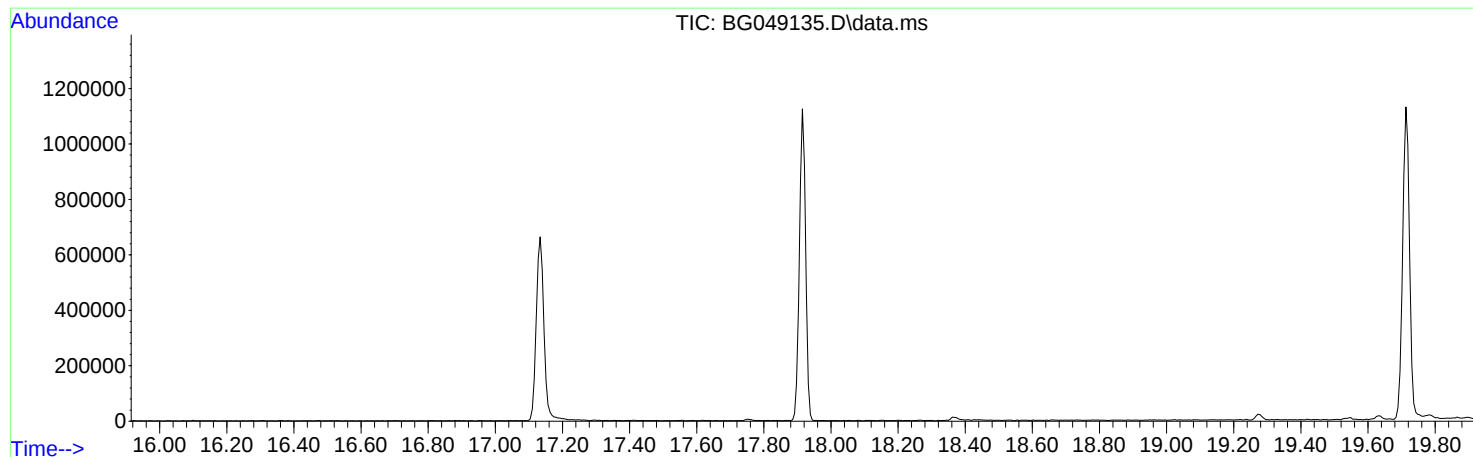

AutoFind: Scans 2531, 2532, 2533; Background Corrected with Scan 2524

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	39192	PASS
68	69	0.00	2	0.9	379	PASS
69	198	0.00	100	44.0	41248	PASS
70	69	0.00	2	0.5	212	PASS
127	198	10	80	49.4	46269	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93653	PASS
199	198	5	9	7.3	6855	PASS
275	198	10	60	32.1	30051	PASS
365	198	1	100	5.3	4961	PASS
441	198	0.01	100	17.1	15988	PASS
442	442	100	100	100.0	95867	PASS
443	442	15	24	19.3	18544	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/30/2021	BNA_G	<u>BG049135.D</u>
Compound Name	Response	Retention Time
DDT	349455	20.95
DDD	2285	20.5
DDE	620	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2905	352360	0.82

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063021\
 Data File : BG049135.D
 Acq On : 30 Jun 2021 9:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 30 10:55:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 30 10:49:10 2021
 Response via : Initial Calibration

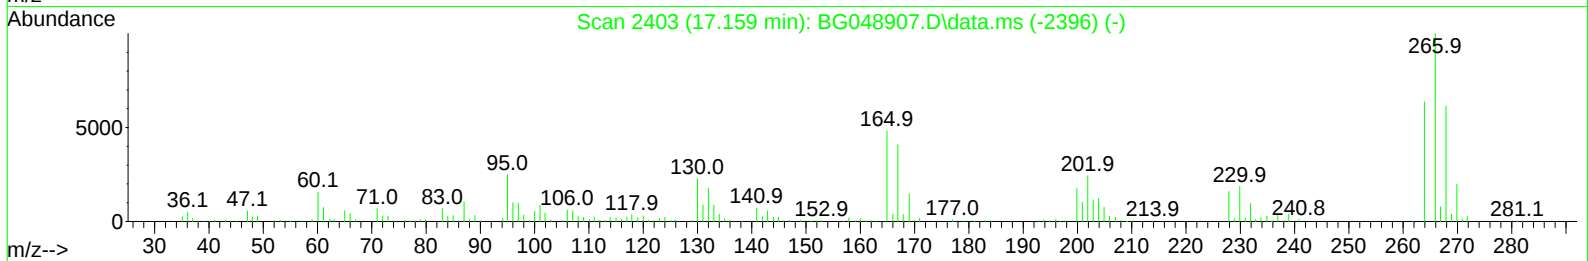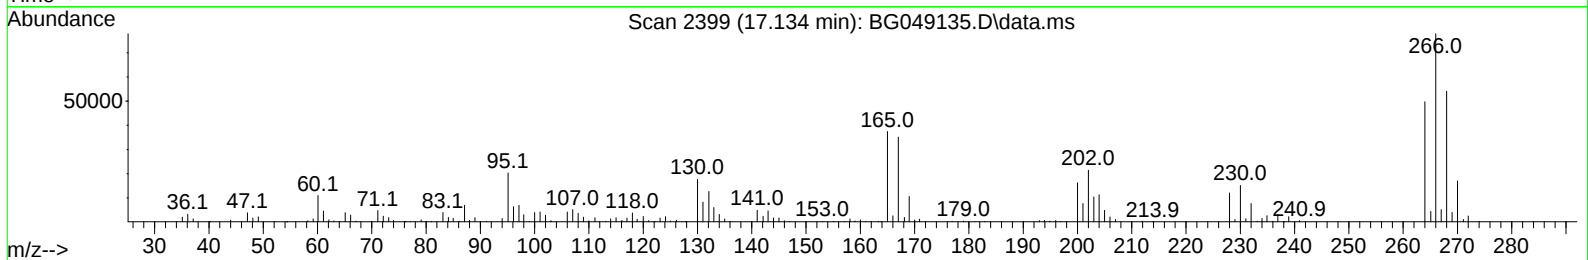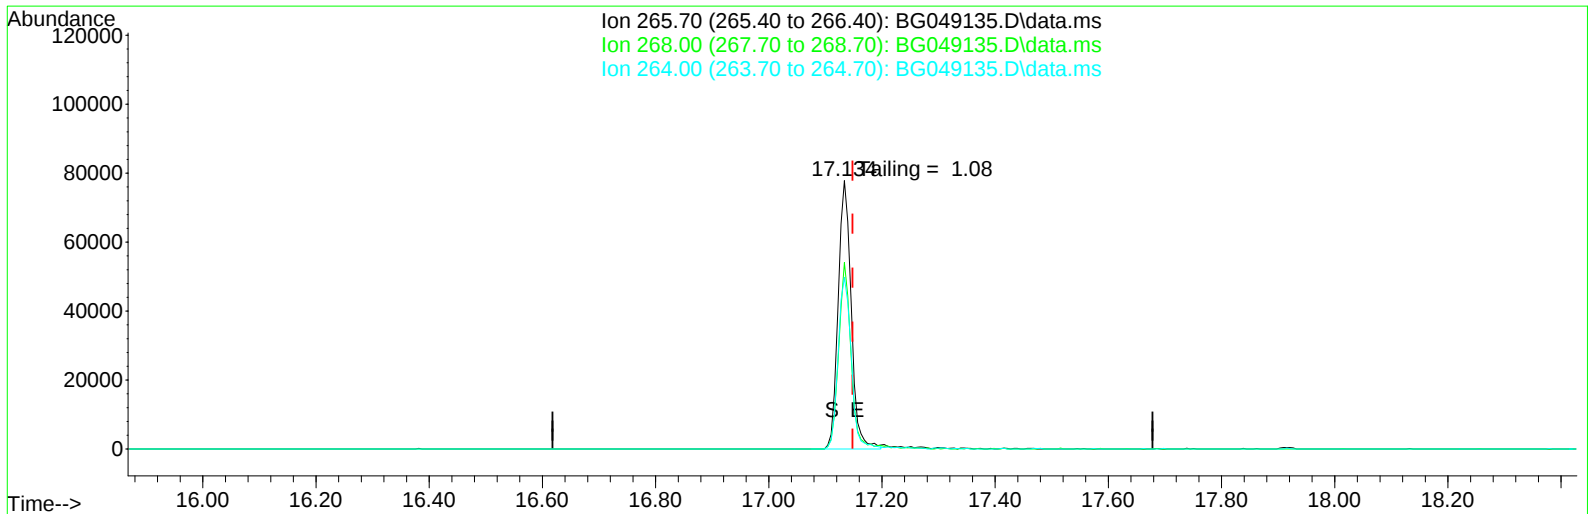

TIC: BG049135.D\data.ms

(70) Pentachlorophenol (C)

17.134min (-0.014) 201789.40 ng




response 126371

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	69.48
264.00	61.30	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063021\
 Data File : BG049135.D
 Acq On : 30 Jun 2021 9:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Jun 30 10:55:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG063021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 30 10:49:10 2021
 Response via : Initial Calibration

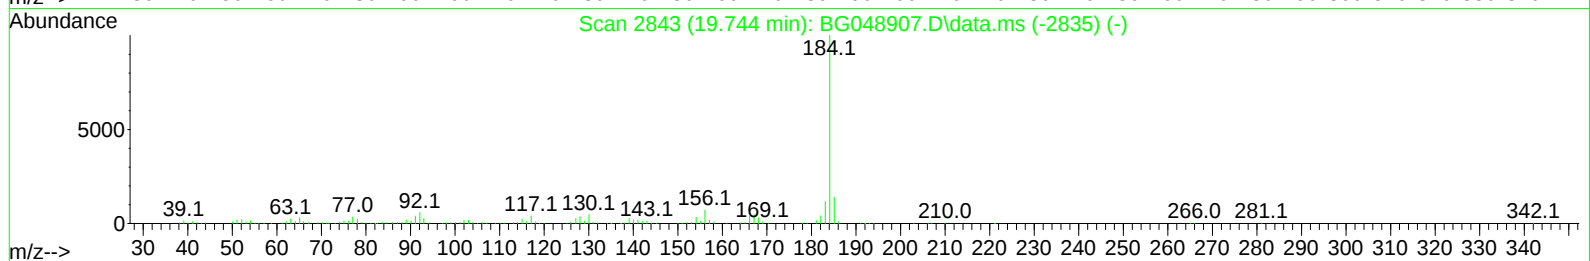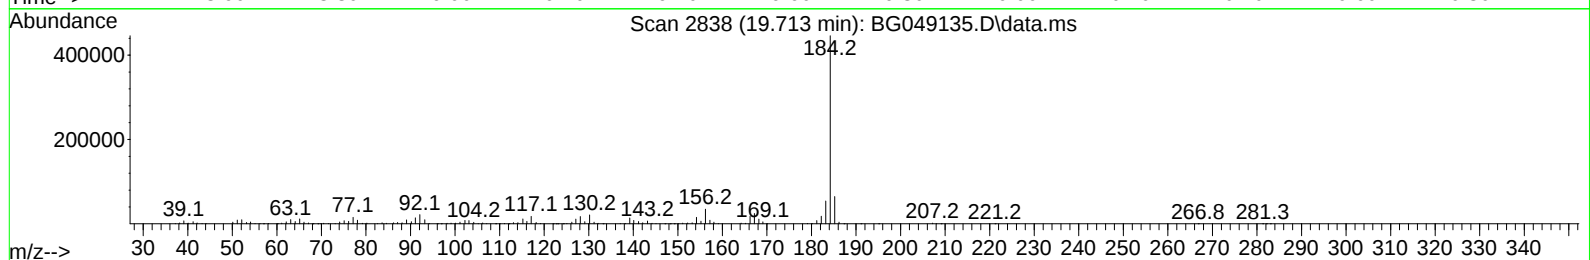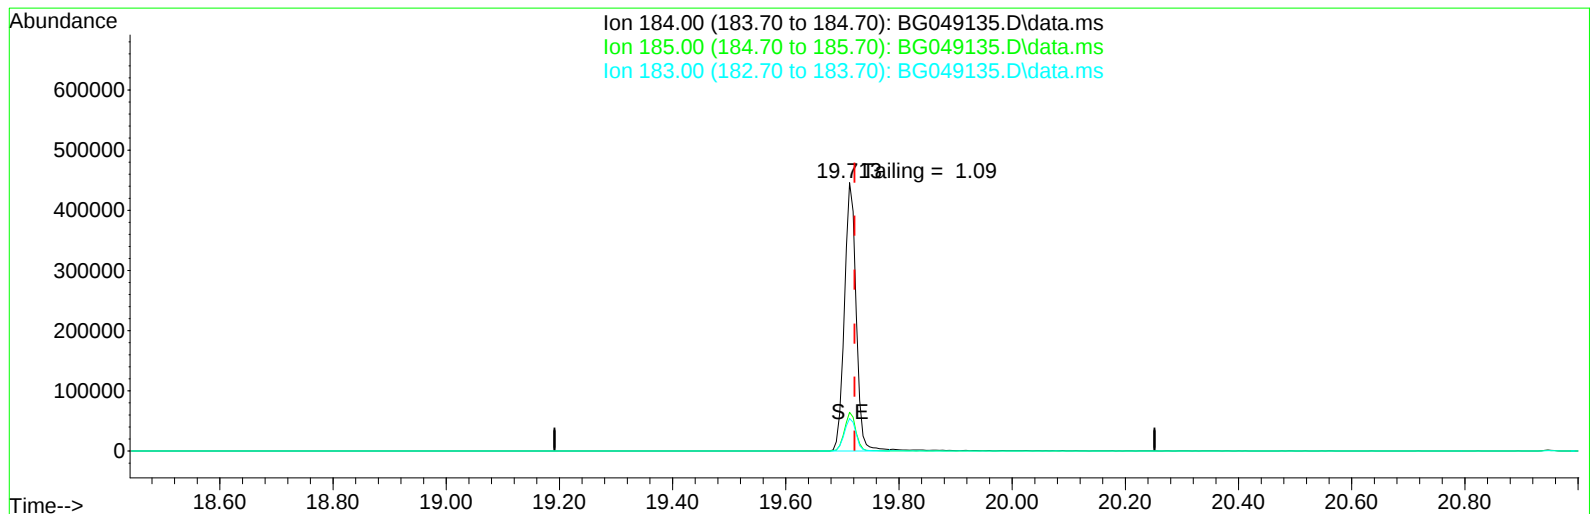

TIC: BG049135.D\data.ms

(77) Benzidine

19.713min (-0.008) 39603.84 ng

response 642243

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.47
183.00	11.70	12.11
0.00	0.00	0.00