

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063022\
 Data File : BG054173.D
 Acq On : 30 Jun 2022 17:26
 Operator : CG/JU
 Sample : N3548-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 V-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG054173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.635	375	382	393	rVB	208094	353151	22.86%	6.156%
2	7.227	646	653	663	rBV	229399	409008	26.48%	7.129%
3	8.061	789	795	803	rVB	52057	92466	5.99%	1.612%
4	9.225	985	993	1005	rVB	144284	267229	17.30%	4.658%
5	10.870	1266	1273	1284	rBB	69895	134256	8.69%	2.340%
6	13.314	1682	1689	1698	rBV	456301	740925	47.96%	12.915%
7	14.689	1917	1923	1931	rBB	133846	216227	14.00%	3.769%
8	16.175	2170	2176	2190	rBV	400323	639424	41.39%	11.145%
9	17.433	2382	2390	2396	rBV	197021	312478	20.23%	5.447%
10	19.483	2731	2739	2744	rBV	19131	28087	1.82%	0.490%
11	19.847	2797	2801	2806	rVB	17394	25184	1.63%	0.439%
12	20.041	2828	2834	2840	rBV	1144963	1544755	100.00%	26.925%
13	21.340	3050	3055	3064	rBV3	45685	82650	5.35%	1.441%
14	21.710	3111	3118	3124	rBV	239701	414953	26.86%	7.233%
15	22.521	3251	3256	3265	rVB7	8787	21565	1.40%	0.376%
16	23.931	3489	3496	3497	rBV4	9245	16264	1.05%	0.283%
17	24.031	3509	3513	3518	rVB7	9847	20946	1.36%	0.365%
18	24.959	3661	3671	3687	rVB2	137473	417582	27.03%	7.279%




Sum of corrected areas: 5737150

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063022\
Data File : BG054173.D
Acq On : 30 Jun 2022 17:26
Operator : CG/JU
Sample : N3548-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
V-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

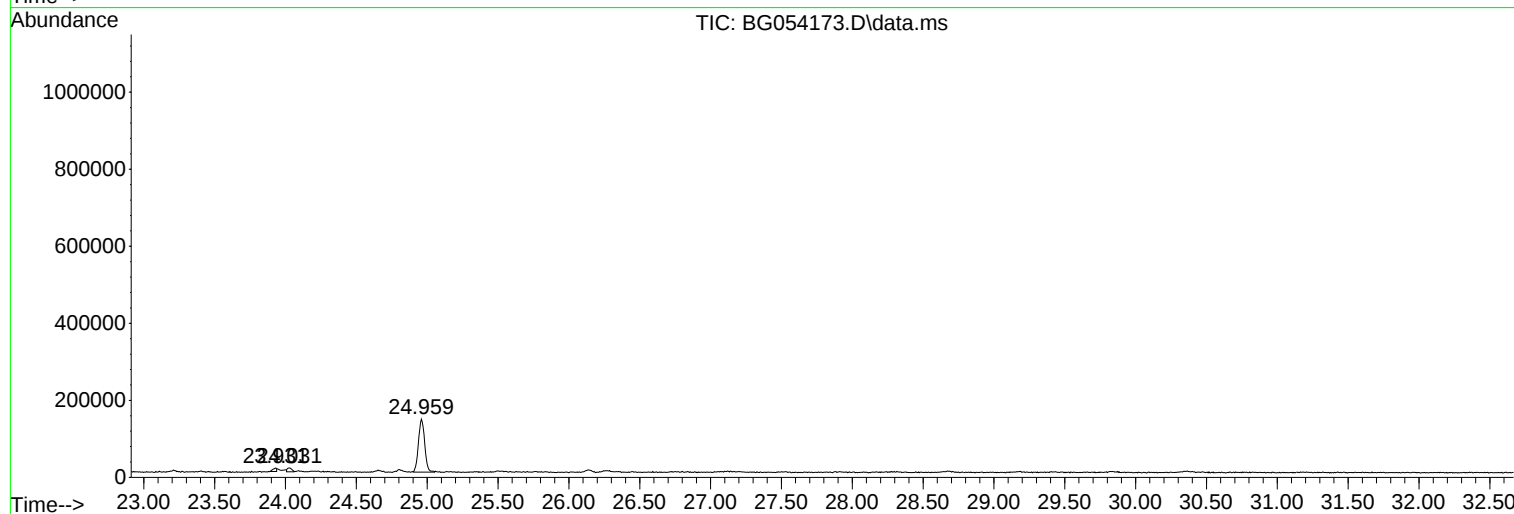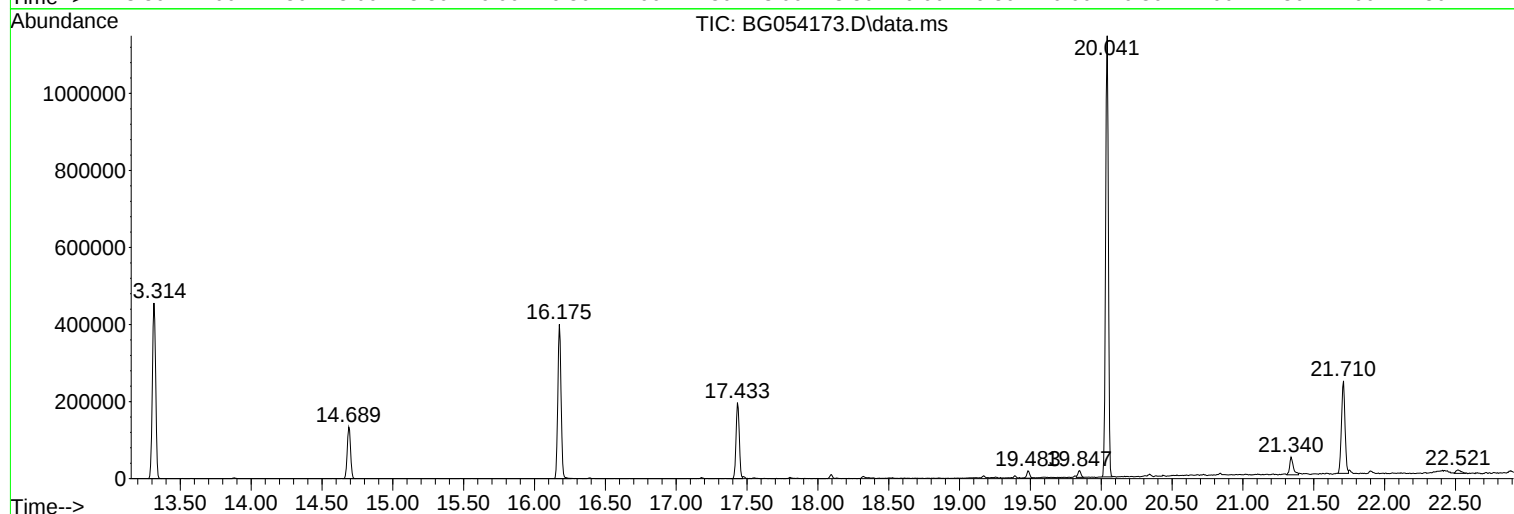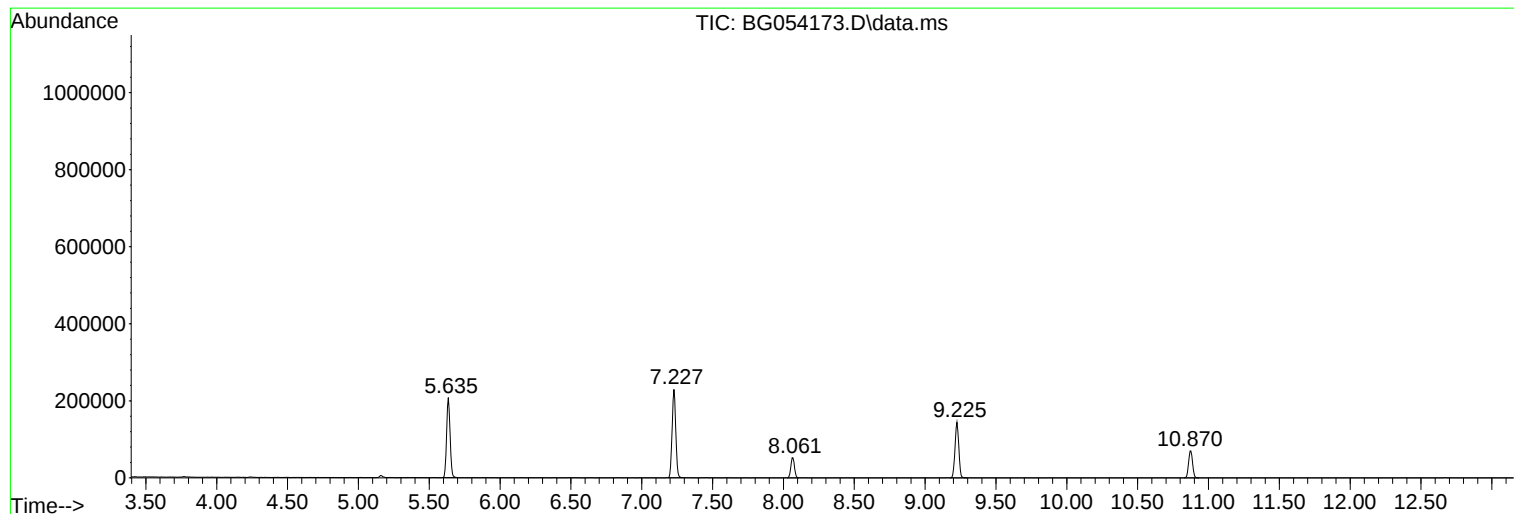

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063022\
Data File : BG054173.D
Acq On : 30 Jun 2022 17:26
Operator : CG/JU
Sample : N3548-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
V-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trifluoroacetoxy hexadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.340	3.98 ng	82650	Chrysene-d12	21.710

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	95
2			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	95
3			Heptafluorobutyric acid, n-tetra...	410	C18H29F7O2	007365-36-8	94
4			1-Heneicosanol	312	C21H44O	015594-90-8	93
5			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	93

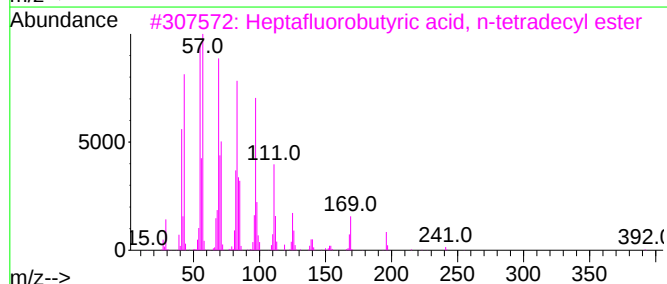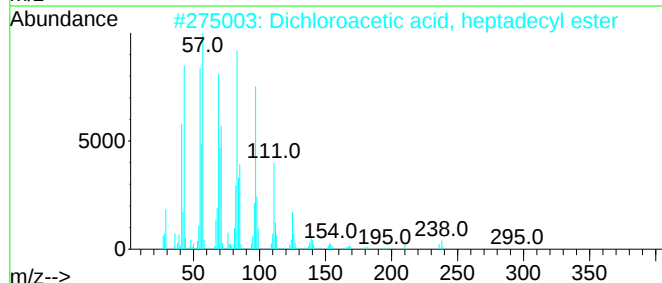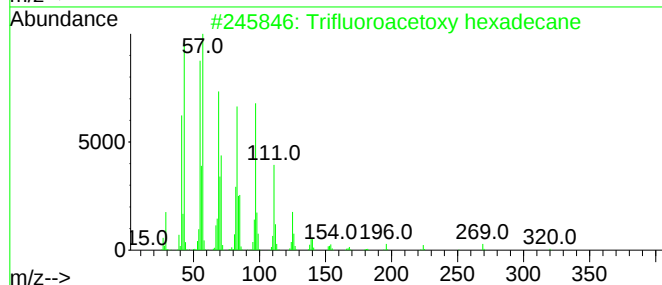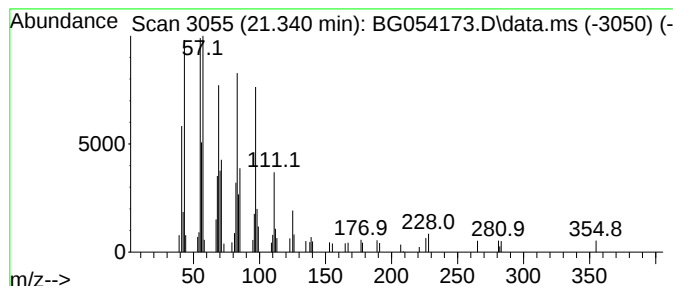

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063022\
Data File : BG054173.D
Acq On : 30 Jun 2022 17:26
Operator : CG/JU
Sample : N3548-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
V-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trifluoroacetox...	21.340	4.0	ng	82650	5	21.710	414953	20.0