
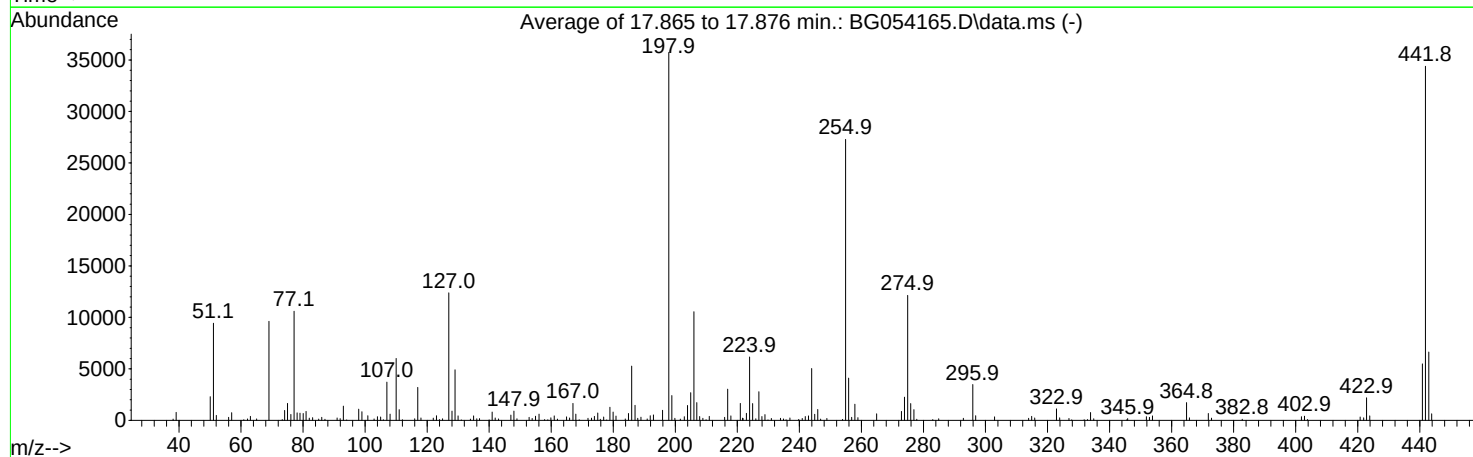


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063022\
Data File : BG054165.D
Acq On : 30 Jun 2022 12:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jun 27 00:27:54 2022

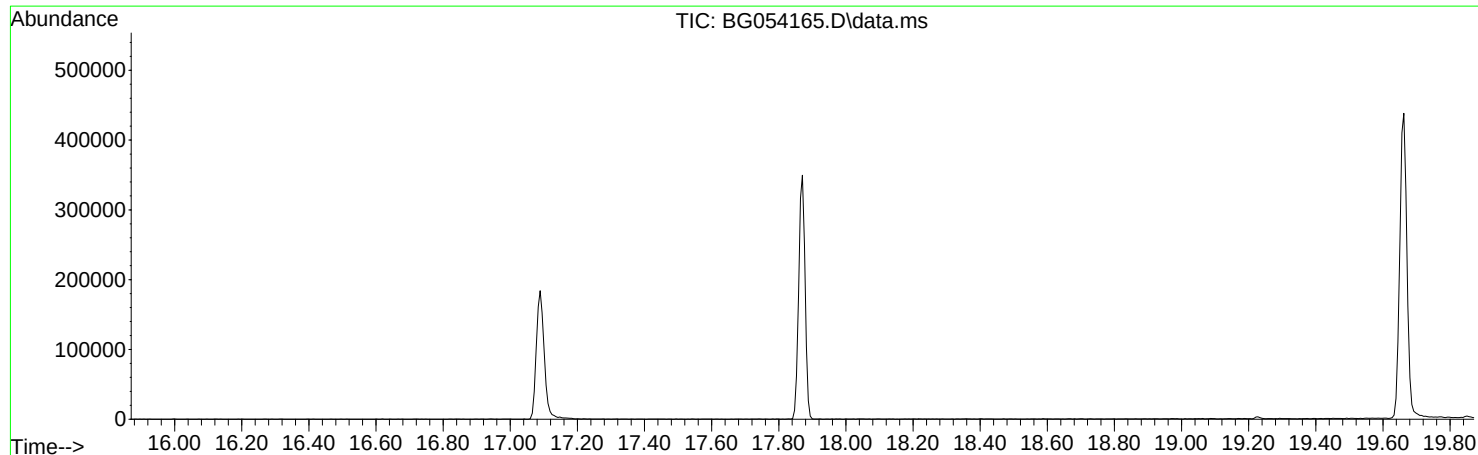




AutoFind: Scans 2464, 2465, 2466; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.4	9435	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.9	9615	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	34.7	12381	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35725	PASS
199	198	5	9	6.7	2411	PASS
275	198	10	60	34.0	12138	PASS
365	198	1	100	4.8	1719	PASS
441	198	0.01	100	15.3	5478	PASS
442	442	50	100	100.0	34387	PASS
443	442	15	24	19.3	6641	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063022\
Data File : BG054165.D
Acq On : 30 Jun 2022 12:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 01 08:46:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

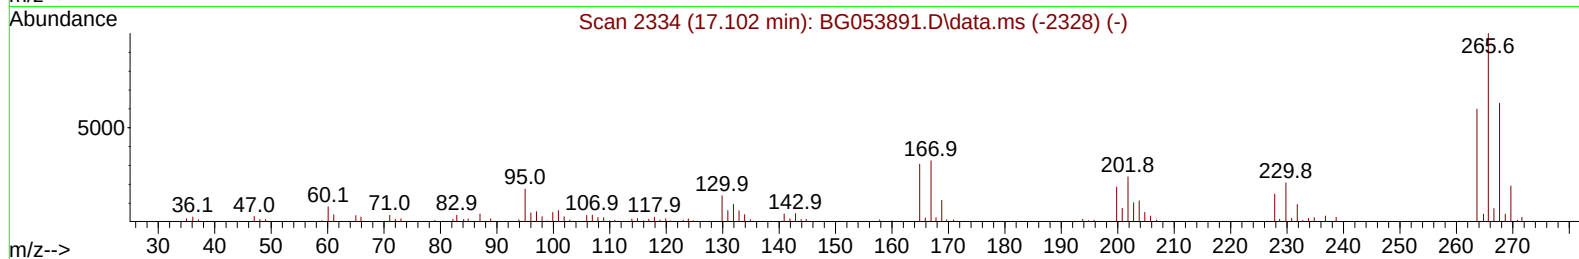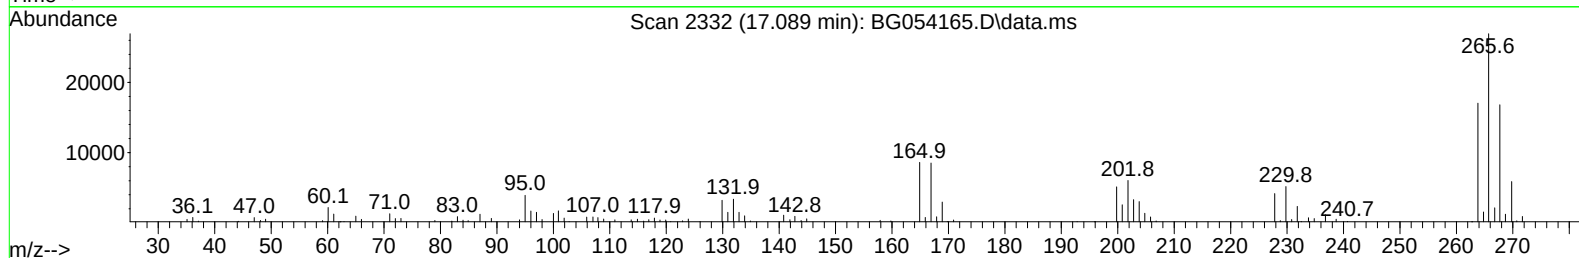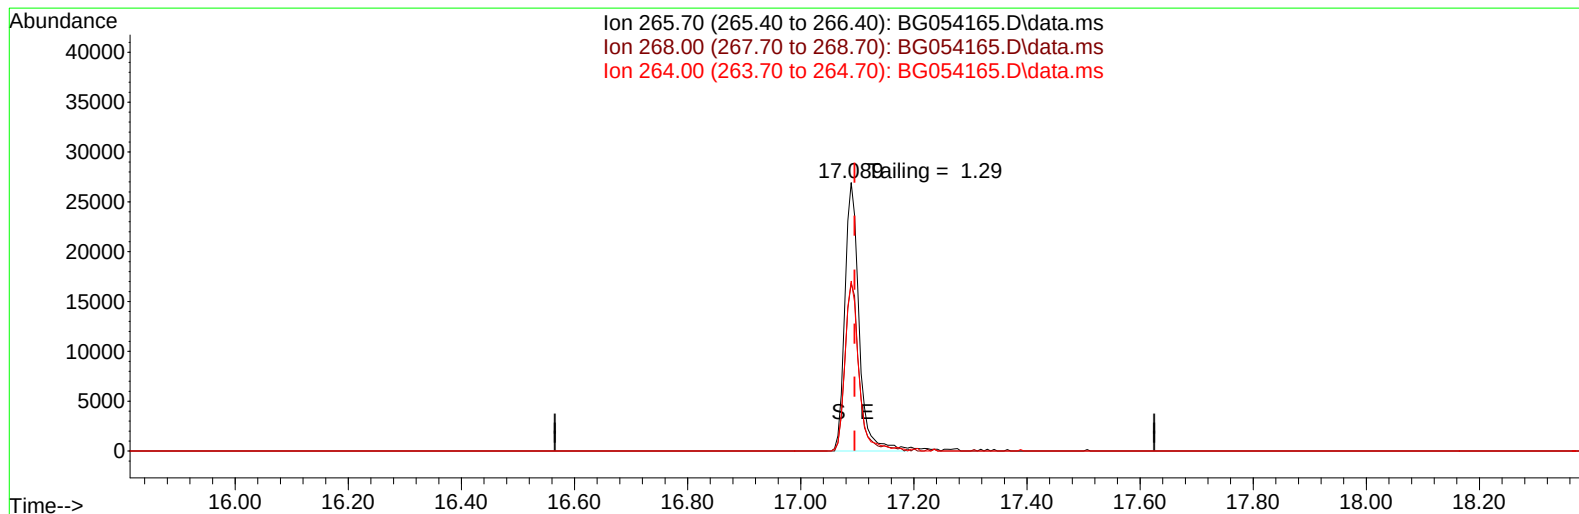

TIC: BG054165.D\data.ms

(70) Pentachlorophenol (C)

17.089min (-0.006) 32304.74 ng




response 47594

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	70.20	67.03
264.00	66.20	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG063022\
Data File : BG054165.D
Acq On : 30 Jun 2022 12:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 01 08:46:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG061322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 27 00:27:54 2022
Response via : Initial Calibration

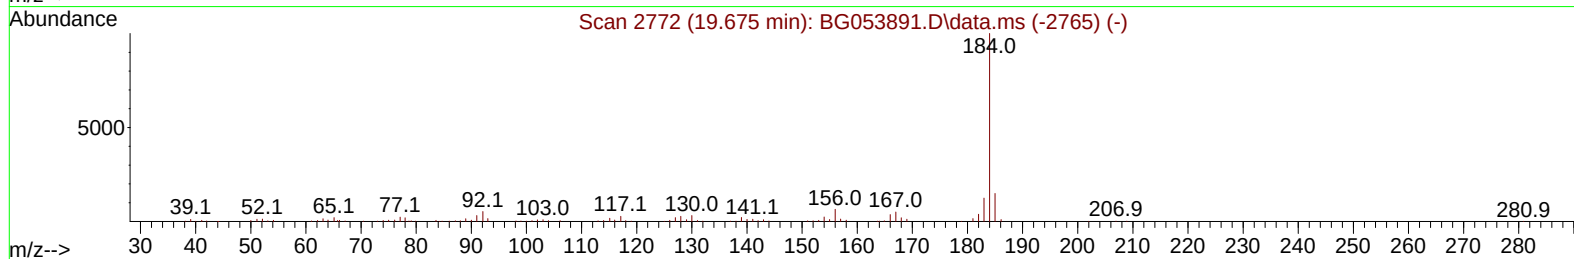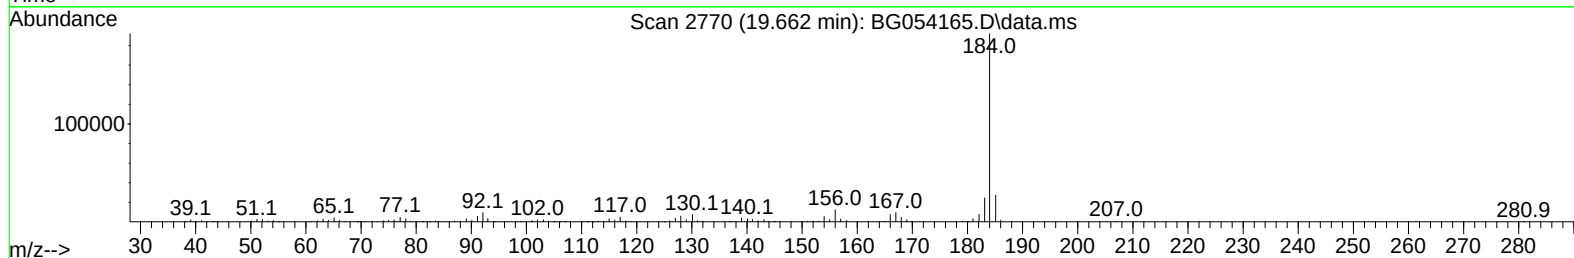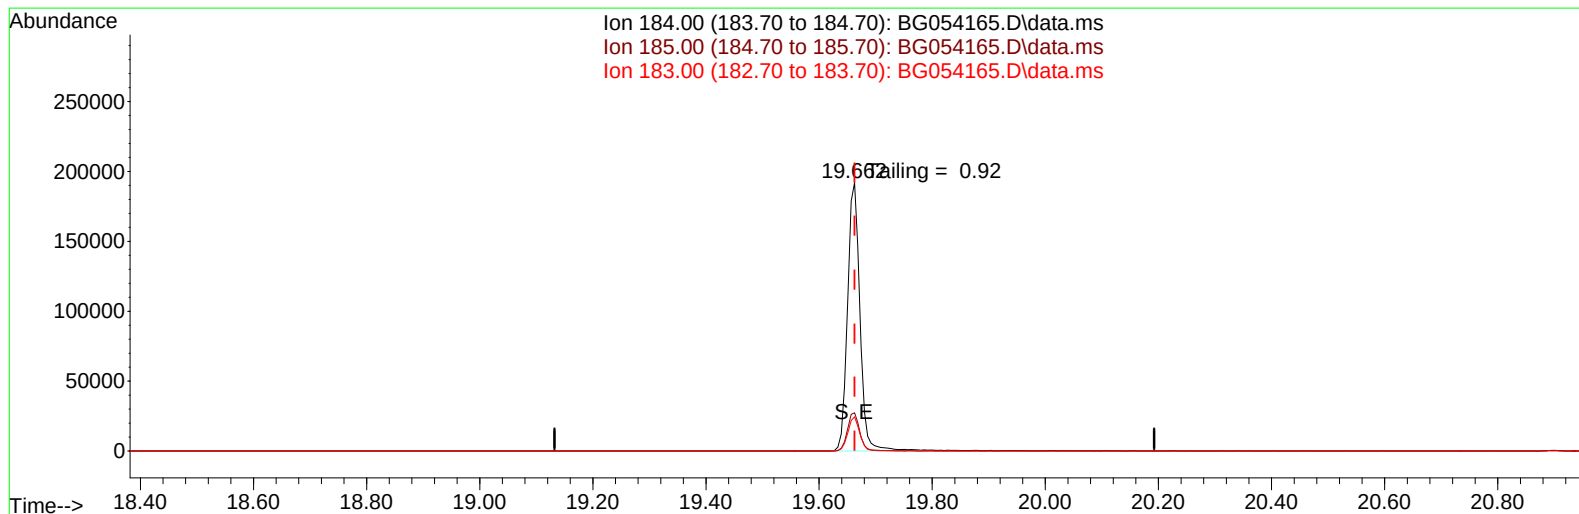

TIC: BG054165.D\data.ms

(77) Benzidine

19.662min (-0.000) 0.00 ng

response 293059

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.23
183.00	11.10	12.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/30/2022	BNA_G	<u>BG054165.D</u>
Compound Name	Response	Retention Time
DDT	160733	20.896
DDD	3777	20.456
DDE	680	19.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4457	165190	2.70

Instrument :
BNA_G
ClientSampleId :
DFTPP