

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
 Data File : BG022769.D
 Acq On : 1 Jul 2016 22:26
 Operator : UM/SJ
 Sample : H3811-19
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4TW7

Quant Time: Jul 02 00:09:49 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 02 00:07:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	172111	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	758349	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	580711	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	1329979	20.00	ng/ul	0.00
75) Chrysene-d12	21.86	240	1477961	20.00	ng/ul	0.00
83) Perylene-d12	25.23	264	1504491	20.00	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.56	96	5082	1.65	ng/uL	0.01
5) Phenol-d5	7.31	99	332359	18.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	206731	20.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	223330	18.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	262507	18.67	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	122689	20.29	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	139996	19.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.61	165	280438	18.39	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	221282	17.13	ng/ul	0.00
43) Dimethylphthalate-d6	14.20	166	954436	20.23	ng/ul	0.00
46) Acenaphthylene-d8	14.50	160	1083392	20.04	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	135915	18.35	ng/ul	0.00
57) Fluorene-d10	15.79	176	882429	19.74	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	165618	19.36	ng/ul	0.00
70) Anthracene-d10	17.65	188	1257485	20.34	ng/ul	0.00
76) Pyrene-d10	19.94	212	1471815	20.85	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	1419712	19.86	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.24	163	265536	5.51	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022769.D
Acq On : 1 Jul 2016 22:26
Operator : UM/SJ
Sample : H3811-19
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4TW7

Quant Time: Jul 02 00:09:49 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 02 00:07:37 2016
Response via : Initial Calibration

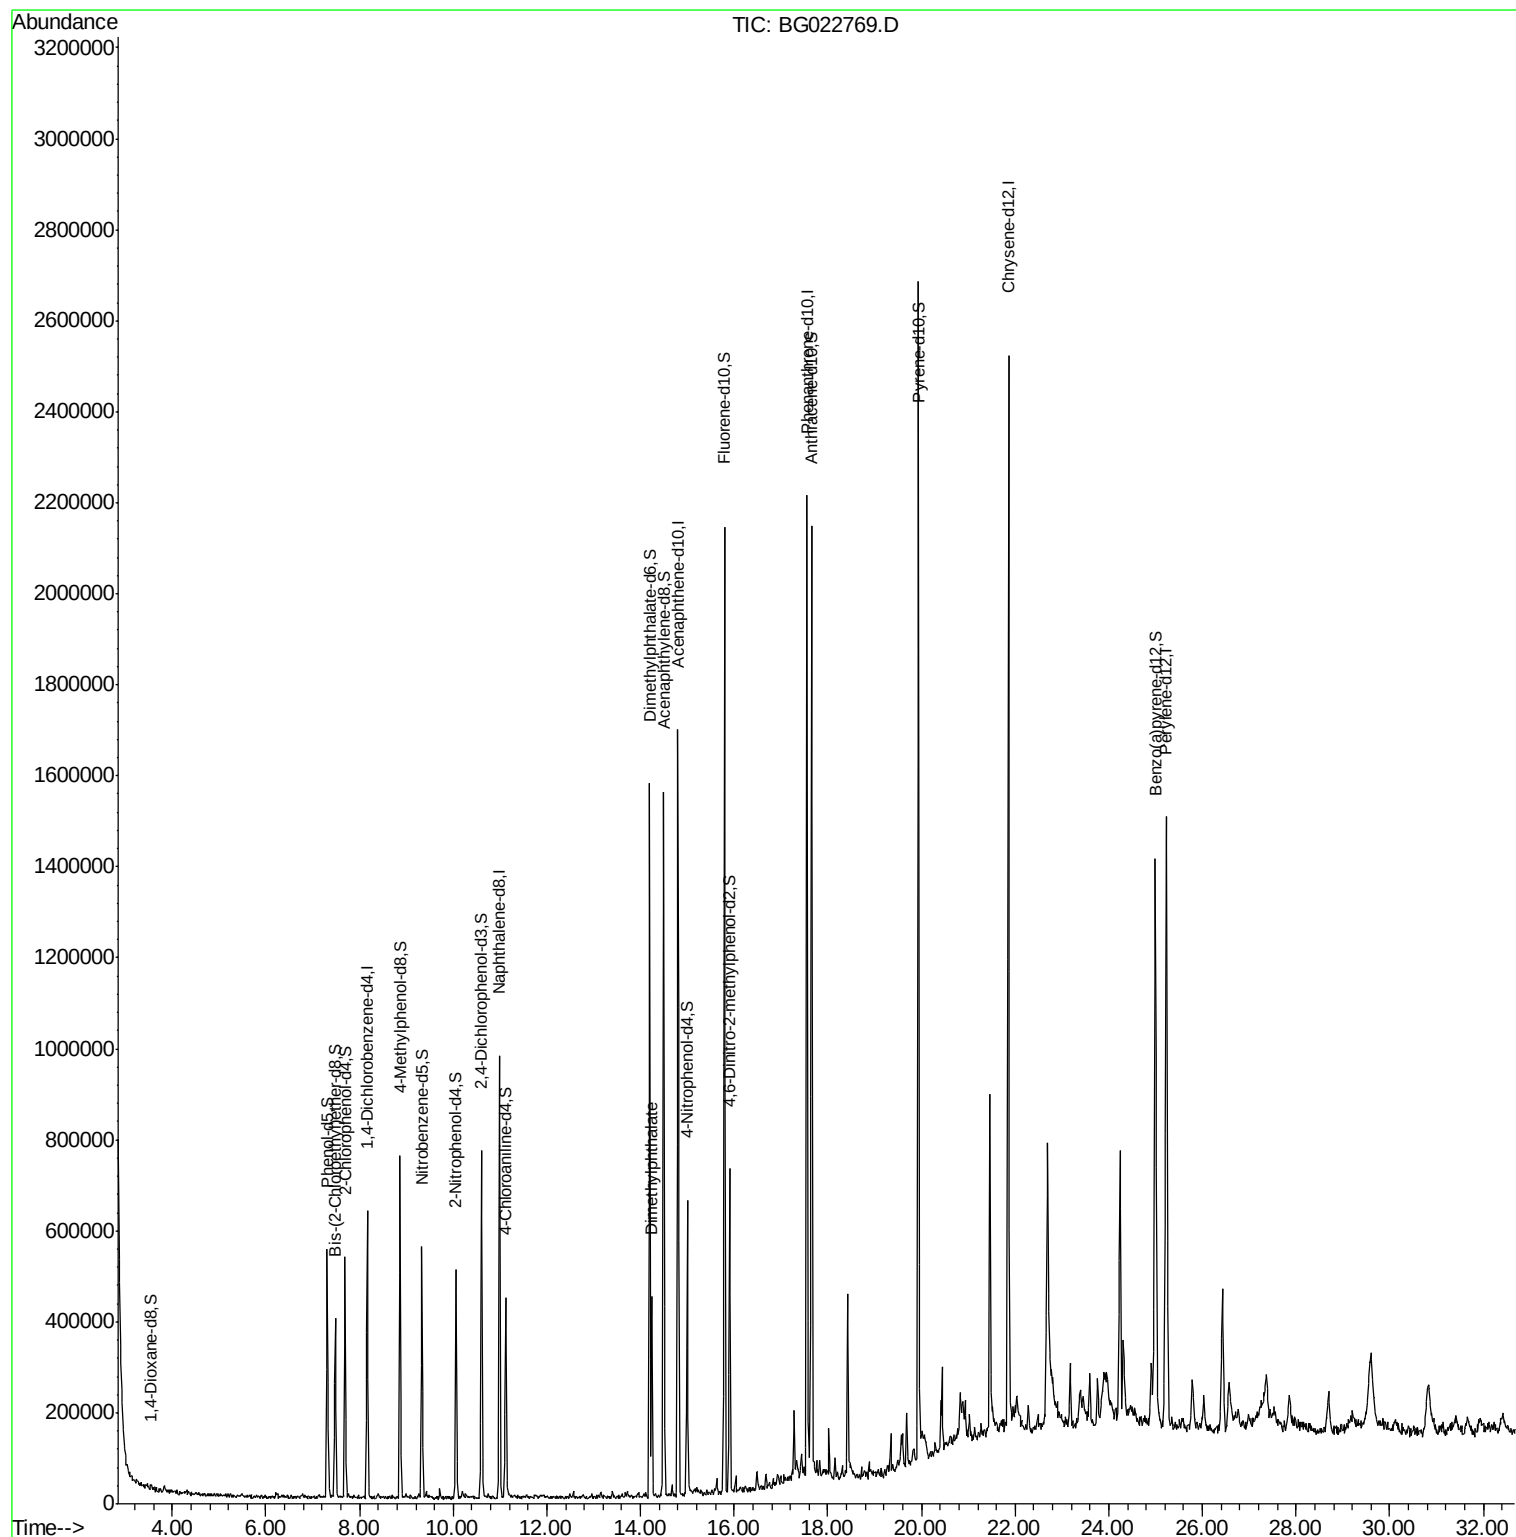

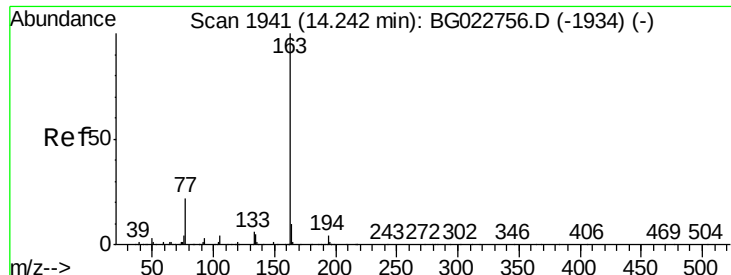

#44

Dimethylphthalate

Concen: 5.51 ng/ul

RT: 14.24 min Scan# 1941

Delta R.T. 0.00 min

Lab File: BG022769.D

Acq: 1 Jul 2016 22:26

Instrument :

BNA_G

ClientSampleId :

A4TW7

Tgt Ion:163 Resp: 265536

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 9.9 8.8 13.2

