

Quantitation Report (QT Reviewed)


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
 Data File : BG022776.D
 Acq On : 2 Jul 2016 3:07
 Operator : UM/SJ
 Sample : H3752-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHL9

Manual Integration

Quant Time: Jul 02 05:13:24 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 02 00:07:37 2016
 Response via : Initial Calibration

APPROVED
 sohil
 7/4/2016 1:32:02 PM

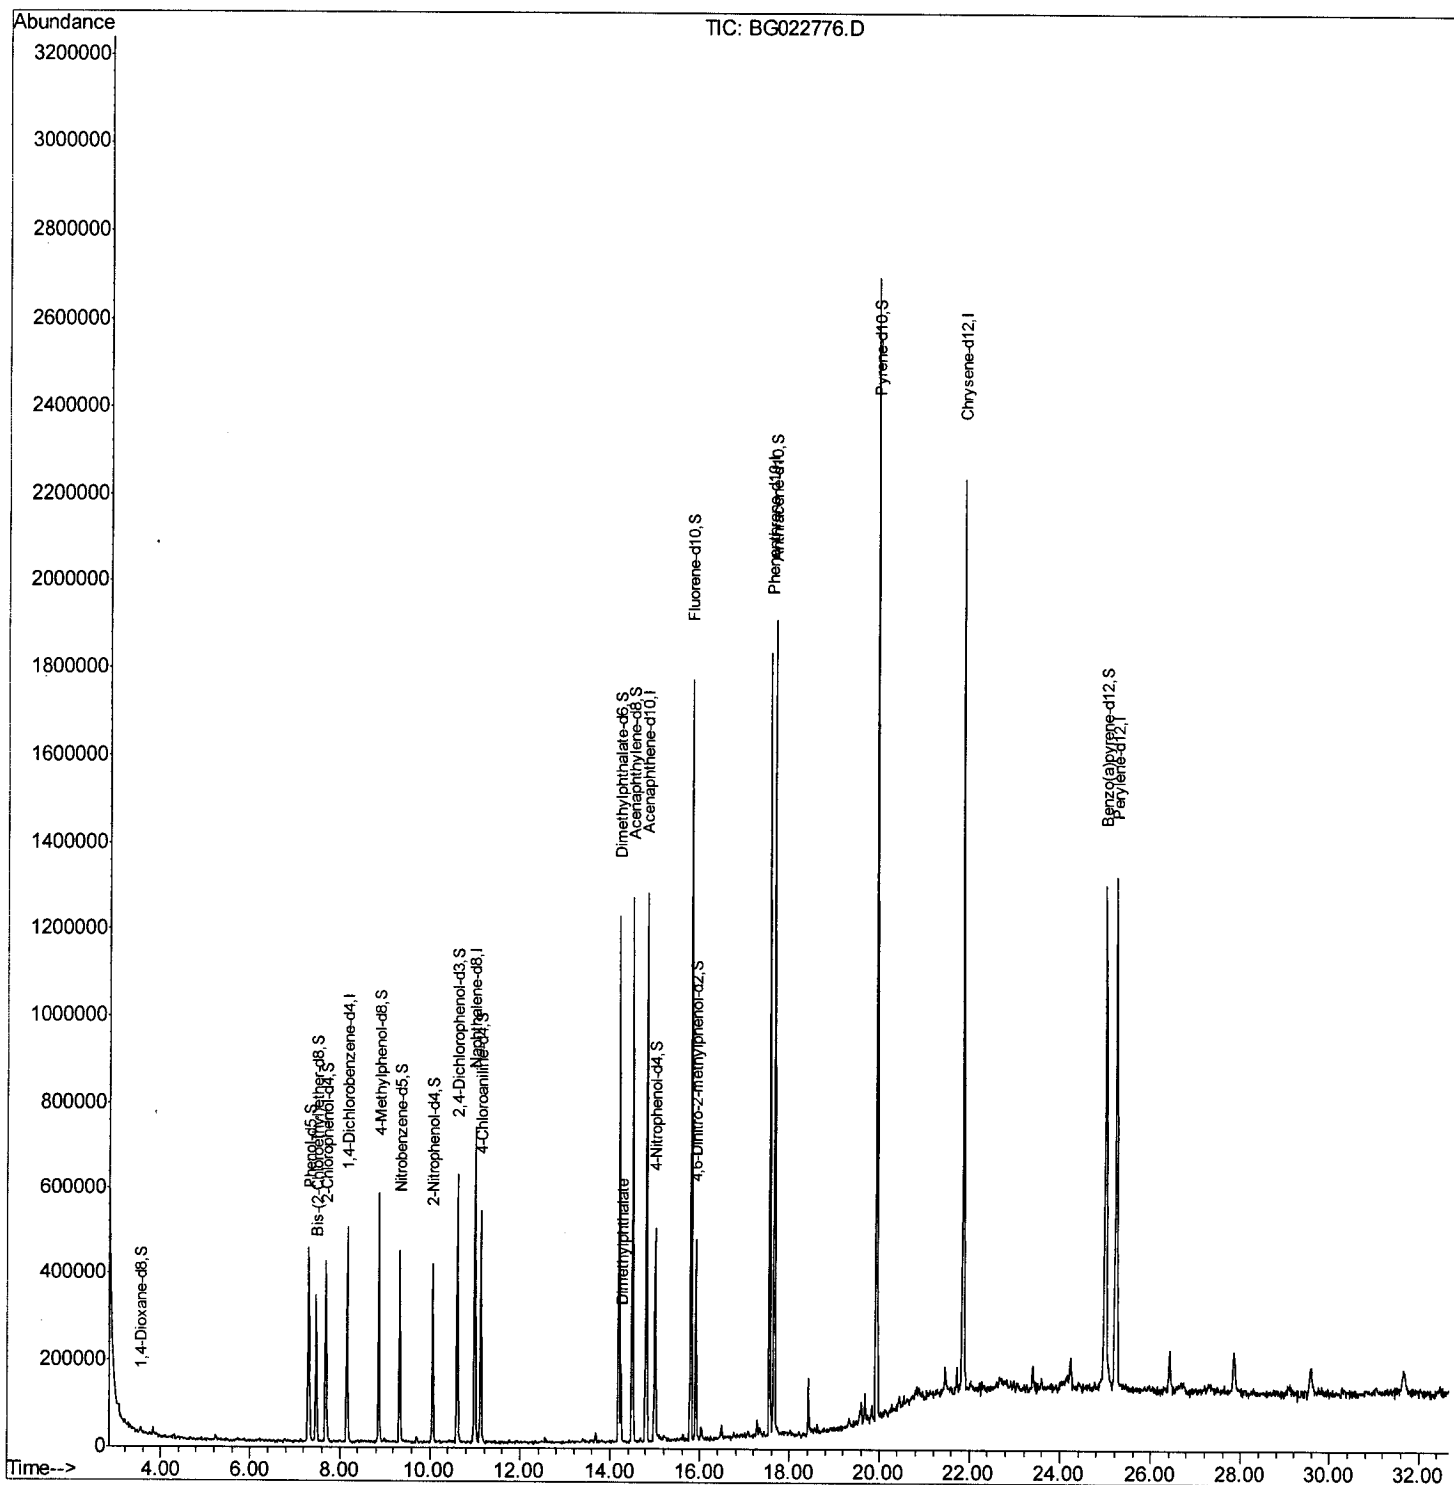

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
 Data File : BG022776.D
 Acq On : 2 Jul 2016 3:07
 Operator : UM/SJ
 Sample : H3752-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHL9

Manual Integration

Quant Time: Jul 02 04:16:15 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 02 00:07:37 2016
 Response via : Initial Calibration

APPROVED
 sohil
 7/4/2016 1:32:02 PM

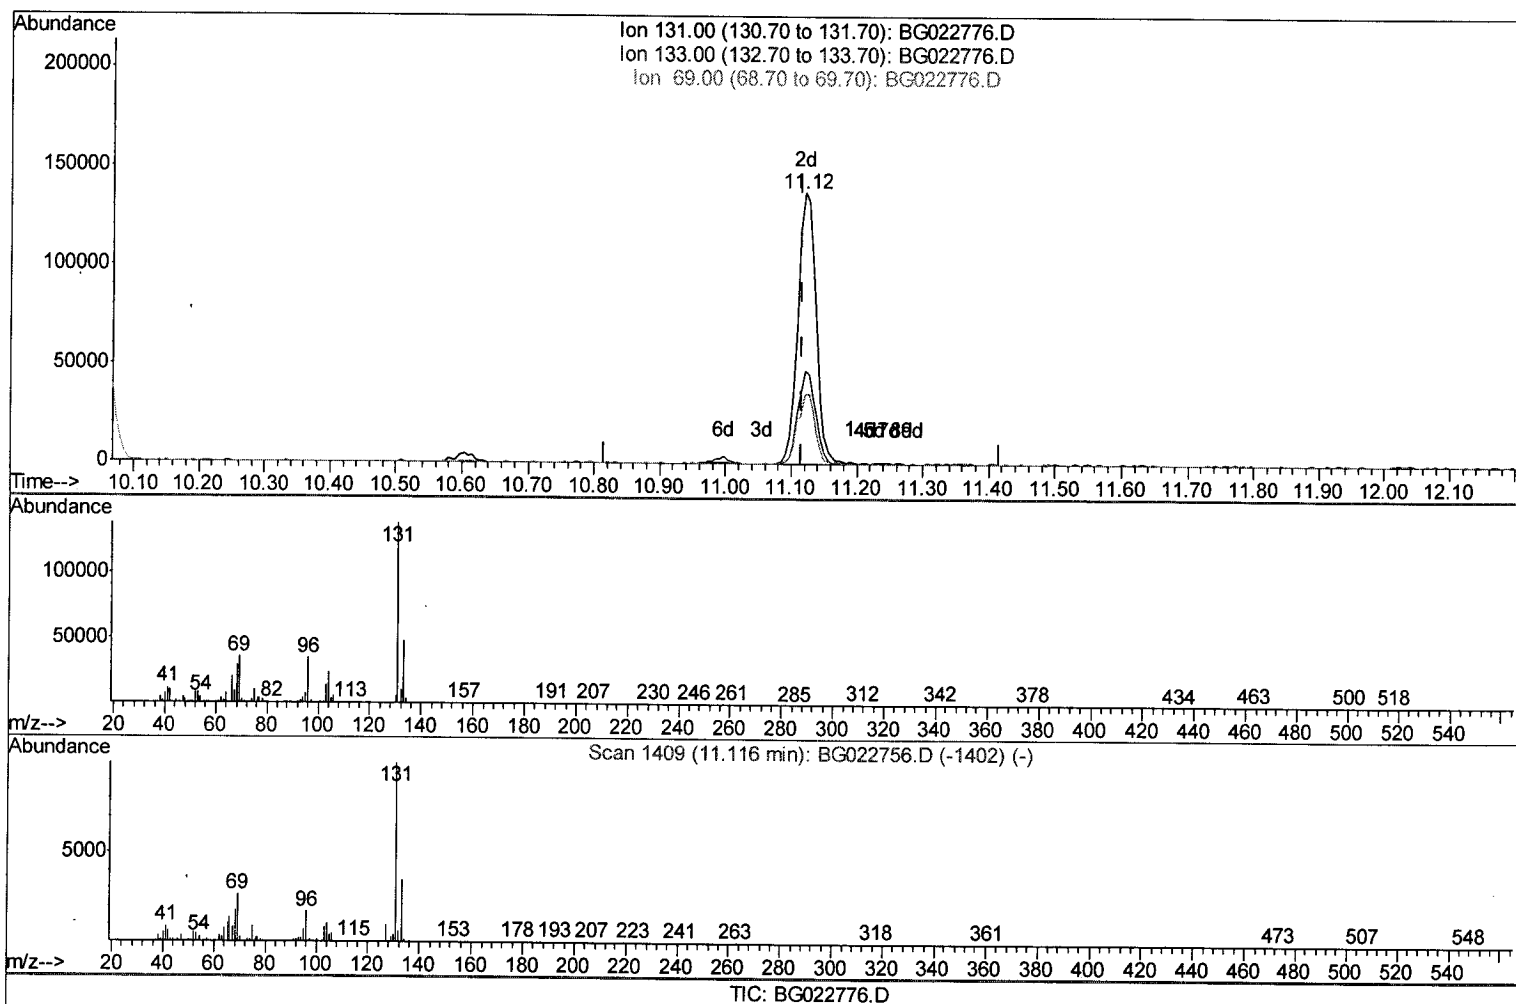

(29) 4-Chloroaniline-d4 (S)

11.120min (+0.004) 26.57ng/ul m U.M

response 260997

Ion	Exp%	Act%
131.00	100	100
133.00	33.10	34.76
69.00	15.40	25.98#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022776.D
Acq On : 2 Jul 2016 3:07
Operator : UM/SJ
Sample : H3752-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHL9

Quant Time: Jul 02 04:16:15 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 02 00:07:37 2016
Response via : Initial Calibration

Manual Integration

APPROVED
sohil
7/4/2016 1:32:02 PM

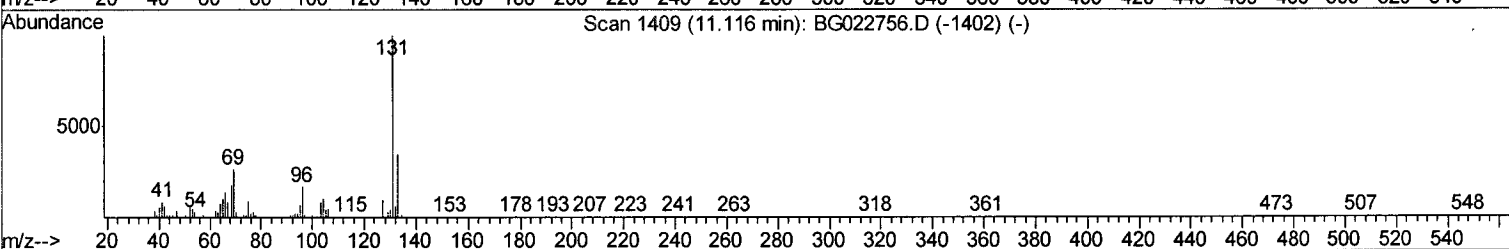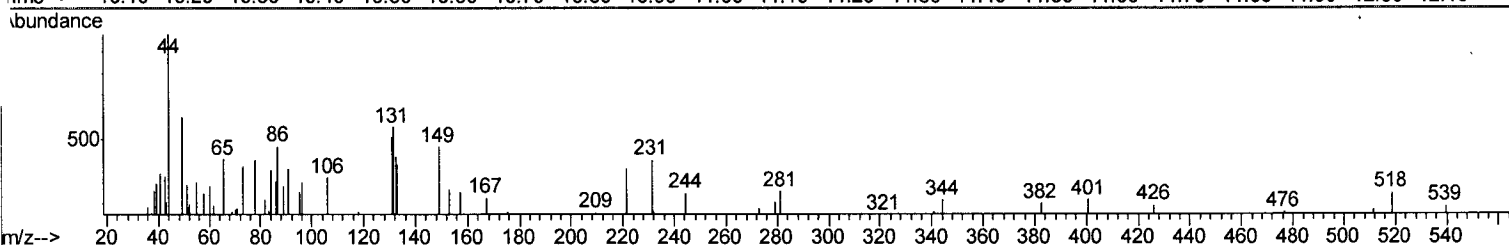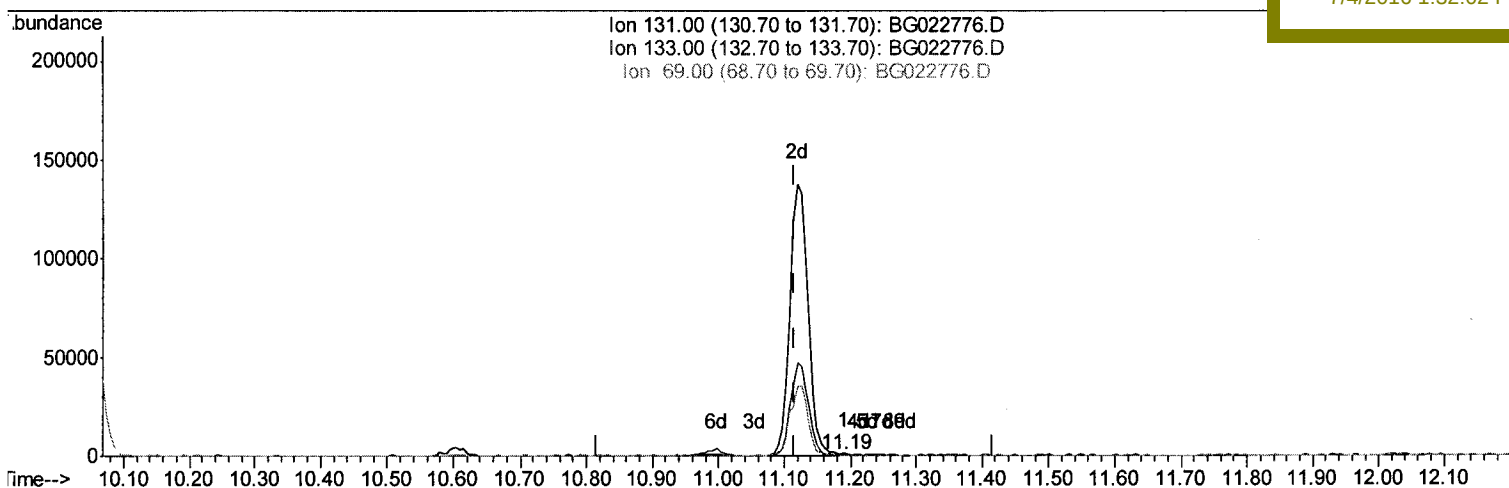

TIC: BG022776.D

(29) 4-Chloroaniline-d4 (S)

11.190min (+0.074) 0.07ng/ul

response 655

Ion	Exp%	Act%
131.00	100	100
133.00	33.10	36.38
69.00	15.40	15.17
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
 Data File : BG022776.D
 Acq On : 2 Jul 2016 3:07
 Operator : UM/SJ
 Sample : H3752-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHL9

Quant Time: Jul 02 05:13:24 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 02 00:07:37 2016
 Response via : Initial Calibration

Manual Integration

sohil
 7/4/2016 1:32:02 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	139199	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	576689	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	445326	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	1114913	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1300399	20.00	ng/ul	0.00
83) Perylene-d12	25.23	264	1318298	20.00	ng/ul	0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	4957	1.99	ng/uL	0.00
5) Phenol-d5	7.31	99	273525	18.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	166834	20.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	182060	18.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	207469	18.24	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	89531	19.47	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	110671	19.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	226225	19.50	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	260997m	26.57	ng/ul	0.00
43) Dimethylphthalate-d6	14.20	166	774117	21.40	ng/ul	0.00
46) Acenaphthylene-d8	14.50	160	870157	20.99	ng/ul	0.00
51) 4-Nitrophenol-d4	15.00	143	104293	18.36	ng/ul	0.00
57) Fluorene-d10	15.80	176	730217	21.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	108253	15.10	ng/ul	0.00
70) Anthracene-d10	17.66	188	1128380	21.77	ng/ul	0.00
76) Pyrene-d10	19.94	212	1366437	22.00	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.00	264	1328915	21.22	ng/ul	0.02

U.M
 07/09/16

Target Compounds					Qvalue
44) Dimethylphthalate	14.25	163	102547	2.78 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed