

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
 Data File : BG022758.D
 Acq On : 1 Jul 2016 13:03
 Operator : UM/SJ
 Sample : H3811-26
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4TX6

Manual Integrations

sohil
 7/4/2016 1:30:38 PM

Quant Time: Jul 03 00:05:17 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 02 00:07:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	98280	20.00	ng/ul	0.02
18) Naphthalene-d8	11.00	136	451282	20.00	ng/ul	0.01
35) Acenaphthene-d10	14.81	164	357317	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	840257	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	949362	20.00	ng/ul	0.00
83) Perylene-d12	25.23	264	976774	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	4164	2.37	ng/uL	0.00
5) Phenol-d5	7.32	99	269819	26.10	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.48	67	163499	28.05	ng/ul	0.01
9) 2-Chlorophenol-d4	7.70	132	171750	24.87	ng/ul	0.01
13) 4-Methylphenol-d8	8.88	113	223035	27.77	ng/ul	0.01
19) Nitrobenzene-d5	9.34	128	98961	27.50	ng/ul	0.01
22) 2-Nitrophenol-d4	10.07	143	115422	26.59	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.61	165	230132	25.35	ng/ul	0.01
29) 4-Chloroaniline-d4	11.13	131	171188	22.27	ng/ul	0.01
43) Dimethylphthalate-d6	14.21	166	907720	31.27	ng/ul	0.01
46) Acenaphthylene-d8	14.51	160	1061040	31.89	ng/ul	0.01
51) 4-Nitrophenol-d4	15.00	143	153640	33.71	ng/ul	0.00
57) Fluorene-d10	15.80	176	919162	33.42	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.91	200	139516	25.82	ng/ul	0.00
70) Anthracene-d10	17.66	188	1432668	36.68	ng/ul	0.00
76) Pyrene-d10	19.93	212	1708760	37.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	1803863	38.87	ng/ul	0.01

Target Compounds

					Qvalue	
4) Benzaldehyde	7.30	77	212615	32.35	ng/ul	89
10) 2-Chlorophenol	7.73	128	25298	3.60	ng/ul#	83
28) Naphthalene	11.05	128	144283	6.25	ng/ul#	95
31) Hexachlorobutadiene	11.33	225	102402	14.57	ng/ul	95
33) 4-Chloro-3-methylphenol	12.26	107	141862	12.29	ng/ul#	82
36) 1,2,4,5-Tetrachlorobenzene	13.01	216	88272	6.61	ng/ul#	95
38) 2,4,6-Trichlorophenol	13.24	196	134027	14.55	ng/ul	92
40) 1,1'-Biphenyl	13.64	154	559428	20.59	ng/ul#	93
44) Dimethylphthalate	14.25	163	844735	28.50	ng/ul	98
45) 2,6-Dinitrotoluene	14.38	165	89333	13.92	ng/ul#	73
52) 4-Nitrophenol	15.02	109	210541	36.32	ng/ul#	60
53) Dibenzofuran	15.20	168	333870	9.50	ng/ul#	88
63) 4,6-Dinitro-2-methylphenol	15.92	198	97836	17.08	ng/ul#	90
66) Hexachlorobenzene	16.86	284	107230	9.01	ng/ul#	92
68) Pentachlorophenol	17.21	266	140493	20.54	ng/ul#	80
69) Phenanthrene	17.60	178	1109772	25.82	ng/ul	100
71) Anthracene	17.69	178	491058	11.12	ng/ul	98
73) Di-n-butylphthalate	18.50	149	742590	17.70	ng/ul#	95
74) Fluoranthene	19.60	202	1112691	24.85	ng/ul#	86
77) Pyrene	19.96	202	1139465	21.44	ng/ul#	85
81) Bis(2-ethylhexyl)phthalate	21.72	149	645090	24.25	ng/ul#	96
82) Chrysene	21.90	228	1002519	19.78	ng/ul	97
88) Benzo(a)pyrene	25.07	252	900289	15.52	ng/ul#	88

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022758.D
Acq On : 1 Jul 2016 13:03
Operator : UM/SJ
Sample : H3811-26
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
A4TX6

Manual Integrations

APPROVED
sohil
7/4/2016 1:30:38 PM

Quant Time: Jul 03 00:05:17 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 02 00:07:37 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
89) Indeno(1,2,3-cd)pyrene	29.07	276	1211435m	19.76	ng/ul	
90) Dibenzo(a,h)anthracene	29.14	278	636411m	12.55	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022758.D
Acq On : 1 Jul 2016 13:03
Operator : UM/SJ
Sample : H3811-26
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
A4TX6

Manual Integrations

sohil
7/4/2016 1:30:38 PM

Quant Time: Jul 03 00:05:17 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 02 00:07:37 2016
Response via : Initial Calibration

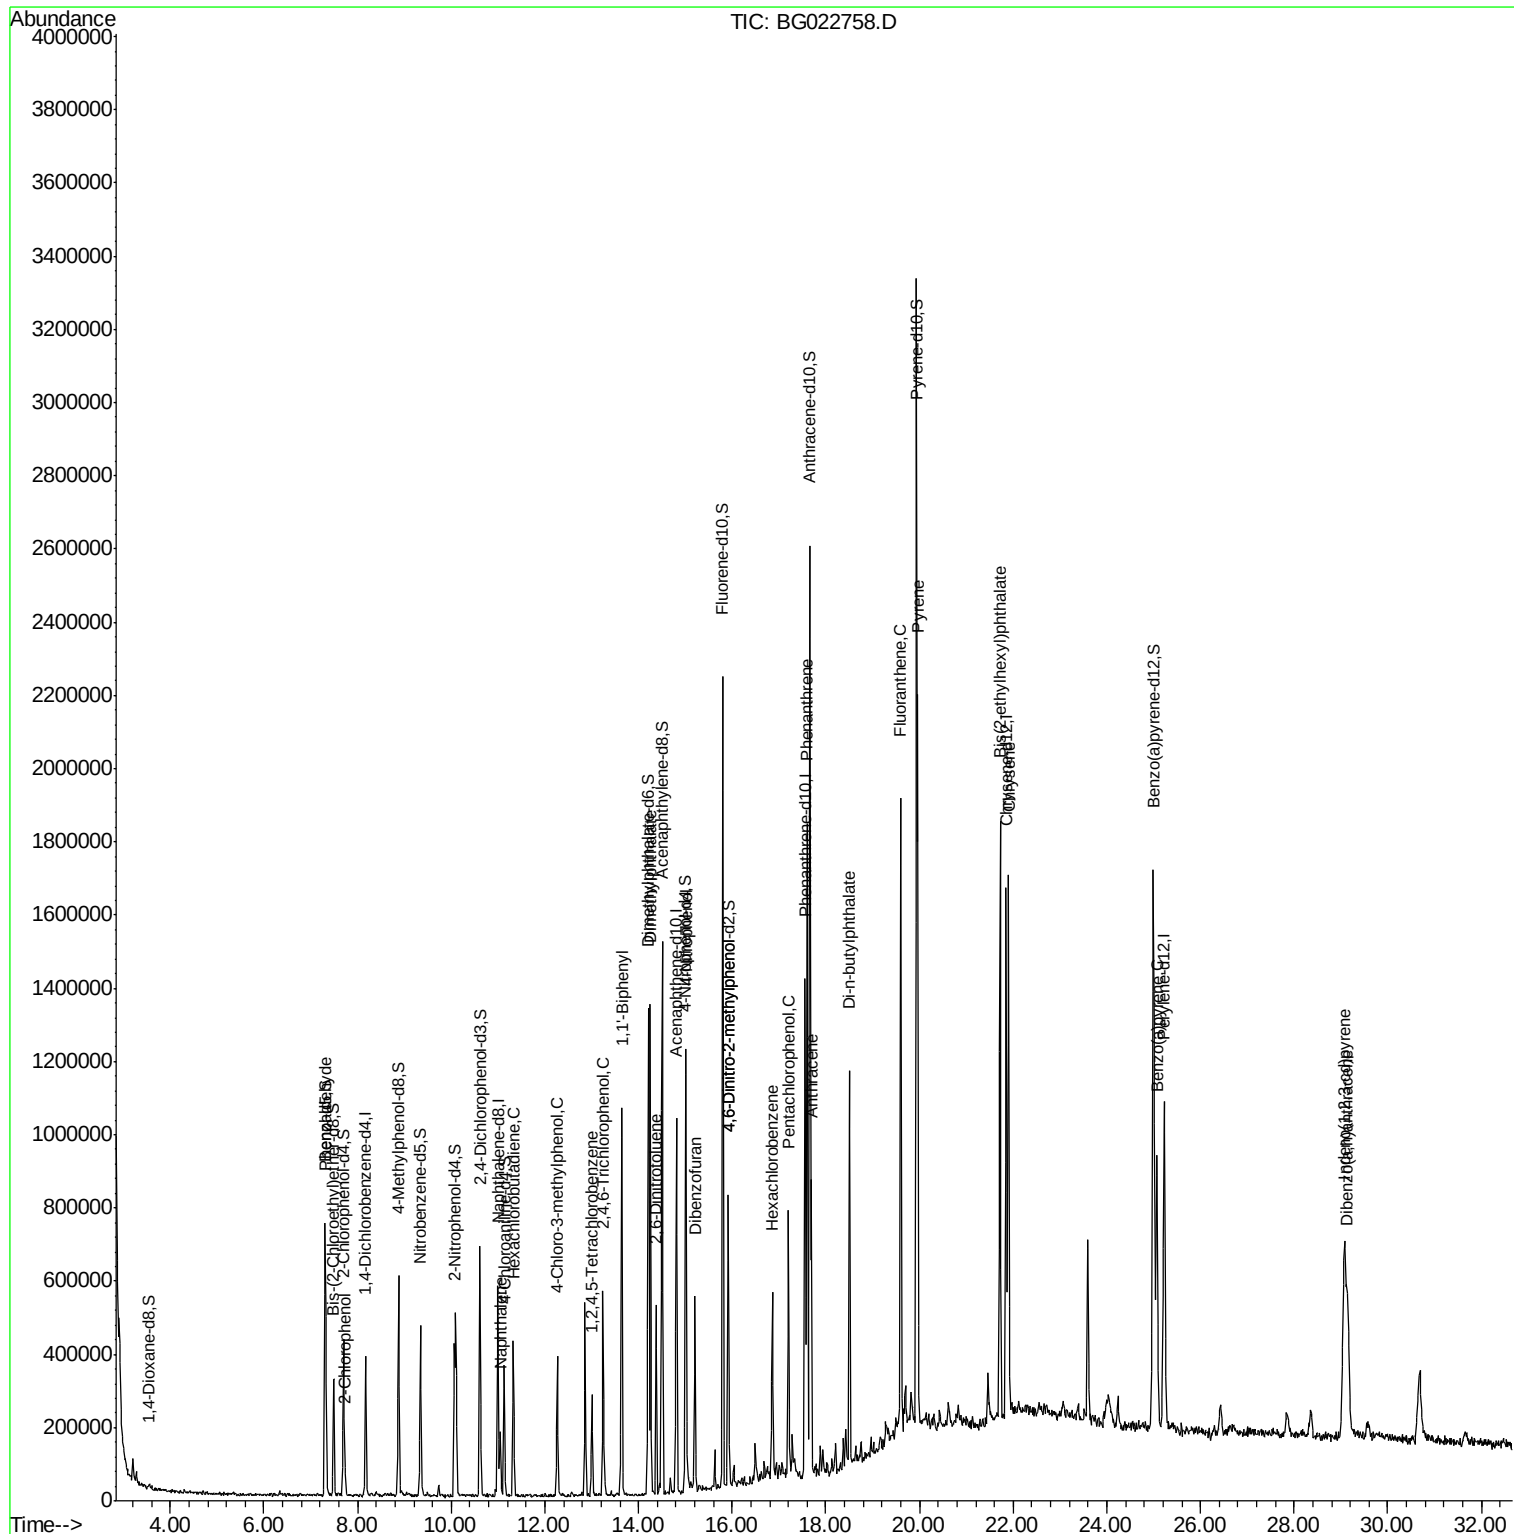

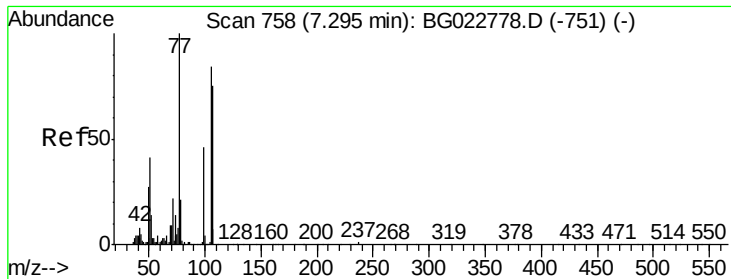

#4

Benzaldehyde

Concen: 32.35 ng/ul

RT: 7.30 min Scan# 760

Delta R.T. 0.01 min

Lab File: BG022758.D

Acq: 1 Jul 2016 13:03

Instrument :

BNA_G

ClientSampleId :





A4TX6

Tgt Ion:	77	Resp:	212615
Ion	Ratio	Lower	Upper
77	100		
105	92.9	83.8	125.8
106	87.2	77.9	116.9

Manual Integrations

sohil

7/4/2016 1:30:38 PM

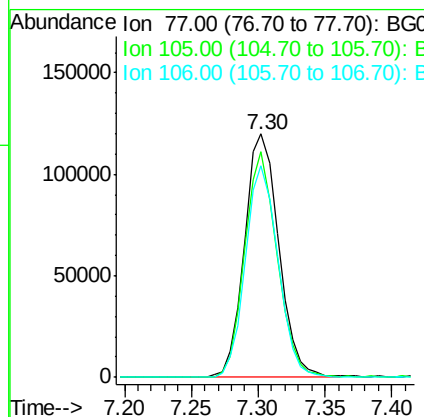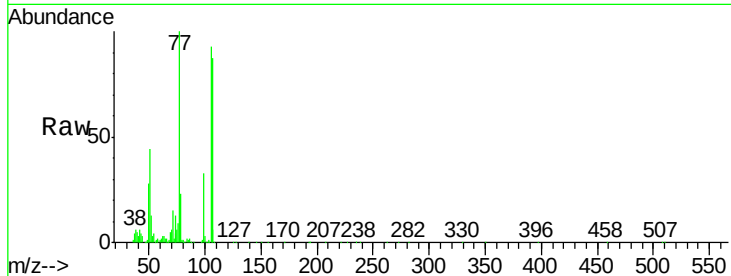

#10

2-Chlorophenol

Concen: 3.60 ng/ul




RT: 7.73 min Scan# 833


Delta R.T. 0.01 min

Lab File: BG022758.D

Acq: 1 Jul 2016 13:03

Tgt Ion:	128	Resp:	25298
Ion	Ratio	Lower	Upper
128	100		
64	57.5	34.2	51.4#
130	27.7	27.0	40.4

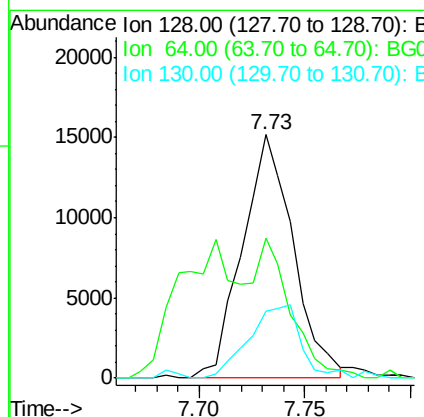

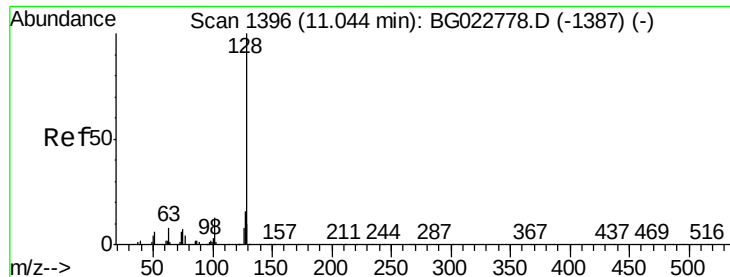





#28
Naphthalene
Concen: 6.25 ng/ul
RT: 11.05 min Scan# 1397
Delta R.T. 0.01 min
Lab File: BG022758.D
Acq: 1 Jul 2016 13:03

Instrument :
BNA_G
ClientSampled :
A4TX6

Tgt Ion	Ratio	Lower	Upper
128	100		
129	11.4	9.4	14.2
127	10.6	11.2	16.8#




Manual Integrations


sohil
7/4/2016 1:30:38 PM

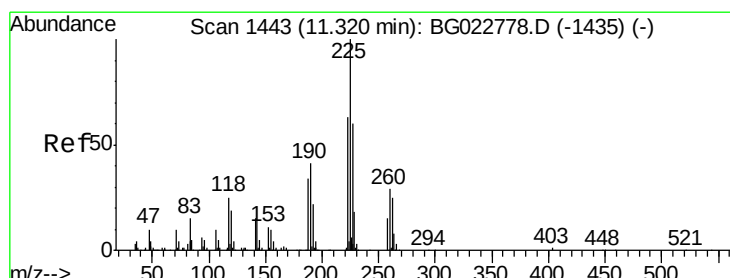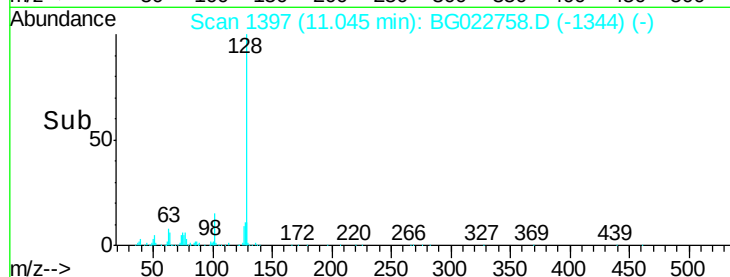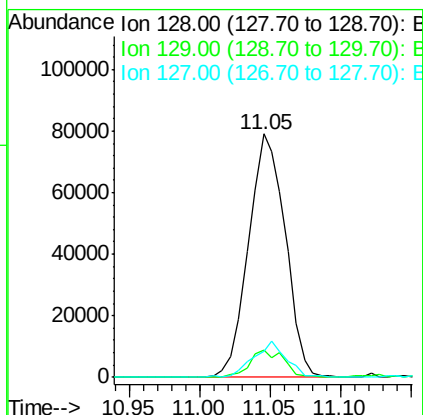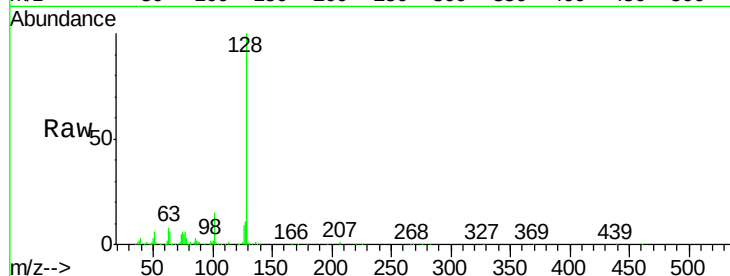

#31
Hexachlorobutadiene
Concen: 14.57 ng/ul
RT: 11.33 min Scan# 1445
Delta R.T. 0.01 min
Lab File: BG022758.D
Acq: 1 Jul 2016 13:03

Tgt Ion	Ratio	Lower	Upper
225	100		
223	61.6	54.7	82.1
227	64.5	52.2	78.4

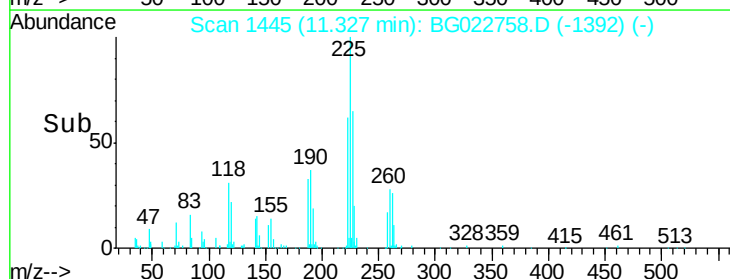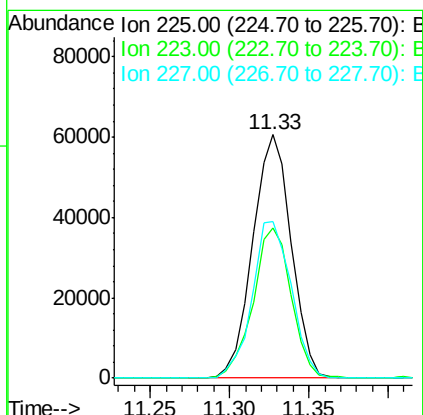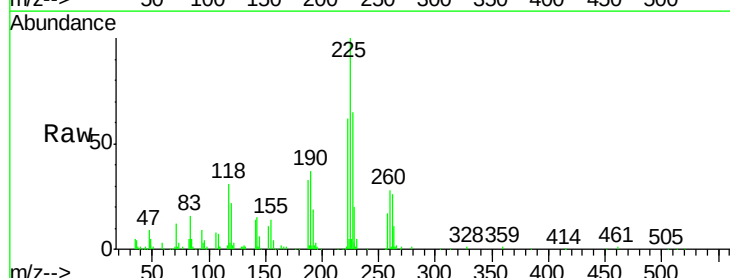







#33
4-Chloro-3-methylphenol
Concen: 12.29 ng/ul
RT: 12.26 min Scan# 1604
Delta R.T. 0.01 min
Lab File: BG022758.D
Acq: 1 Jul 2016 13:03

Instrument :
BNA_G
ClientSampleId :
A4TX6

Tgt Ion	Ratio	Lower	Upper
107	100		
144	22.9	22.7	34.1
142	69.8	71.6	107.4#




Manual Integrations


sohil
7/4/2016 1:30:38 PM

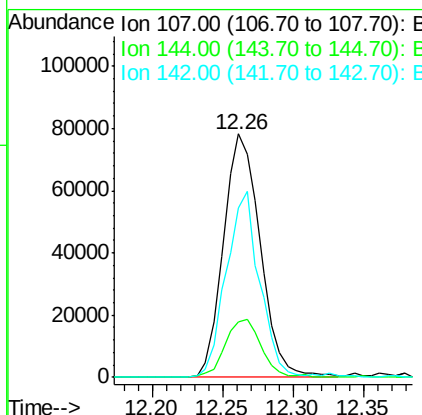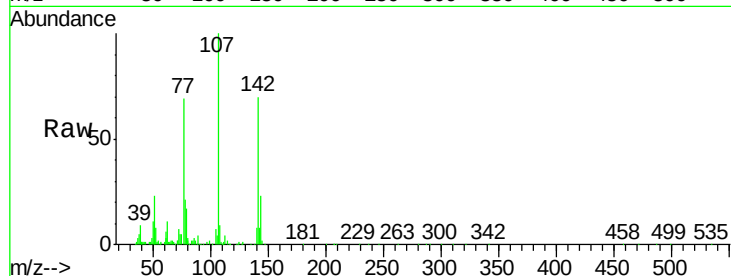

#36
1,2,4,5-Tetrachlorobenzene
Concen: 6.61 ng/ul
RT: 13.01 min Scan# 1731
Delta R.T. 0.01 min
Lab File: BG022758.D
Acq: 1 Jul 2016 13:03

Tgt Ion	Ratio	Lower	Upper
216	100		
214	73.4	61.7	92.5
179	21.9	17.0	25.4
108	12.7	14.2	21.2#

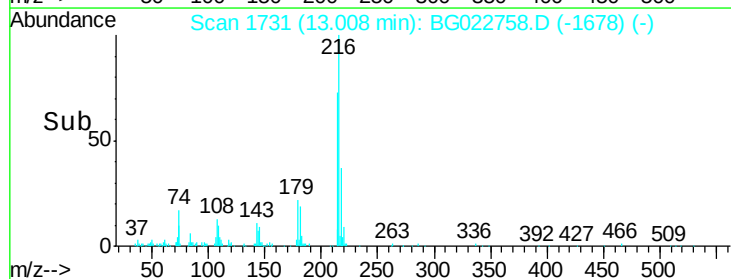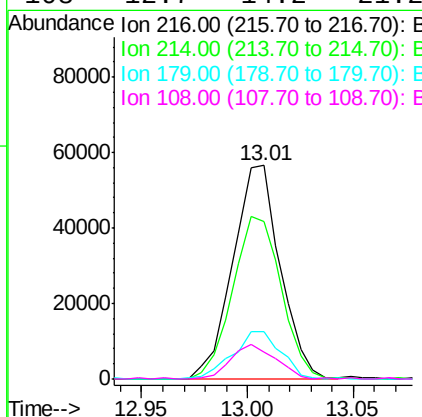







#38
 2,4,6-Trichlorophenol
 Concen: 14.55 ng/ul
 RT: 13.24 min Scan# 1771
 Delta R.T. 0.01 min
 Lab File: BG022758.D
 Acq: 1 Jul 2016 13:03

Instrument :
 BNA_G
 ClientSampleId :
 A4TX6

Tgt Ion	Ratio	Resp	Lower	Upper
196	100	134027		
198	104.6	77.4	116.0	
200	36.7	26.6	39.8	




Manual Integrations


sohil
 7/4/2016 1:30:38 PM

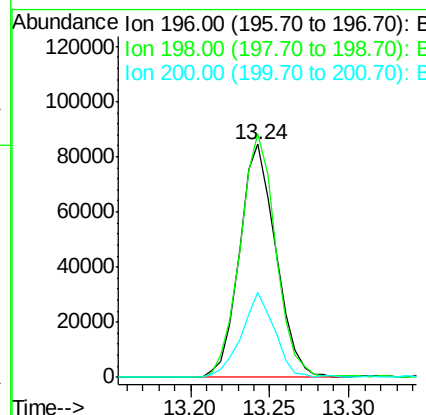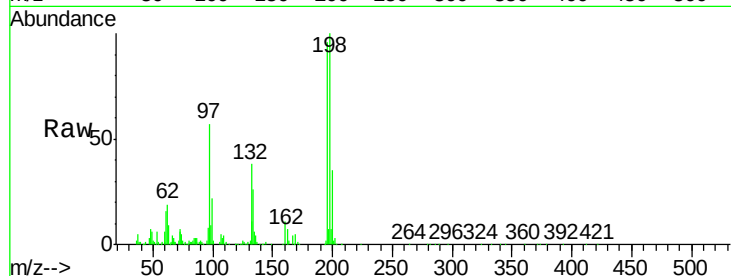

#40
 1,1'-Biphenyl
 Concen: 20.59 ng/ul
 RT: 13.64 min Scan# 1839
 Delta R.T. 0.01 min
 Lab File: BG022758.D
 Acq: 1 Jul 2016 13:03

Tgt Ion	Ratio	Resp	Lower	Upper
154	100	559428		
153	38.8	34.6	52.0	
76	11.7	11.9	17.9	

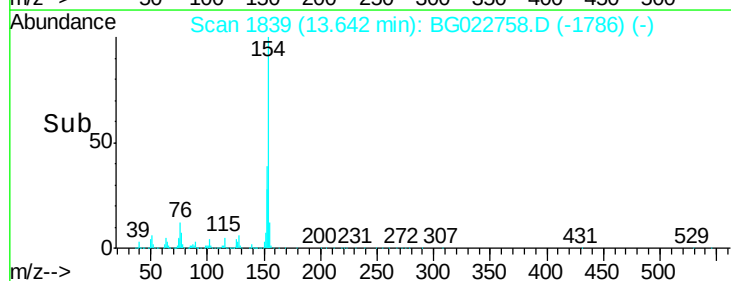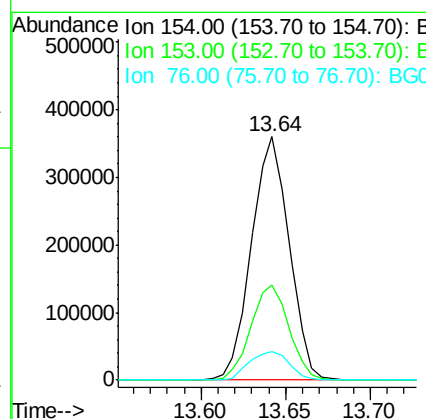

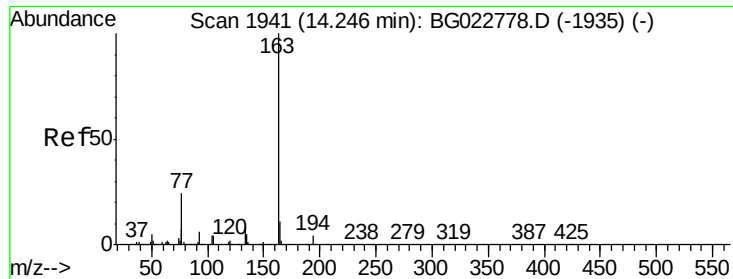





#44
Dimethylphthalate
Concen: 28.50 ng/ul
RT: 14.25 min Scan# 1943
Delta R.T. 0.01 min
Lab File: BG022758.D
Acq: 1 Jul 2016 13:03

Instrument :
BNA_G
ClientSampleId :
A4TX6

Tgt Ion	Ratio	Lower	Upper
163	100		
194	5.1	3.4	5.2
164	11.6	8.8	13.2




Manual Integrations


sohil
7/4/2016 1:30:38 PM

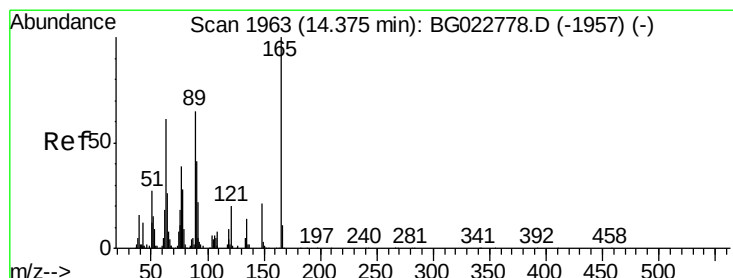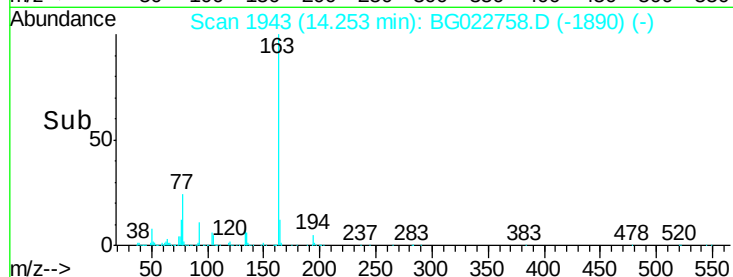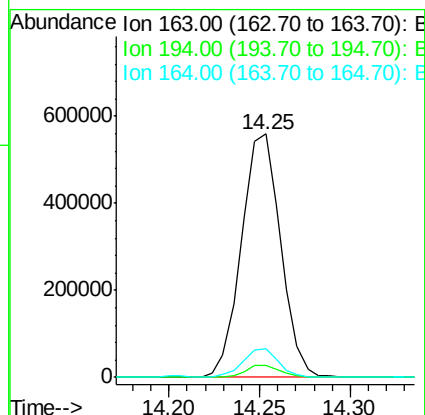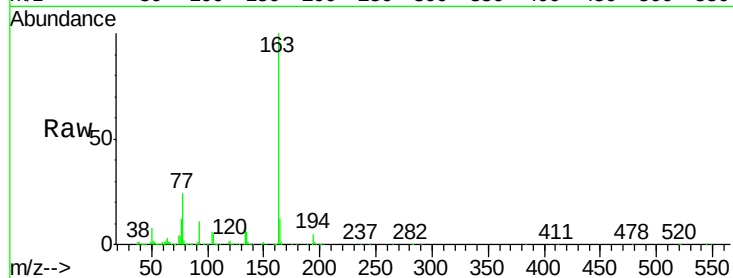

#45
2,6-Dinitrotoluene
Concen: 13.92 ng/ul
RT: 14.38 min Scan# 1964
Delta R.T. 0.01 min
Lab File: BG022758.D
Acq: 1 Jul 2016 13:03

Tgt Ion	Ratio	Lower	Upper
165	100		
89	76.8	41.5	62.3#
121	24.0	17.0	25.4

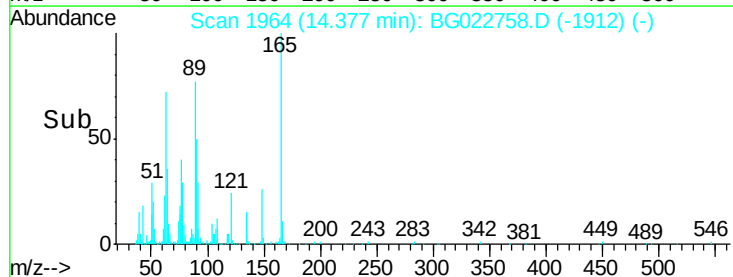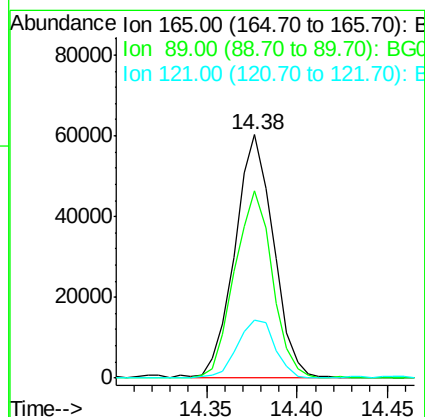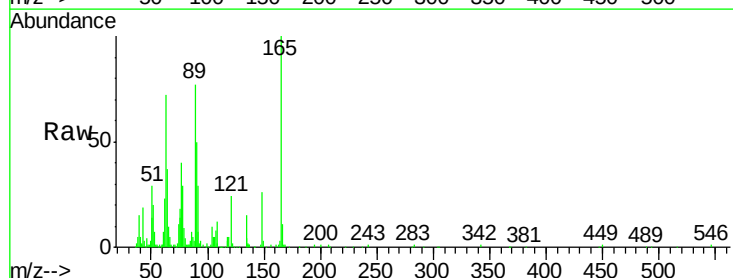







#52
4-Nitrophenol
Concen: 36.32 ng/ul
RT: 15.02 min Scan# 2073
Delta R.T. 0.01 min
Lab File: BG022758.D
Acq: 1 Jul 2016 13:03

Instrument :
BNA_G
ClientSampleId :
A4TX6

Tgt Ion	Ratio	Lower	Upper
109	100		
139	87.3	136.1	204.1#
65	115.8	106.0	159.0




Manual Integrations


sohil
7/4/2016 1:30:38 PM

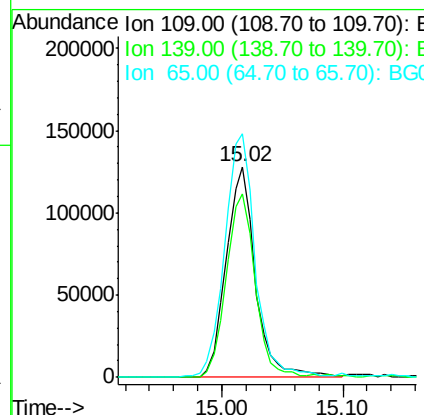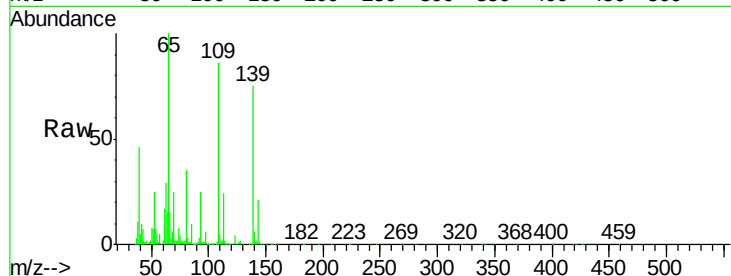

#53
Dibenzofuran
Concen: 9.50 ng/ul
RT: 15.20 min Scan# 2105
Delta R.T. 0.01 min
Lab File: BG022758.D
Acq: 1 Jul 2016 13:03

Tgt Ion	Ratio	Lower	Upper
168	100		
139	41.3	27.4	41.0#

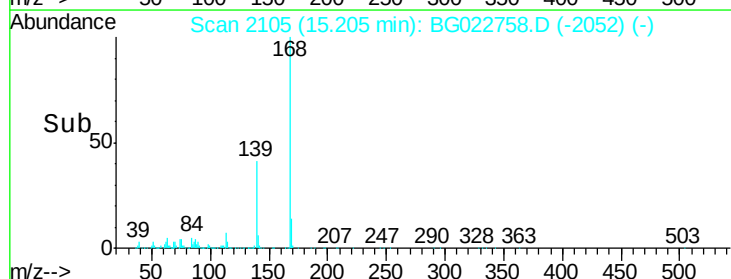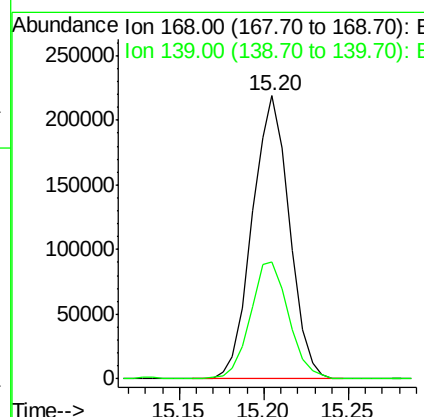

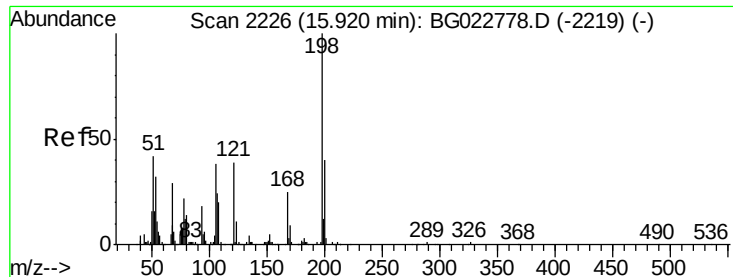

#63

4,6-Dinitro-2-methylphenol

Concen: 17.08 ng/ul

RT: 15.92 min Scan# 2227

Delta R.T. 0.01 min

Lab File: BG022758.D

Acq: 1 Jul 2016 13:03

Instrument :

BNA_G

ClientSampleId :

A4TX6

Tgt Ion:198 Resp: 97836

Ion Ratio Lower Upper

198 100


182 5.3 4.2 6.2

77 26.7 16.7 25.1#

Manual Integrations

sohil




7/4/2016 1:30:38 PM

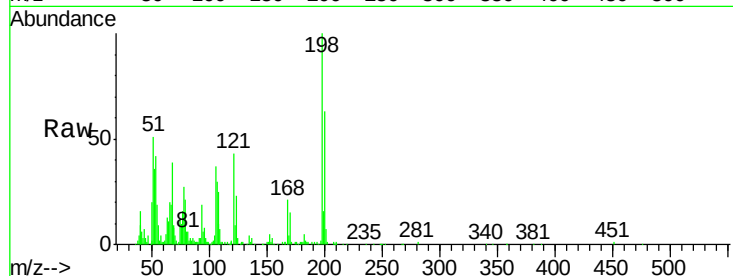

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 182.00 (181.70 to 182.70): E

Ion 77.00 (76.70 to 77.70): B

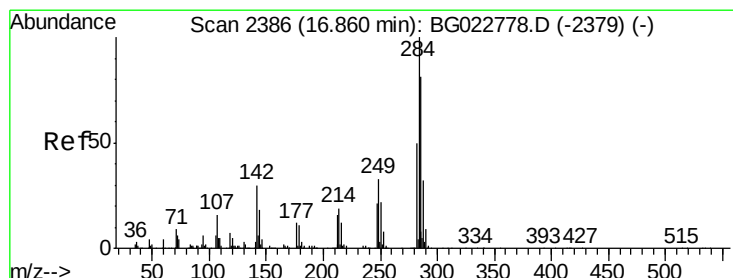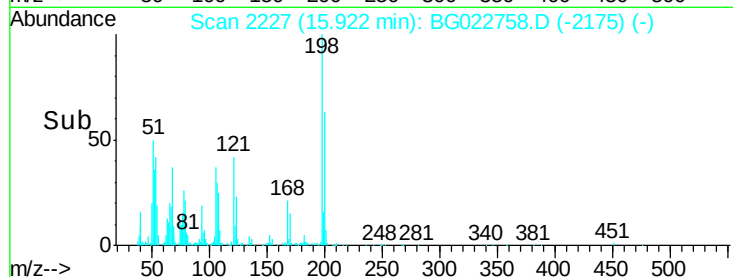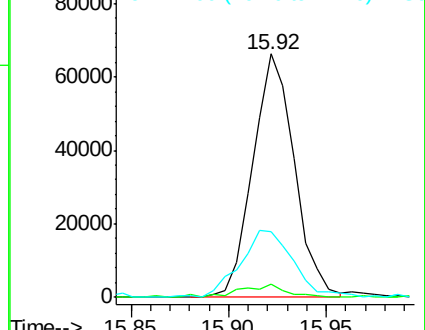

#66

Hexachlorobenzene

Concen: 9.01 ng/ul

RT: 16.86 min Scan# 2386

Delta R.T. 0.01 min

Lab File: BG022758.D

Acq: 1 Jul 2016 13:03


Tgt Ion:284 Resp: 107230

Ion Ratio Lower Upper

284 100

142 27.8 27.8 41.8#



249 28.8 24.4 36.6

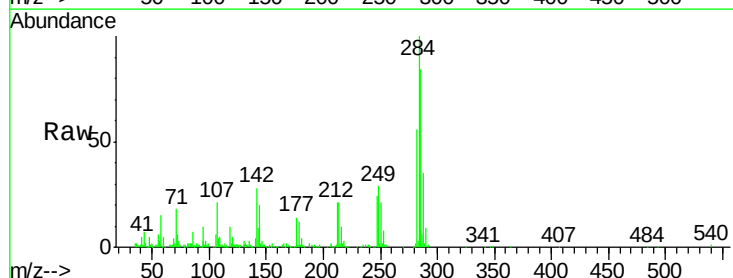


Abundance Ion 284.00 (283.70 to 284.70): E

Ion 142.00 (141.70 to 142.70): E

Ion 249.00 (248.70 to 249.70): E

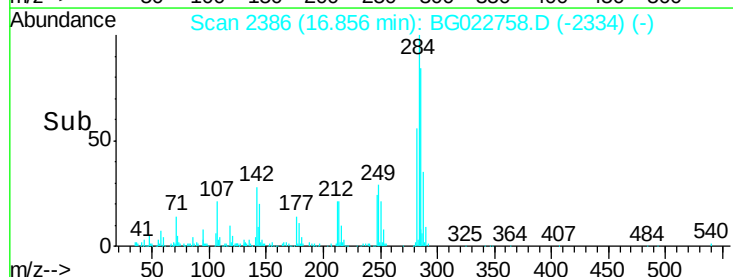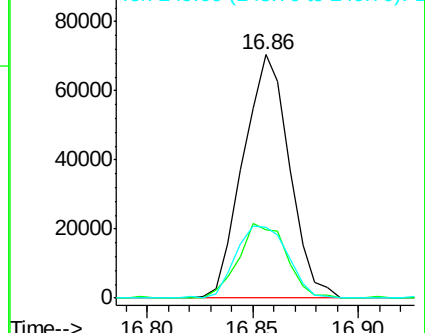

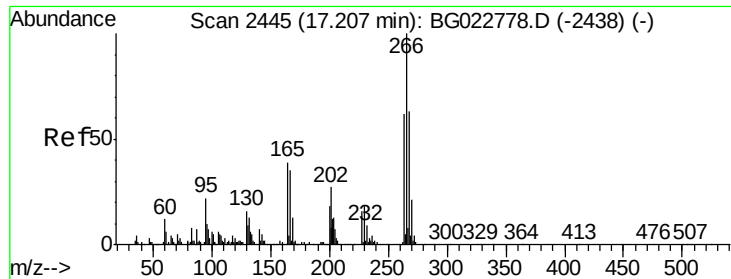





#68
 Pentachlorophenol
 Concen: 20.54 ng/ul
 RT: 17.21 min Scan# 2446
 Delta R.T. 0.01 min
 Lab File: BG022758.D
 Acq: 1 Jul 2016 13:03

Instrument :
 BNA_G
 ClientSampleId :
 A4TX6

Tgt Ion	Ratio	Lower	Upper
266	100		
264	51.7	54.7	82.1#
268	56.1	57.8	86.8#




Manual Integrations


sohil
 7/4/2016 1:30:38 PM

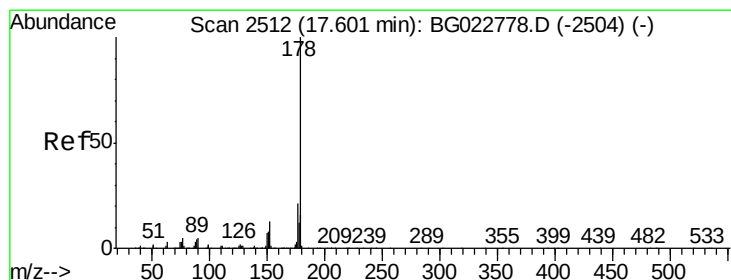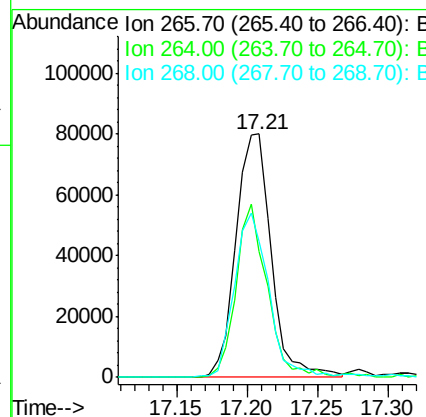

#69
 Phenanthrene
 Concen: 25.82 ng/ul
 RT: 17.60 min Scan# 2512
 Delta R.T. 0.01 min
 Lab File: BG022758.D
 Acq: 1 Jul 2016 13:03

Tgt Ion	Ratio	Lower	Upper
178	100		
179	16.0	12.9	19.3
176	19.5	15.8	23.8

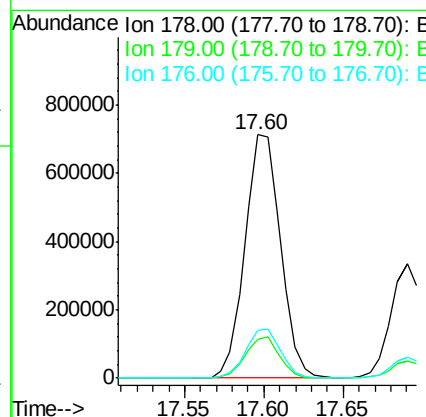

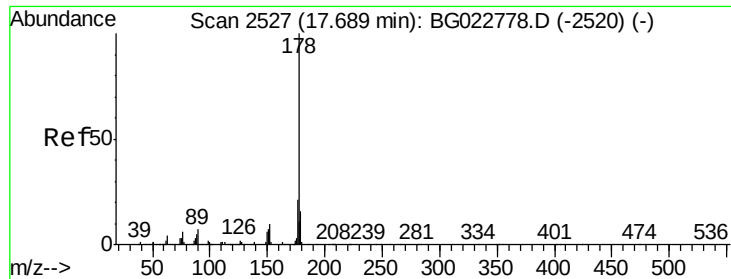

#71

Anthracene

Concen: 11.12 ng/ul

RT: 17.69 min Scan# 2528

Delta R.T. 0.01 min

Lab File: BG022758.D


Acq: 1 Jul 2016 13:03

Instrument :

BNA_G

ClientSampleId :




A4TX6

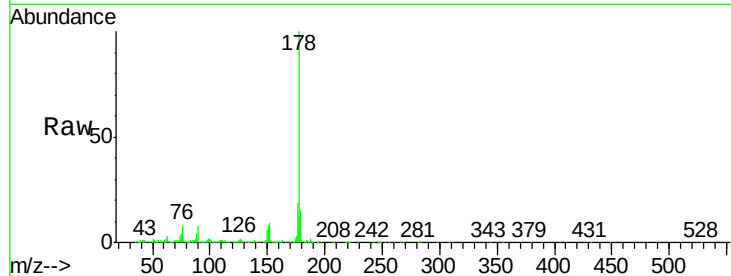

Tgt Ion:	178	Resp:	491058
Ion Ratio	Lower	Upper	
178	100		
179	15.3	12.3	18.5
176	18.6	16.3	24.5

Manual Integrations

sohil
7/4/2016 1:30:38 PM

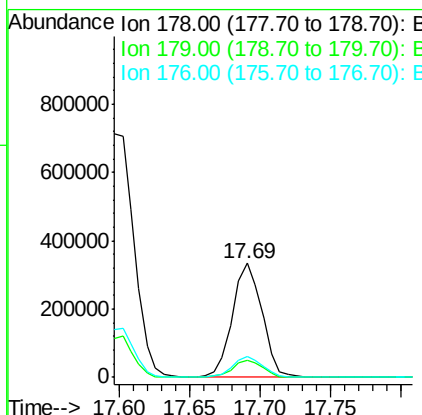

#73

Di-n-butylphthalate

Concen: 17.70 ng/ul




RT: 18.50 min Scan# 2666


Delta R.T. 0.01 min

Lab File: BG022758.D

Acq: 1 Jul 2016 13:03

Tgt Ion:	149	Resp:	742590
Ion Ratio	Lower	Upper	
149	100		
150	10.3	7.1	10.7
104	6.9	3.3	4.9#

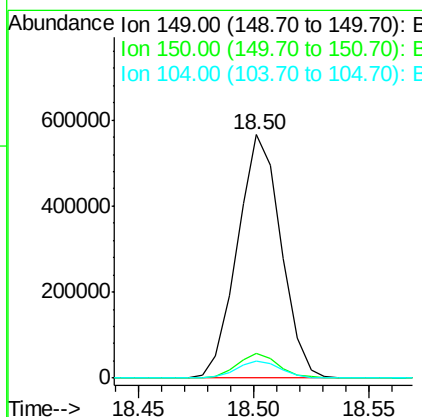

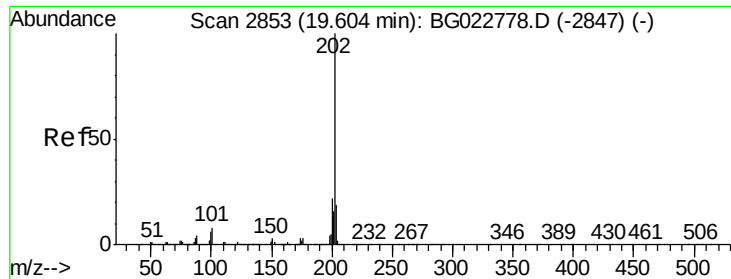

#74

Fluoranthene

Concen: 24.85 ng/ul

RT: 19.60 min Scan# 2853

Delta R.T. 0.01 min

Lab File: BG022758.D

Acq: 1 Jul 2016 13:03

Instrument :

BNA_G

ClientSampleId :

A4TX6

Tgt Ion:202 Resp: 1112691

Ion Ratio Lower Upper

202 100


101 6.9 10.6 16.0#

100 6.5 8.7 13.1#

Manual Integrations

sohil




7/4/2016 1:30:38 PM

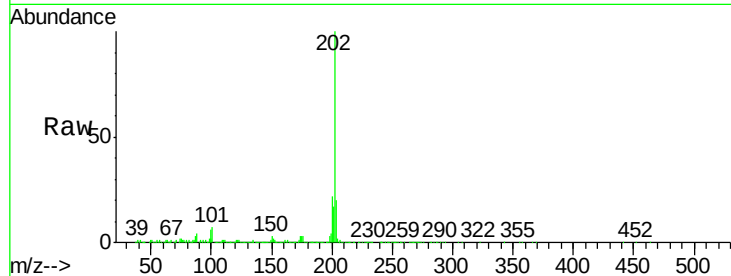

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

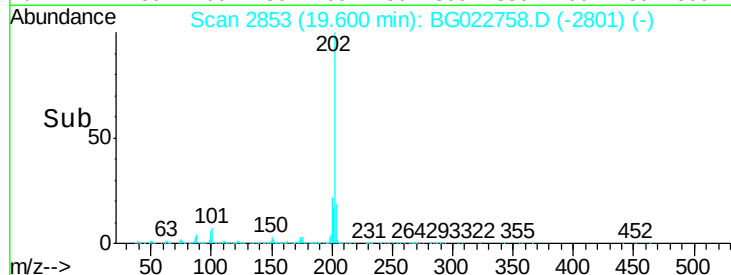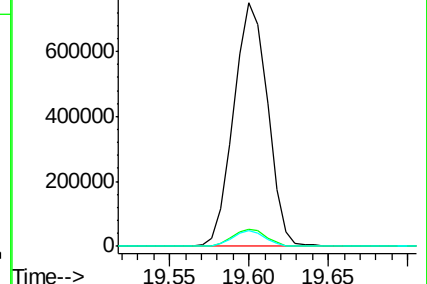

#77

Pyrene

Concen: 21.44 ng/ul

RT: 19.96 min Scan# 2915

Delta R.T. 0.01 min

Lab File: BG022758.D

Acq: 1 Jul 2016 13:03


Tgt Ion:202 Resp: 1139465

Ion Ratio Lower Upper

202 100

101 9.1 12.5 18.7#



100 7.5 10.2 15.4#




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

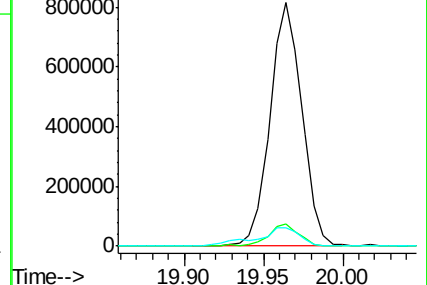







#81
 Bis(2-ethylhexyl)phthalate
 Concen: 24.25 ng/ul
 RT: 21.72 min Scan# 3214
 Delta R.T. 0.01 min
 Lab File: BG022758.D
 Acq: 1 Jul 2016 13:03

Instrument :
 BNA_G
 ClientSampleId :
 A4TX6

Tgt Ion	Ratio	Lower	Upper
149	100		
167	29.2	21.9	32.9
279	6.2	2.9	4.3#




Manual Integrations


sohil
 7/4/2016 1:30:38 PM

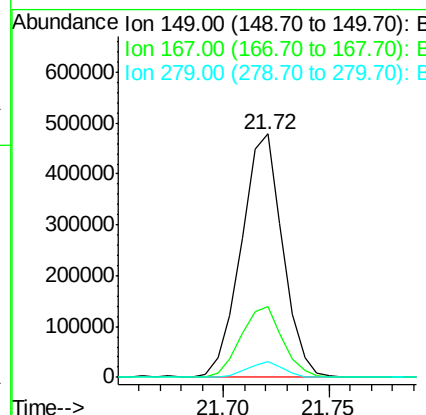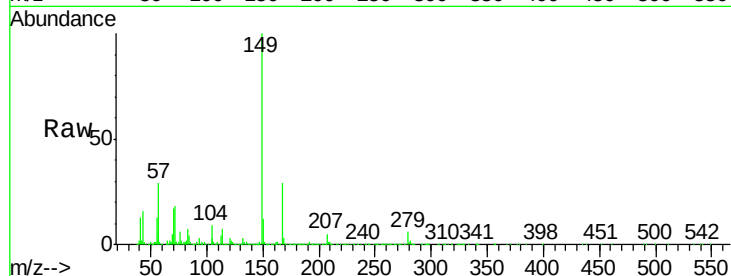

#82
 Chrysene
 Concen: 19.78 ng/ul
 RT: 21.90 min Scan# 3245
 Delta R.T. 0.01 min
 Lab File: BG022758.D
 Acq: 1 Jul 2016 13:03

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.6	24.2	36.4
229	20.4	15.0	22.6

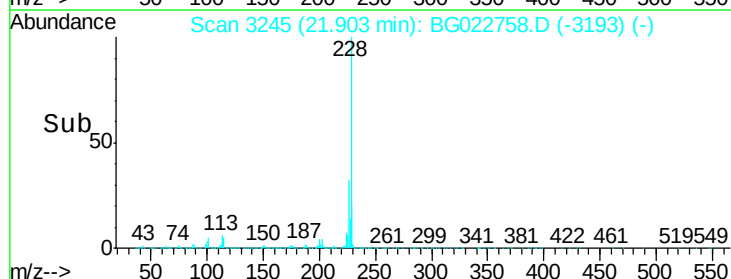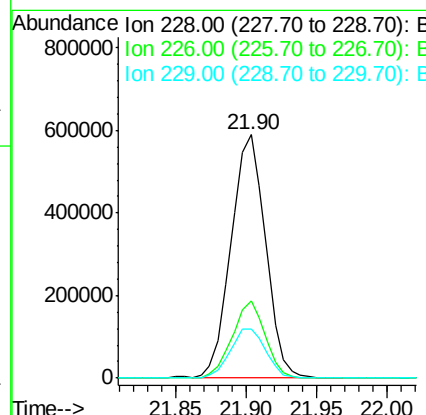

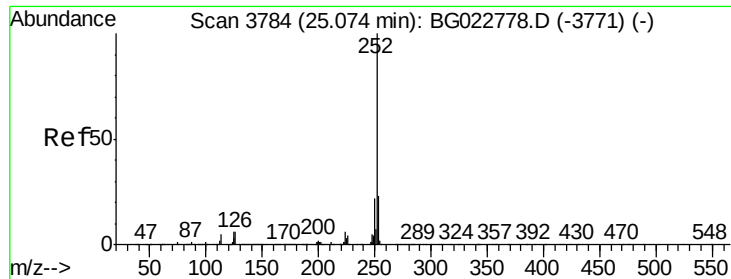





#88
Benzo(a)pyrene
Concen: 15.52 ng/ul
RT: 25.07 min Scan# 3784
Delta R.T. 0.02 min
Lab File: BG022758.D
Acq: 1 Jul 2016 13:03

Instrument :
BNA_G
ClientSampleId :
A4TX6

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.1	19.0	28.4
125	5.4	12.0	18.0




Manual Integrations


sohil
7/4/2016 1:30:38 PM

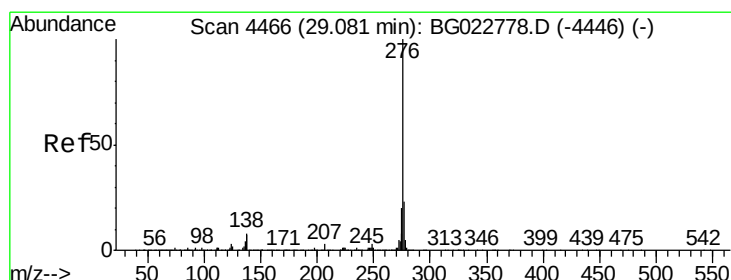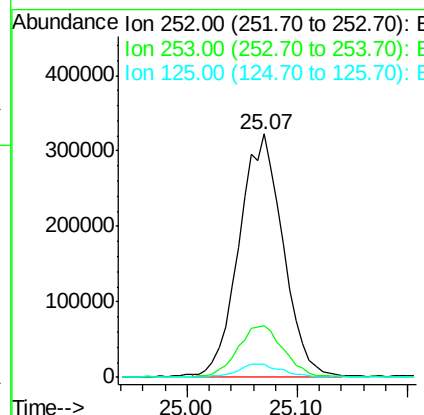

#89
Indeno(1,2,3-cd)pyrene
Concen: 19.76 ng/ul m
RT: 29.07 min Scan# 4465
Delta R.T. 0.01 min
Lab File: BG022758.D
Acq: 1 Jul 2016 13:03

Tgt Ion	Ratio	Lower	Upper
276	100		
138	7.5	20.8	31.2
277	24.8	17.6	26.4

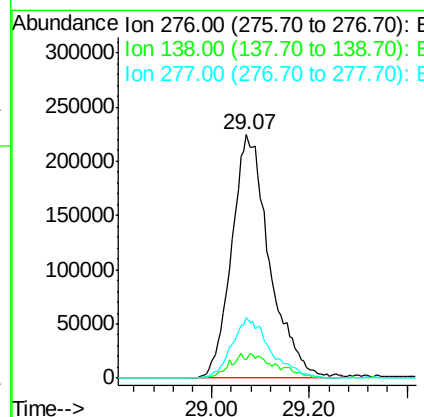

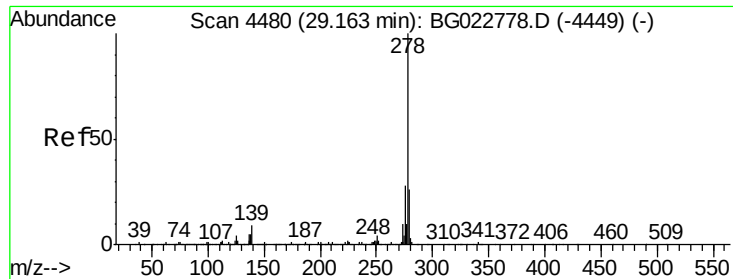

#90

Dibenzo(a,h)anthracene

Concen: 12.55 ng/ul m

RT: 29.14 min Scan# 4477

Delta R.T. 0.02 min

Lab File: BG022758.D


Acq: 1 Jul 2016 13:03

Instrument :

BNA_G

ClientSampleId :

A4TX6

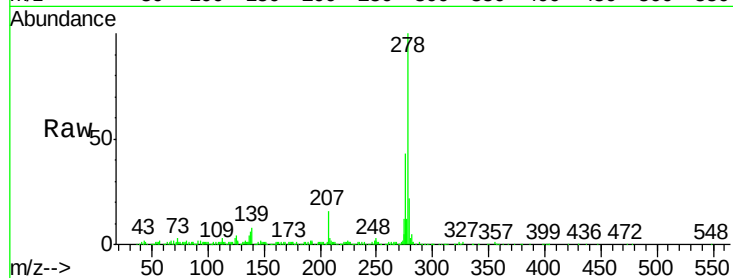

Tgt	Ion	278	Resp	636411
	Ratio	100	Lower	Upper
	278	100		
	139	8.4	16.3	24.5#
	279	22.4	19.1	28.7

Manual Integrations

sohil

7/4/2016 1:30:38 PM

