

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
 Data File : BG022771.D
 Acq On : 1 Jul 2016 23:46
 Operator : UM/SJ
 Sample : H3811-21
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 A4TW9

Manual Integrations

sohil
 7/4/2016 1:31:16 PM

Quant Time: Jul 02 01:44:08 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 02 00:07:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	147181	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	681479	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	553481	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.56	188	1317038m	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1480059m	20.00	ng/ul	0.00
83) Perylene-d12	25.22	264	1525726	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	6048	2.30	ng/uL	0.00
5) Phenol-d5	7.31	99	406249	26.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.47	67	235588	26.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	261852	25.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	326262	27.13	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	138973	25.57	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	171045	26.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	351034	25.61	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	335551	28.91	ng/ul	0.00
43) Dimethylphthalate-d6	14.20	166	1175219	26.14	ng/ul	0.00
46) Acenaphthylene-d8	14.50	160	1345570	26.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	195050	27.63	ng/ul	0.00
57) Fluorene-d10	15.79	176	1122561	26.35	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.91	200	224027m	26.45	ng/ul	0.00
70) Anthracene-d10	17.65	188	1597321	26.09	ng/ul	0.00
76) Pyrene-d10	19.94	212	1868325m	26.42	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.99	264	1898628	26.19	ng/ul	0.01

Target Compounds					Qvalue
44) Dimethylphthalate	14.24	163	352104	7.67 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022771.D
Acq On : 1 Jul 2016 23:46
Operator : UM/SJ
Sample : H3811-21
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
A4TW9

Manual Integrations

Quant Time: Jul 02 01:44:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 02 00:07:37 2016
Response via : Initial Calibration

sohil
7/4/2016 1:31:16 PM

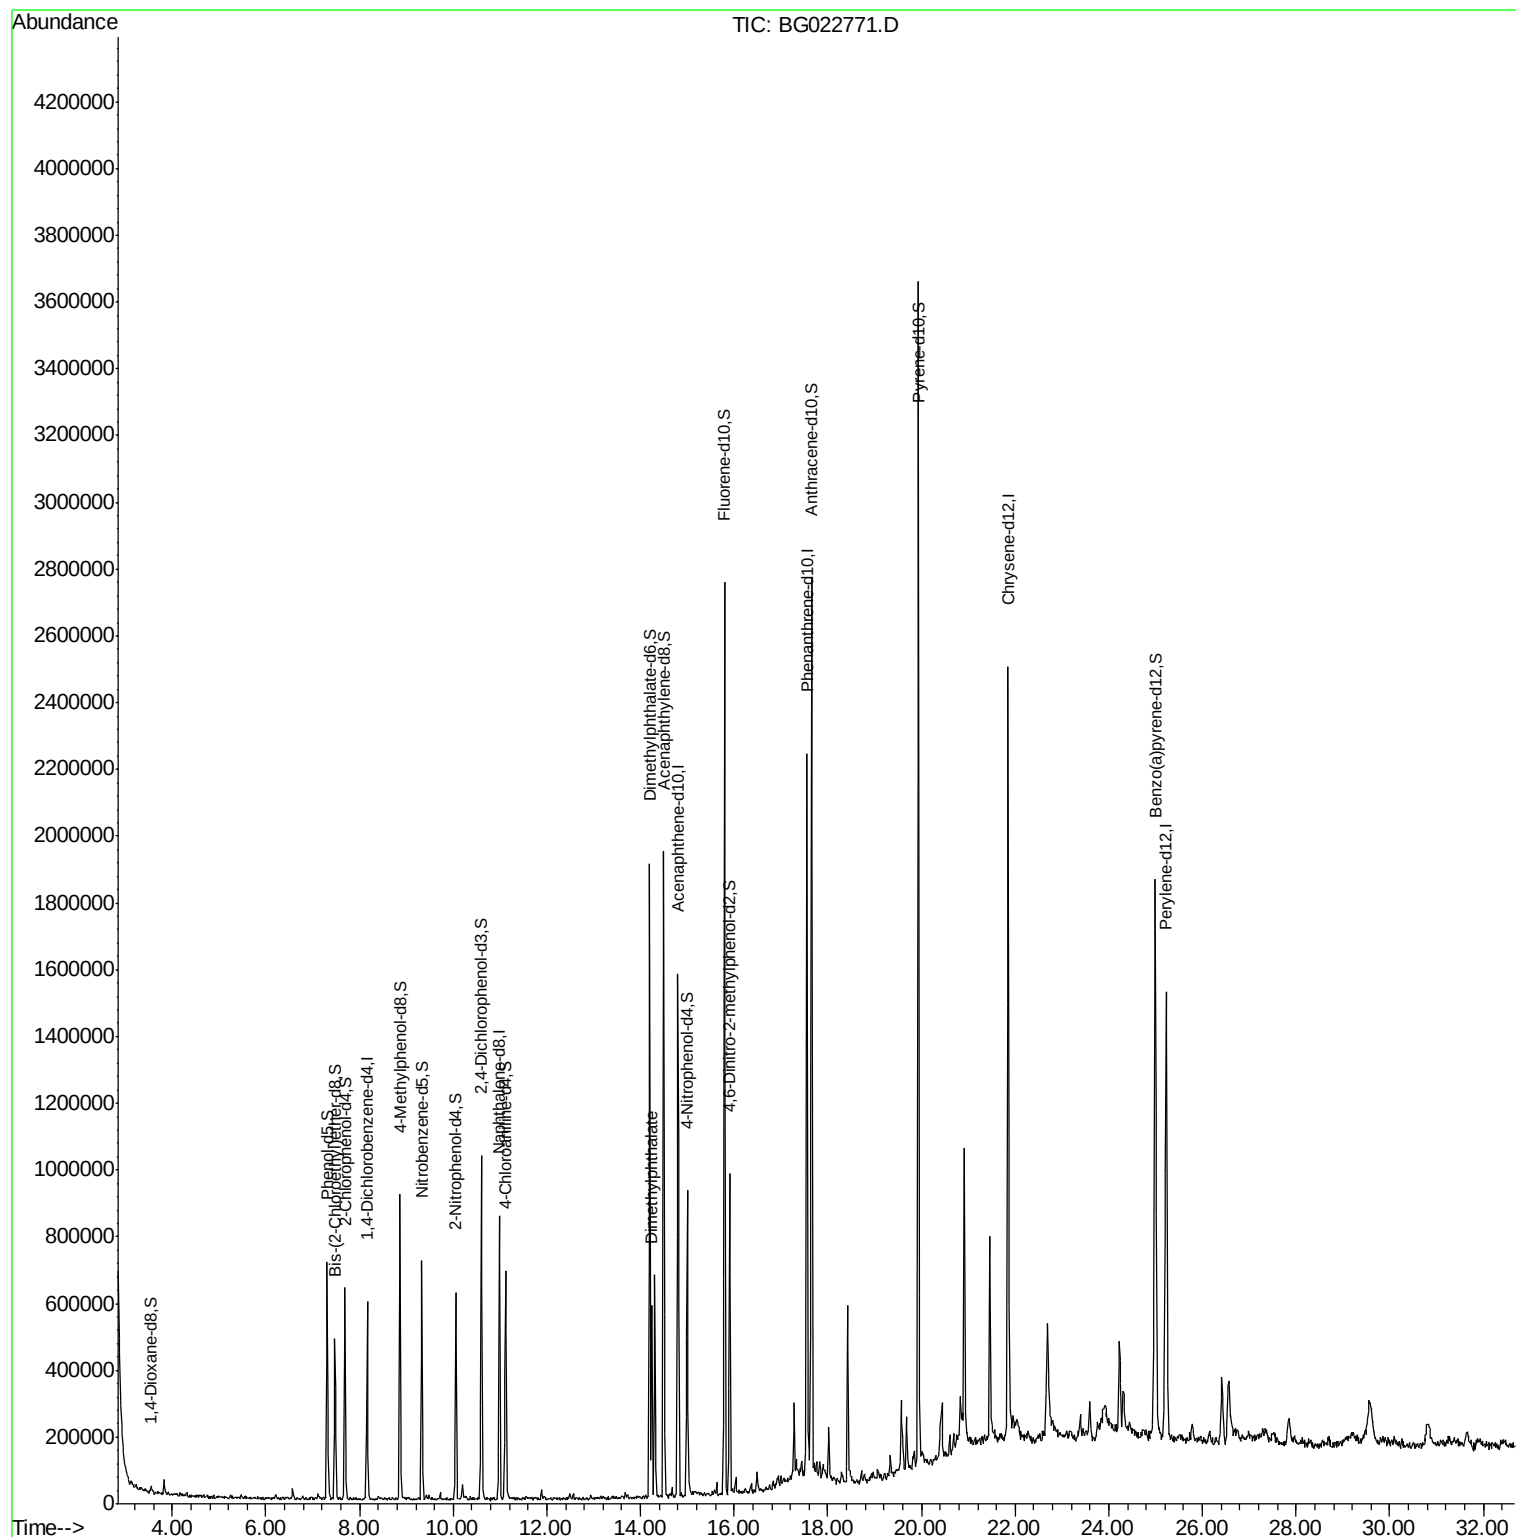

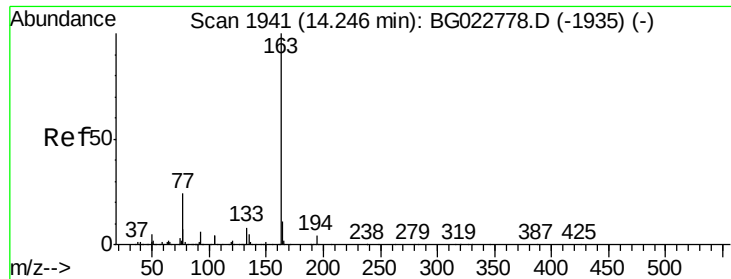

#44

Dimethylphthalate

Concen: 7.67 ng/ul

RT: 14.24 min Scan# 1941

Delta R.T. 0.00 min

Lab File: BG022771.D


Acq: 1 Jul 2016 23:46

Instrument :

BNA_G

ClientSampleId :

A4TW9

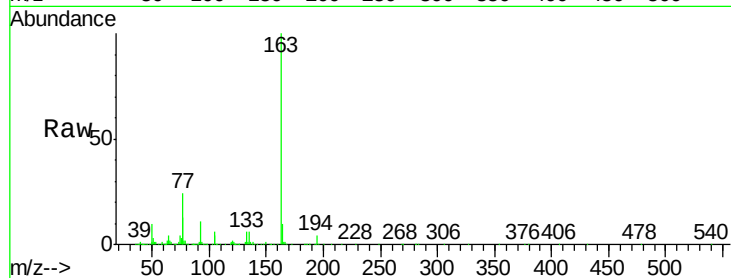

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.2
164	9.8	8.8	13.2

Manual Integrations

sohil

7/4/2016 1:31:16 PM

