

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
 Data File : BG022780.D
 Acq On : 2 Jul 2016 5:48
 Operator : UM/SJ
 Sample : H3752-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHM3

Manual Integrations

sohil
 7/4/2016 1:32:22 PM

Quant Time: Jul 02 06:34:07 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 02 00:07:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	133313	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	566504	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.80	164	443406	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.55	188	1156230m	20.00	ng/ul	0.00
75) Chrysene-d12	21.85	240	1341245m	20.00	ng/ul	0.00
83) Perylene-d12	25.22	264	1362492	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	6065m	2.54	ng/uL	0.00
5) Phenol-d5	7.31	99	307526	21.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	177997	22.51	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	201368	21.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	234386	21.52	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	98598	21.83	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	120194	22.06	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	245977	21.59	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	278942	28.91	ng/ul	0.00
43) Dimethylphthalate-d6	14.20	166	836227	23.21	ng/ul	0.00
46) Acenaphthylene-d8	14.50	160	949089	22.99	ng/ul	0.00
51) 4-Nitrophenol-d4	14.99	143	123753	21.88	ng/ul	0.00
57) Fluorene-d10	15.79	176	824263	24.15	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.90	200	119620m	16.09	ng/ul	0.00
70) Anthracene-d10	17.65	188	1289624	24.00	ng/ul	0.00
76) Pyrene-d10	19.93	212	1551114	24.21	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.98	264	1543941	23.85	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	14.24	163	188291	5.12 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022780.D
Acq On : 2 Jul 2016 5:48
Operator : UM/SJ
Sample : H3752-07
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDHM3

Manual Integrations

sohil
7/4/2016 1:32:22 PM


Quant Time: Jul 02 06:34:07 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 02 00:07:37 2016
Response via : Initial Calibration

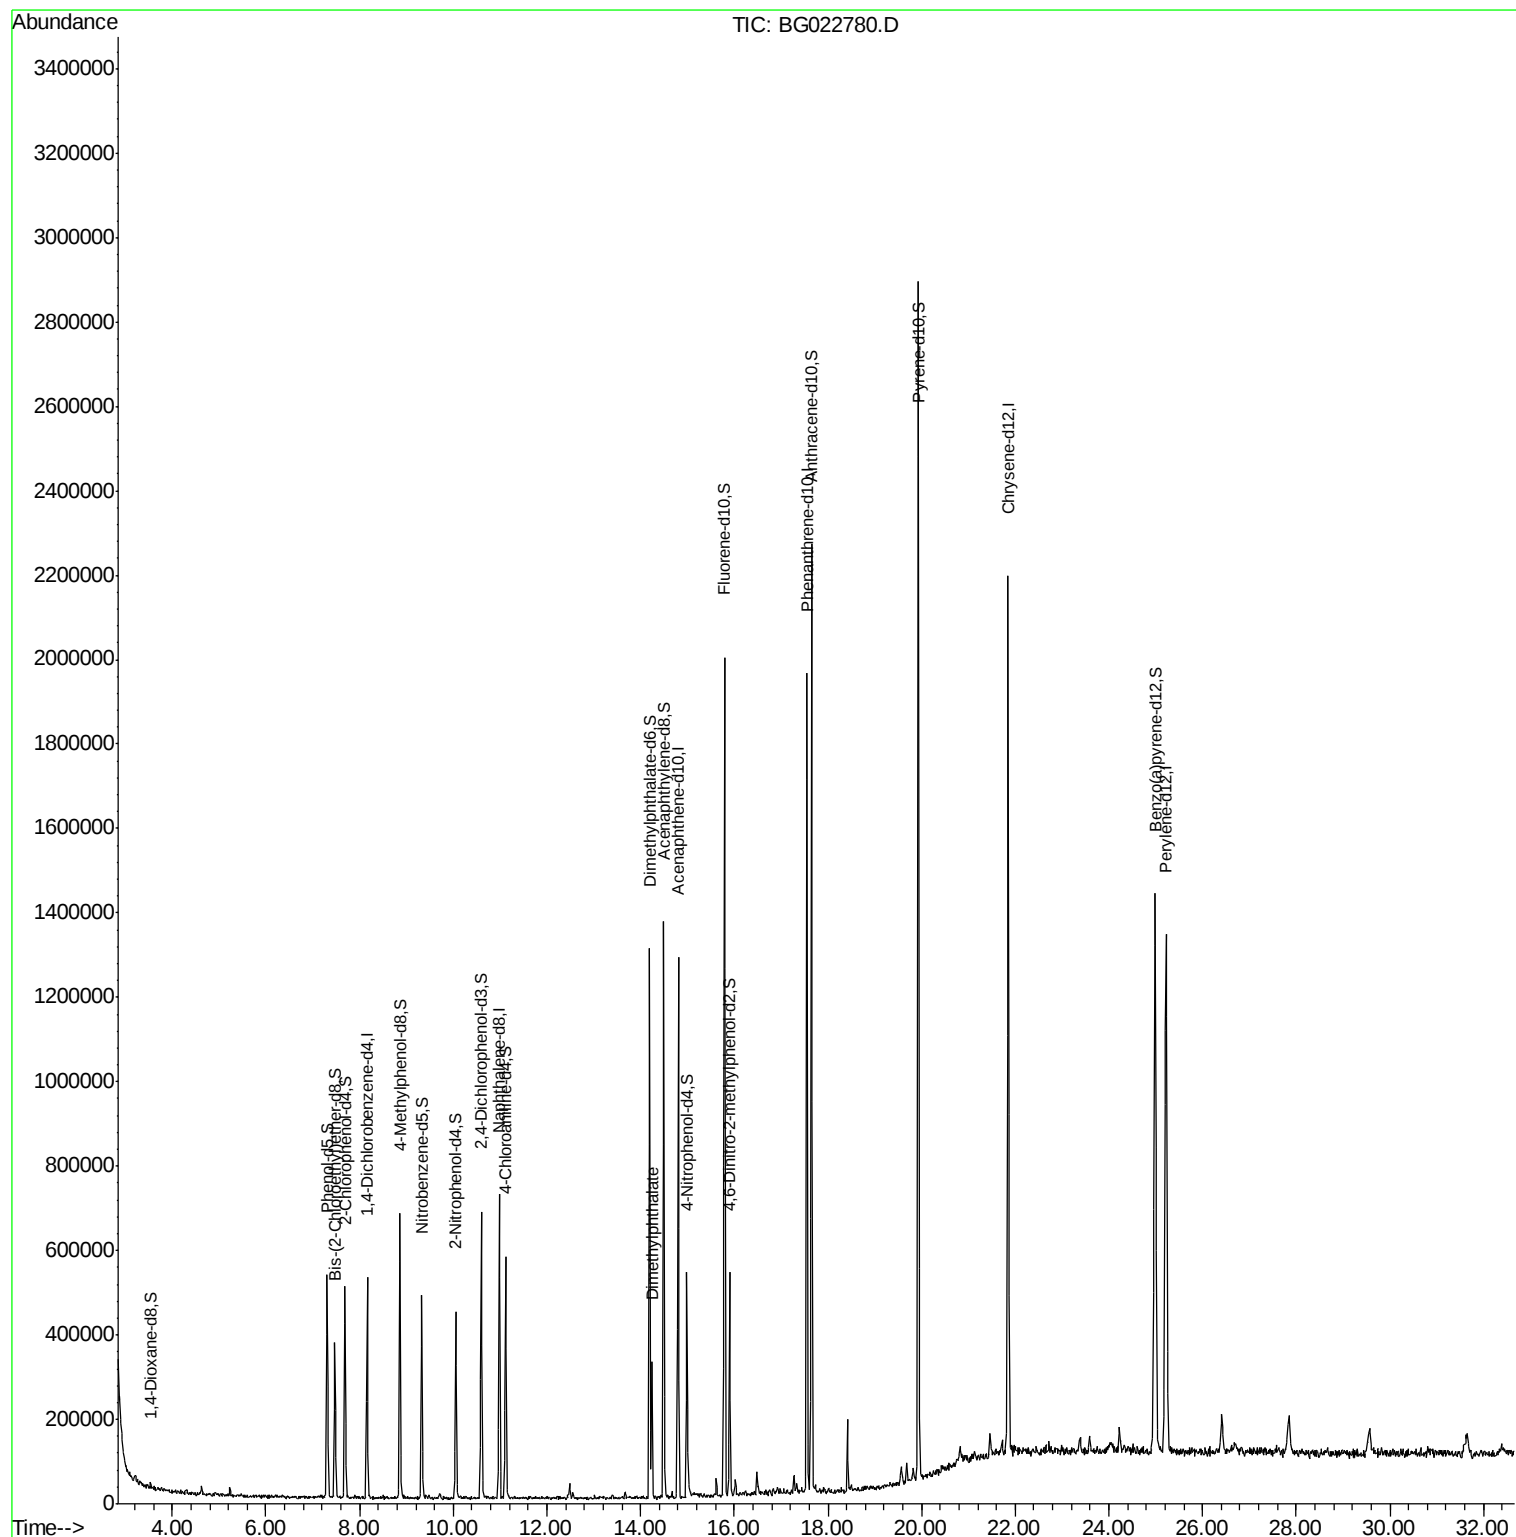

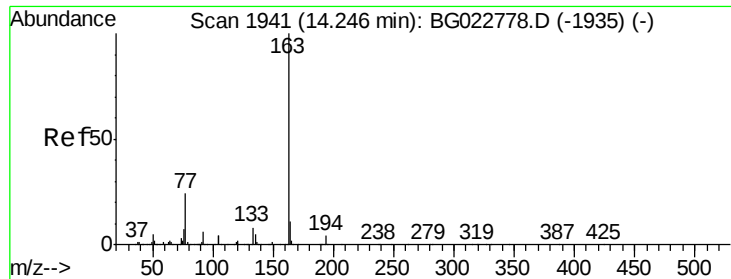

#44
 Dimethylphthalate
 Concen: 5.12 ng/ul
 RT: 14.24 min Scan# 1941
 Delta R.T. 0.00 min
 Lab File: BG022780.D
 Acq: 2 Jul 2016 5:48

Instrument :
 BNA_G
 ClientSampleId :
 BDHM3

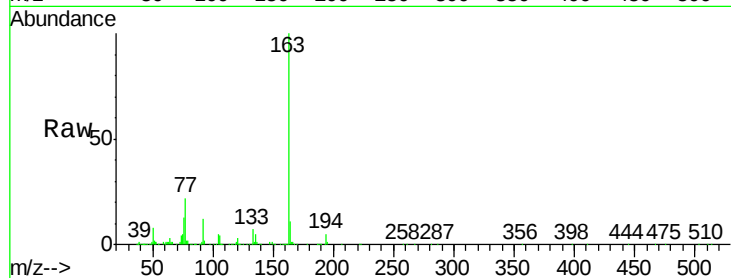

Tgt	Ion	Ratio	Resp	Lower	Upper
163	100		188291		
194	5.0	3.4	5.2		
164	11.4	8.8	13.2		

Manual Integrations

sohil
 7/4/2016 1:32:22 PM

