

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
 Data File : BG022757.D
 Acq On : 1 Jul 2016 11:10
 Operator : UM/SJ
 Sample : PB91677BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.285	74	76	78	rVB2	11521	9481	0.12%	0.013%
2	3.544	116	120	125	rVB6	22800	36659	0.48%	0.051%
3	3.796	160	163	165	rBV4	7554	9645	0.13%	0.013%
4	4.307	247	250	253	rVB4	15376	20745	0.27%	0.029%
5	5.582	465	467	471	rVB4	7888	8237	0.11%	0.011%
6	5.618	471	473	480	rBV7	6892	14637	0.19%	0.020%
7	6.346	593	597	598	rBV4	10892	10779	0.14%	0.015%
8	6.358	598	599	603	rVB4	8427	8972	0.12%	0.012%
9	6.705	655	658	661	rBV3	5953	8393	0.11%	0.012%
10	7.310	753	761	773	rVB	1000069	1815784	23.69%	2.502%
11	7.433	778	782	783	rBV2	6117	8454	0.11%	0.012%
12	7.474	783	789	799	rVB	678103	1187510	15.49%	1.636%
13	7.686	817	825	835	rBV	891285	1639227	21.39%	2.258%
14	8.156	897	905	915	rBV	537608	973274	12.70%	1.341%
15	8.491	958	962	965	rBV3	7023	10513	0.14%	0.014%
16	8.861	1016	1025	1037	rBV	1282157	2323936	30.32%	3.202%
17	9.225	1085	1087	1090	rBV2	6805	7883	0.10%	0.011%
18	9.331	1097	1105	1114	rBV	982499	1786683	23.31%	2.461%
19	9.407	1114	1118	1119	rVV3	7376	9425	0.12%	0.013%
20	9.425	1119	1121	1123	rVV3	8972	9594	0.13%	0.013%
21	9.478	1126	1130	1131	rVV3	8333	7702	0.10%	0.011%
22	9.648	1156	1159	1162	rBV2	6039	8252	0.11%	0.011%
23	9.825	1187	1189	1192	rBV	7447	8459	0.11%	0.012%
24	10.060	1220	1229	1237	rBV	895516	1650667	21.53%	2.274%
25	10.600	1313	1321	1333	rBV	1356894	2479822	32.35%	3.416%
26	10.988	1378	1387	1395	rBV	840324	1501367	19.59%	2.068%
27	11.117	1401	1409	1421	rBV2	1270486	2361787	30.81%	3.254%
28	11.769	1516	1520	1523	rBV2	6472	9646	0.13%	0.013%
29	12.069	1569	1571	1574	rBV4	6657	8702	0.11%	0.012%
30	12.292	1607	1609	1615	rVB5	5889	9024	0.12%	0.012%
31	12.486	1639	1642	1646	rVB3	5627	9103	0.12%	0.013%
32	12.562	1648	1655	1661	rVB4	27318	51815	0.68%	0.071%
33	13.679	1839	1845	1849	rVV4	17624	30497	0.40%	0.042%
34	14.196	1926	1933	1945	rVV	2746071	4127034	53.84%	5.686%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
 Data File : BG022757.D
 Acq On : 1 Jul 2016 11:10
 Operator : UM/SJ
 Sample : PB91677BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleID :
 SBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Title : SVOA CALIBRATION

35	14.496	1976	1984	1991	rBV	2643790	4291994	55.99%	5.913%
36	14.801	2028	2036	2045	rVV2	1545092	2525940	32.95%	3.480%
37	14.989	2061	2068	2084	rBV	1217279	2149152	28.04%	2.961%
38	15.095	2084	2086	2092	rVV5	12995	21326	0.28%	0.029%
39	15.165	2095	2098	2102	rVB5	7408	11559	0.15%	0.016%
40	15.283	2116	2118	2121	rVB3	8046	8464	0.11%	0.012%
41	15.330	2121	2126	2127	rBV4	6785	8575	0.11%	0.012%
42	15.788	2194	2204	2212	rBV	3672963	5981192	78.03%	8.240%
43	15.900	2217	2223	2236	rVV	1284043	1961361	25.59%	2.702%
44	16.029	2239	2245	2251	rVB3	50837	93031	1.21%	0.128%
45	16.575	2334	2338	2340	rBV5	8425	10148	0.13%	0.014%
46	16.934	2398	2399	2404	rVB2	11206	13290	0.17%	0.018%
47	17.110	2425	2429	2431	rVB4	7337	10156	0.13%	0.014%
48	17.157	2431	2437	2439	rBV4	5162	10794	0.14%	0.015%
49	17.339	2462	2468	2470	rVV3	16938	29915	0.39%	0.041%
50	17.427	2478	2483	2485	rBV4	5689	9751	0.13%	0.013%
51	17.551	2497	2504	2512	rVB2	2158065	3334333	43.50%	4.594%
52	17.651	2514	2521	2529	rVV	4330020	6575458	85.78%	9.059%
53	17.803	2544	2547	2549	rBV4	9295	8249	0.11%	0.011%
54	17.839	2549	2553	2557	rVV6	9469	13857	0.18%	0.019%
55	17.927	2565	2568	2572	rVB3	11951	14532	0.19%	0.020%
56	18.203	2610	2615	2616	rBV3	12824	12866	0.17%	0.018%
57	18.367	2641	2643	2645	rBV3	8923	8417	0.11%	0.012%
58	18.444	2651	2656	2657	rBV5	6597	8166	0.11%	0.011%
59	18.597	2680	2682	2685	rVB4	9583	7905	0.10%	0.011%
60	18.755	2707	2709	2711	rBV3	7307	8106	0.11%	0.011%
61	18.790	2711	2715	2718	rVV4	11124	16953	0.22%	0.023%
62	18.931	2734	2739	2740	rBV5	10339	12355	0.16%	0.017%
63	19.002	2748	2751	2753	rVB4	7655	8628	0.11%	0.012%
64	19.355	2809	2811	2814	rVB4	12072	8557	0.11%	0.012%
65	19.419	2820	2822	2827	rBV5	5067	8866	0.12%	0.012%
66	19.490	2832	2834	2839	rVB5	9365	12500	0.16%	0.017%
67	19.537	2839	2842	2843	rBV3	10963	8344	0.11%	0.011%
68	19.566	2843	2847	2852	rVV2	57596	89983	1.17%	0.124%
69	19.825	2885	2891	2896	rBV3	74436	119118	1.55%	0.164%
70	19.936	2902	2910	2920	rBV	5019887	7665268	100.00%	10.560%
71	20.230	2959	2960	2962	rBV2	13078	11910	0.16%	0.016%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022757.D
Acq On : 1 Jul 2016 11:10
Operator : UM/SJ
Sample : PB91677BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK77

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Title : SVOA CALIBRATION

72	20.823	3059	3061	3065	rBV4	17078	19899	0.26%	0.027%
73	20.870	3067	3069	3072	rVB4	32719	24900	0.32%	0.034%
74	21.429	3162	3164	3166	rVB3	16552	8356	0.11%	0.012%
75	21.852	3229	3236	3245	rBV	2302890	3951084	51.55%	5.443%
76	22.186	3291	3293	3294	rBV2	13964	8980	0.12%	0.012%
77	22.486	3342	3344	3345	rBV2	15777	10712	0.14%	0.015%
78	22.662	3372	3374	3379	rVB6	29516	25512	0.33%	0.035%
79	24.419	3671	3673	3674	rBV2	14882	11253	0.15%	0.016%
80	25.001	3759	3772	3785	rBV3	2433695	7249056	94.57%	9.987%
81	25.224	3798	3810	3826	rVB2	1288366	3881330	50.64%	5.347%
82	25.459	3848	3850	3852	rBV3	17605	16237	0.21%	0.022%
83	25.894	3922	3924	3926	rBV3	17228	10471	0.14%	0.014%
84	26.634	4048	4050	4053	rBV3	16910	13210	0.17%	0.018%
85	27.815	4248	4251	4252	rBV3	30109	35316	0.46%	0.049%
86	27.933	4269	4271	4272	rBV2	16374	8813	0.11%	0.012%
87	28.127	4302	4304	4305	rBV2	17972	11187	0.15%	0.015%
88	28.385	4346	4348	4351	rBV4	17503	24093	0.31%	0.033%
89	32.210	4997	4999	5000	rVB2	21614	12603	0.16%	0.017%
90	32.316	5015	5017	5020	rBV4	15746	9729	0.13%	0.013%


Sum of corrected areas: 72587468

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022757.D
Acq On : 1 Jul 2016 11:10
Operator : UM/SJ
Sample : PB91677BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK77

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

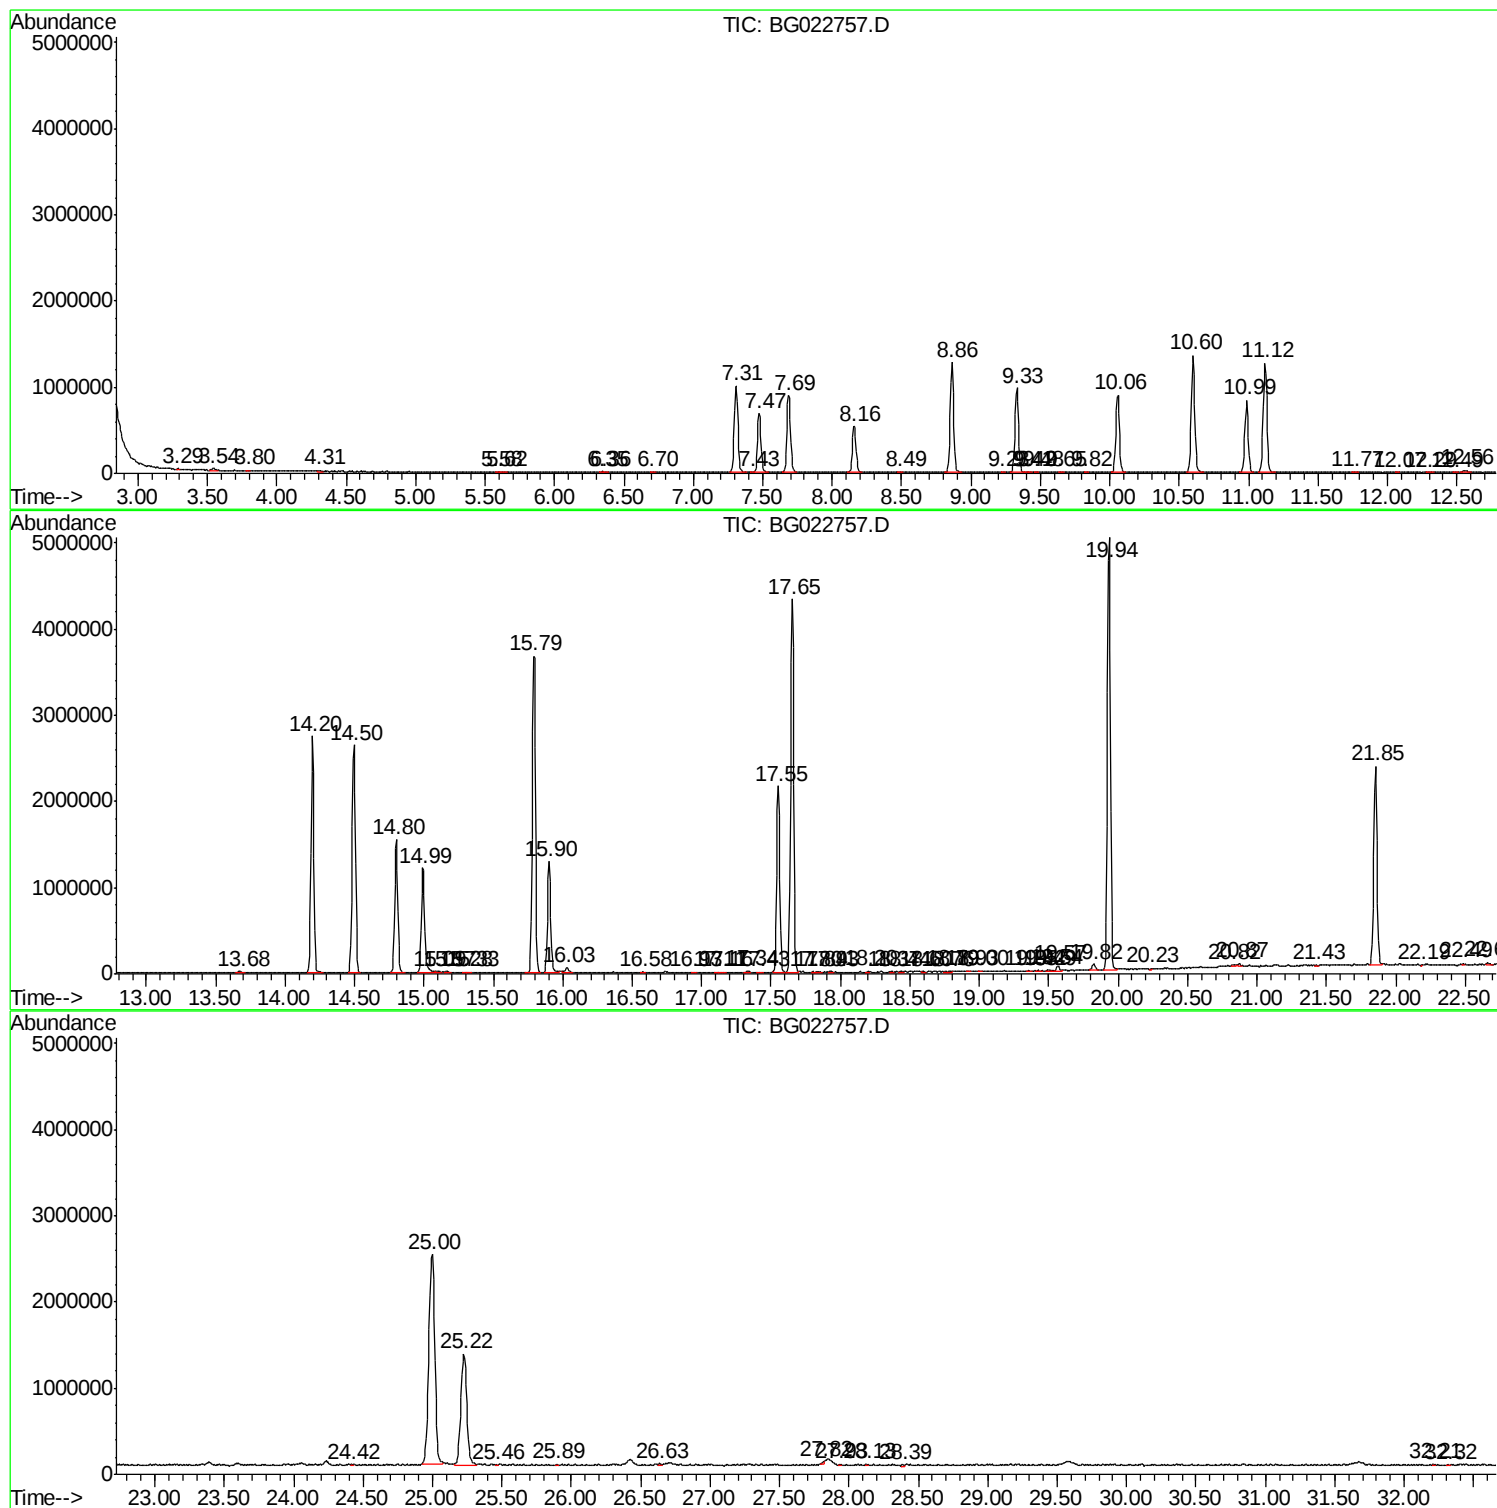

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022757.D
Acq On : 1 Jul 2016 11:10
Operator : UM/SJ
Sample : PB91677BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK77

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022757.D
Acq On : 1 Jul 2016 11:10
Operator : UM/SJ
Sample : PB91677BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK77

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc