

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
 Data File : BG022775.D
 Acq On : 2 Jul 2016 2:27
 Operator : UM/SJ
 Sample : H3752-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHL7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.814	163	166	171	rBV2	35241	67150	1.88%	0.175%
2	4.901	349	351	353	rVB	9285	5478	0.15%	0.014%
3	4.942	357	358	360	rVB2	12456	8663	0.24%	0.023%
4	4.960	360	361	365	rBV2	8689	11998	0.34%	0.031%
5	5.289	415	417	418	rBV2	8051	5776	0.16%	0.015%
6	5.447	442	444	450	rBV5	3977	8153	0.23%	0.021%
7	5.741	492	494	497	rBV3	5840	6619	0.19%	0.017%
8	5.794	501	503	507	rVV4	6611	9779	0.27%	0.025%
9	5.829	507	509	513	rVB4	6052	6181	0.17%	0.016%
10	5.870	513	516	518	rBV4	4793	6033	0.17%	0.016%
11	6.211	572	574	579	rVB6	8969	10683	0.30%	0.028%
12	6.352	597	598	600	rVB2	8527	5620	0.16%	0.015%
13	6.446	610	614	615	rBV3	5132	5959	0.17%	0.015%
14	6.487	619	621	622	rBV2	5962	5471	0.15%	0.014%
15	6.564	632	634	638	rVB3	6217	6744	0.19%	0.018%
16	6.746	659	665	666	rBV4	8032	9752	0.27%	0.025%
17	7.028	712	713	719	rVB4	4368	6855	0.19%	0.018%
18	7.310	755	761	773	rVV	375725	681875	19.09%	1.772%
19	7.474	783	789	798	rBV	253635	419290	11.74%	1.090%
20	7.539	798	800	803	rVB4	5734	6149	0.17%	0.016%
21	7.568	803	805	808	rBV4	6951	8020	0.22%	0.021%
22	7.692	817	826	833	rBV	336811	591275	16.55%	1.537%
23	8.068	887	890	894	rVB6	5263	6073	0.17%	0.016%
24	8.162	899	906	918	rVB2	388176	689807	19.31%	1.793%
25	8.714	997	1000	1004	rVB3	6194	7993	0.22%	0.021%
26	8.767	1004	1009	1012	rBV5	5796	6269	0.18%	0.016%
27	8.867	1019	1026	1035	rVB	479935	843473	23.61%	2.192%
28	9.002	1047	1049	1053	rBV4	5819	9571	0.27%	0.025%
29	9.149	1071	1074	1076	rBV2	4806	5843	0.16%	0.015%
30	9.178	1076	1079	1080	rBV2	5196	5483	0.15%	0.014%
31	9.331	1099	1105	1112	rBV	369451	646499	18.10%	1.680%
32	9.725	1165	1172	1175	rVB6	16527	25825	0.72%	0.067%
33	9.783	1179	1182	1185	rBV4	4900	7079	0.20%	0.018%
34	9.883	1196	1199	1201	rBV3	5416	5288	0.15%	0.014%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
 Data File : BG022775.D
 Acq On : 2 Jul 2016 2:27
 Operator : UM/SJ
 Sample : H3752-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDHL7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
 Title : SVOA CALIBRATION

35	10.060	1222	1229	1235	rBV2	322118	583504	16.33%	1.517%
36	10.201	1249	1253	1256	rVB5	5830	7778	0.22%	0.020%
37	10.371	1279	1282	1284	rBV4	4770	5664	0.16%	0.015%
38	10.512	1304	1306	1311	rVB4	4975	6428	0.18%	0.017%
39	10.600	1315	1321	1332	rVB2	507230	980610	27.45%	2.549%
40	10.747	1343	1346	1347	rBV3	10068	10273	0.29%	0.027%
41	10.988	1379	1387	1395	rBV	621652	1127855	31.57%	2.932%
42	11.123	1402	1410	1419	rBV	475293	904714	25.32%	2.352%
43	11.211	1423	1425	1430	rVB4	4983	5522	0.15%	0.014%
44	11.276	1435	1436	1442	rBV2	7956	6954	0.19%	0.018%
45	11.358	1448	1450	1452	rBV2	7637	7677	0.21%	0.020%
46	11.411	1457	1459	1460	rBV3	6253	5382	0.15%	0.014%
47	11.940	1547	1549	1552	rVB4	6906	5803	0.16%	0.015%
48	12.063	1569	1570	1573	rVB2	7637	5342	0.15%	0.014%
49	12.104	1575	1577	1580	rVB3	8191	6572	0.18%	0.017%
50	12.145	1580	1584	1586	rBV2	7589	7822	0.22%	0.020%
51	12.210	1591	1595	1600	rVB6	7604	13889	0.39%	0.036%
52	12.257	1600	1603	1604	rBV2	5630	6281	0.18%	0.016%
53	12.369	1618	1622	1623	rBV3	6542	7718	0.22%	0.020%
54	12.445	1632	1635	1636	rVV3	6662	5301	0.15%	0.014%
55	12.463	1636	1638	1641	rVB3	7433	5778	0.16%	0.015%
56	12.515	1646	1647	1650	rBV2	6682	5931	0.17%	0.015%
57	12.545	1650	1652	1653	rBV	7570	5859	0.16%	0.015%
58	12.563	1653	1655	1659	rVB4	12382	13232	0.37%	0.034%
59	12.839	1700	1702	1705	rBV4	7455	7150	0.20%	0.019%
60	13.150	1752	1755	1756	rBV3	6878	7356	0.21%	0.019%
61	13.315	1779	1783	1786	rBV5	7828	11530	0.32%	0.030%
62	13.391	1793	1796	1797	rBV2	8261	7664	0.21%	0.020%
63	13.409	1797	1799	1801	rVB3	10049	7456	0.21%	0.019%
64	13.438	1801	1804	1806	rVB4	6654	8166	0.23%	0.021%
65	13.456	1806	1807	1811	rBV4	5137	7915	0.22%	0.021%
66	13.679	1841	1845	1851	rBV8	18183	35313	0.99%	0.092%
67	14.002	1897	1900	1903	rBV4	7386	7767	0.22%	0.020%
68	14.196	1925	1933	1938	rBV	1146770	1722371	48.21%	4.477%
69	14.243	1938	1941	1948	rVB	167073	237973	6.66%	0.619%
70	14.496	1977	1984	1991	rBV	1134500	1827505	51.15%	4.750%
71	14.672	2012	2014	2019	rVB4	13665	17779	0.50%	0.046%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022775.D
Acq On : 2 Jul 2016 2:27
Operator : UM/SJ
Sample : H3752-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHL7

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Title : SVOA CALIBRATION

72	14.801	2030	2036	2044	rBV3	1228538	2054408	57.50%	5.340%
73	14.995	2063	2069	2080	rBV	459677	807531	22.60%	2.099%
74	15.165	2094	2098	2101	rBV6	7908	12230	0.34%	0.032%
75	15.289	2117	2119	2122	rBV4	7798	10905	0.31%	0.028%
76	15.624	2173	2176	2182	rVB4	23036	32103	0.90%	0.083%
77	15.671	2182	2184	2189	rBV6	5856	7352	0.21%	0.019%
78	15.794	2199	2205	2215	rVB	1689333	2665241	74.60%	6.928%
79	15.906	2218	2224	2235	rBV	479026	725324	20.30%	1.885%
80	16.029	2242	2245	2252	rVB6	28607	42636	1.19%	0.111%
81	16.182	2268	2271	2272	rBV3	5935	6937	0.19%	0.018%
82	16.276	2286	2287	2289	rBV2	6705	5519	0.15%	0.014%
83	16.493	2319	2324	2331	rBV3	48801	85589	2.40%	0.222%
84	16.575	2336	2338	2340	rVV3	8598	5334	0.15%	0.014%
85	16.611	2342	2344	2347	rBV4	11420	10360	0.29%	0.027%
86	16.675	2352	2355	2359	rBV6	11714	18521	0.52%	0.048%
87	16.758	2364	2369	2370	rBV5	11324	18646	0.52%	0.048%
88	16.987	2407	2408	2409	rBV	12901	8678	0.24%	0.023%
89	17.286	2455	2459	2462	rBV3	44382	55626	1.56%	0.145%
90	17.557	2498	2505	2512	rBV	1850425	2822196	79.00%	7.336%
91	17.657	2516	2522	2531	rVB2	1896549	2954423	82.70%	7.679%
92	17.827	2548	2551	2552	rBV2	16517	16985	0.48%	0.044%
93	18.420	2648	2652	2658	rBV2	173585	237953	6.66%	0.619%
94	19.261	2793	2795	2796	rBV2	16253	11482	0.32%	0.030%
95	19.689	2864	2868	2871	rBV5	82837	113217	3.17%	0.294%
96	19.936	2904	2910	2918	rBV2	2405797	3572622	100.00%	9.286%
97	21.722	3210	3214	3221	rVB	205619	279740	7.83%	0.727%
98	21.858	3231	3237	3244	rVB	1993375	3347554	93.70%	8.701%
99	25.001	3762	3772	3785	rBV	1154470	3354098	93.88%	8.718%
100	25.236	3803	3812	3825	rVB2	1136239	3388121	94.84%	8.807%


Sum of corrected areas: 38471891

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022775.D
Acq On : 2 Jul 2016 2:27
Operator : UM/SJ
Sample : H3752-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHL7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

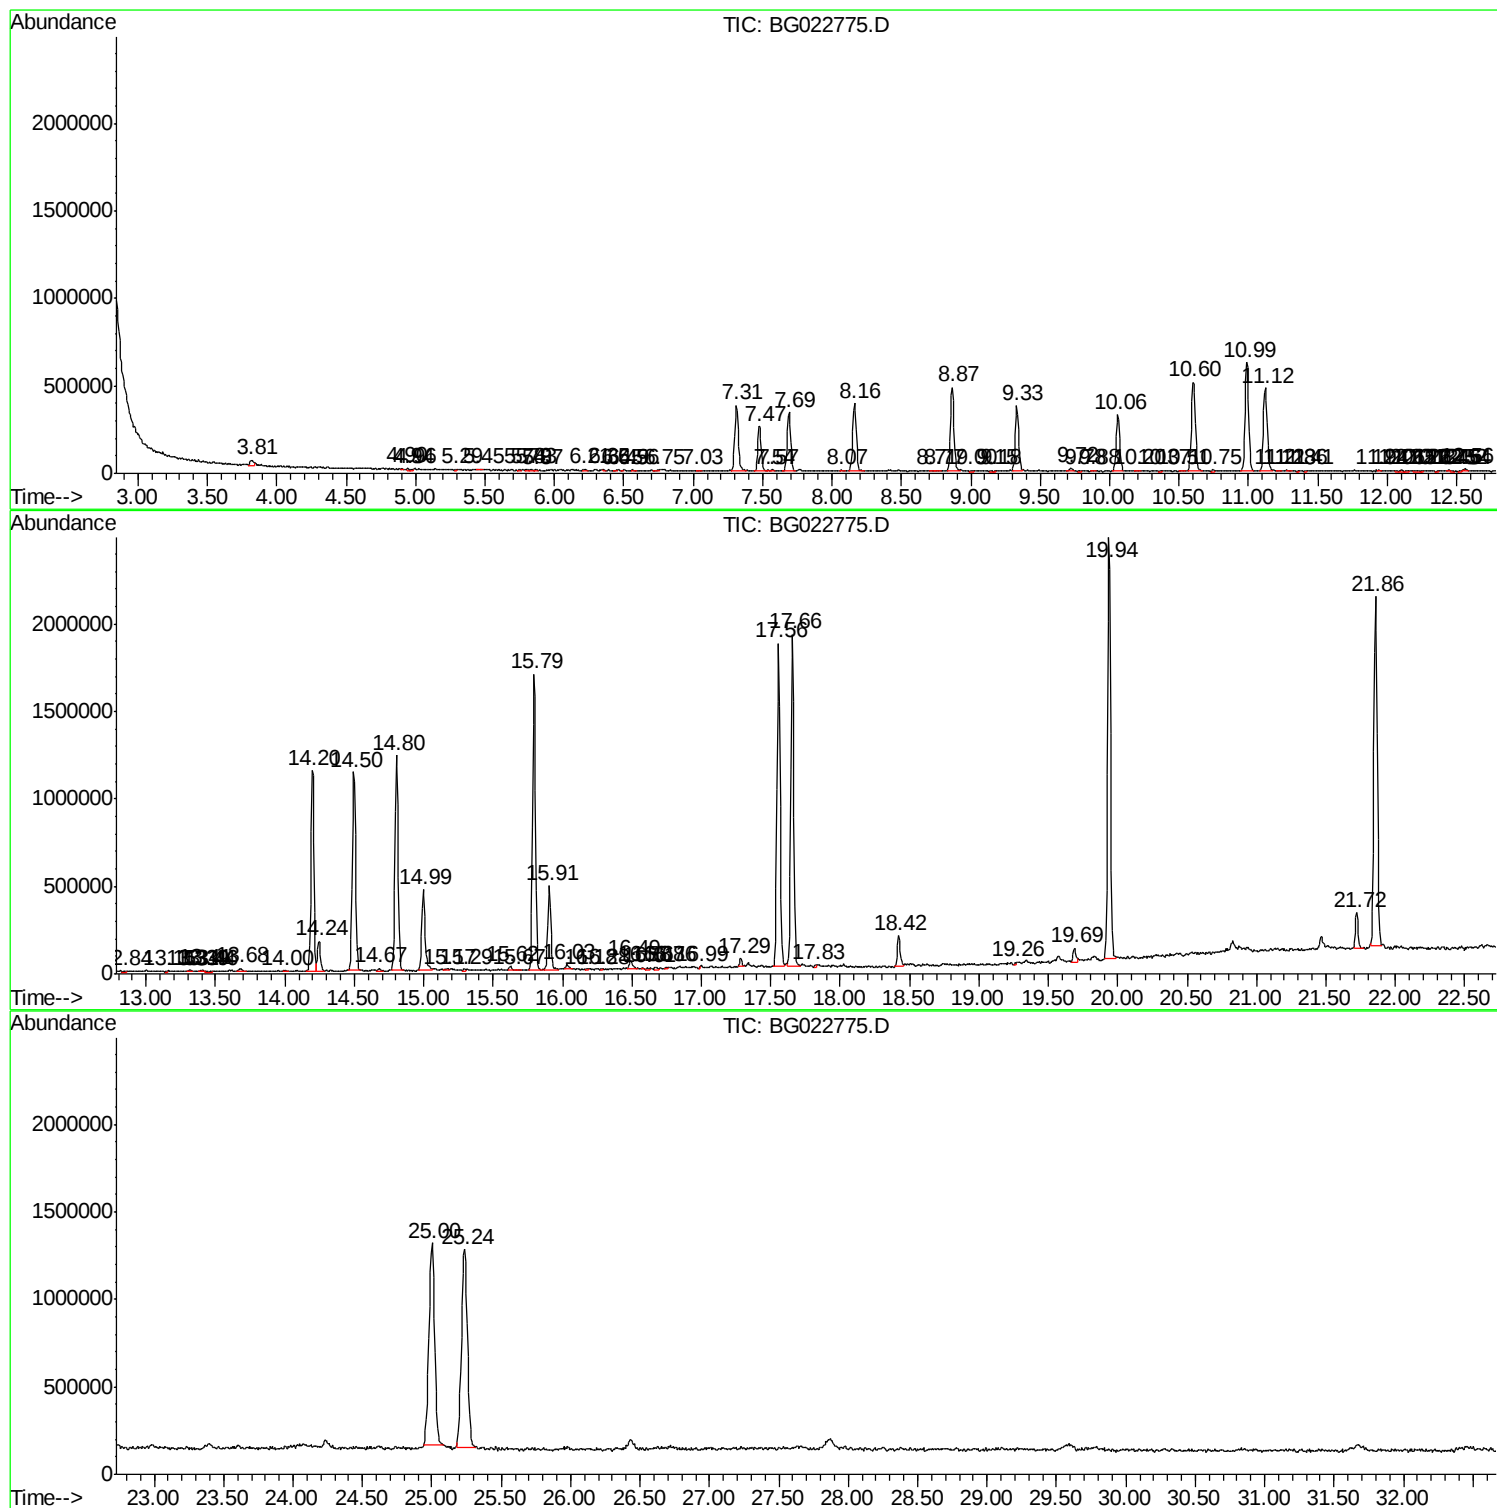

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022775.D
Acq On : 2 Jul 2016 2:27
Operator : UM/SJ
Sample : H3752-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHL7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070116\
Data File : BG022775.D
Acq On : 2 Jul 2016 2:27
Operator : UM/SJ
Sample : H3752-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDHL7

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG063016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc