

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070117\
 Data File : BG027790.D
 Acq On : 1 Jul 2017 19:12
 Operator : SJ/JU
 Sample : I3982-12
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jul 03 06:55:31 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 19:26:37 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.48	152	30362	20.00	ng	0.00
21) Naphthalene-d8	11.30	136	148957	20.00	ng	0.00
38) Acenaphthene-d10	15.06	164	99358	20.00	ng	0.00
63) Phenanthrene-d10	17.81	188	247793	20.00	ng	0.00
75) Chrysene-d12	22.18	240	251555	20.00	ng	0.00
86) Perylene-d12	25.79	264	250830	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.06	112	274583	139.26	ng	0.00
7) Phenol-d6	7.62	99	352430	117.00	ng	0.00
23) Nitrobenzene-d5	9.64	82	245322	91.80	ng	0.00
41) 2,4,6-Tribromophenol	16.56	330	247091	181.31	ng	0.00
44) 2-Fluorobiphenyl	13.69	172	671996	96.59	ng	0.00
78) Terphenyl-d14	20.39	244	1211863	112.94	ng	0.00
Target Compounds						
76) Benzidine	20.04	184	57	3.23	ng	Qvalue # 64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG070117\
Data File : BG027790.D
Acq On : 1 Jul 2017 19:12
Operator : SJ/JU
Sample : I3982-12
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jul 03 06:55:31 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 19:26:37 2017
Response via : Initial Calibration

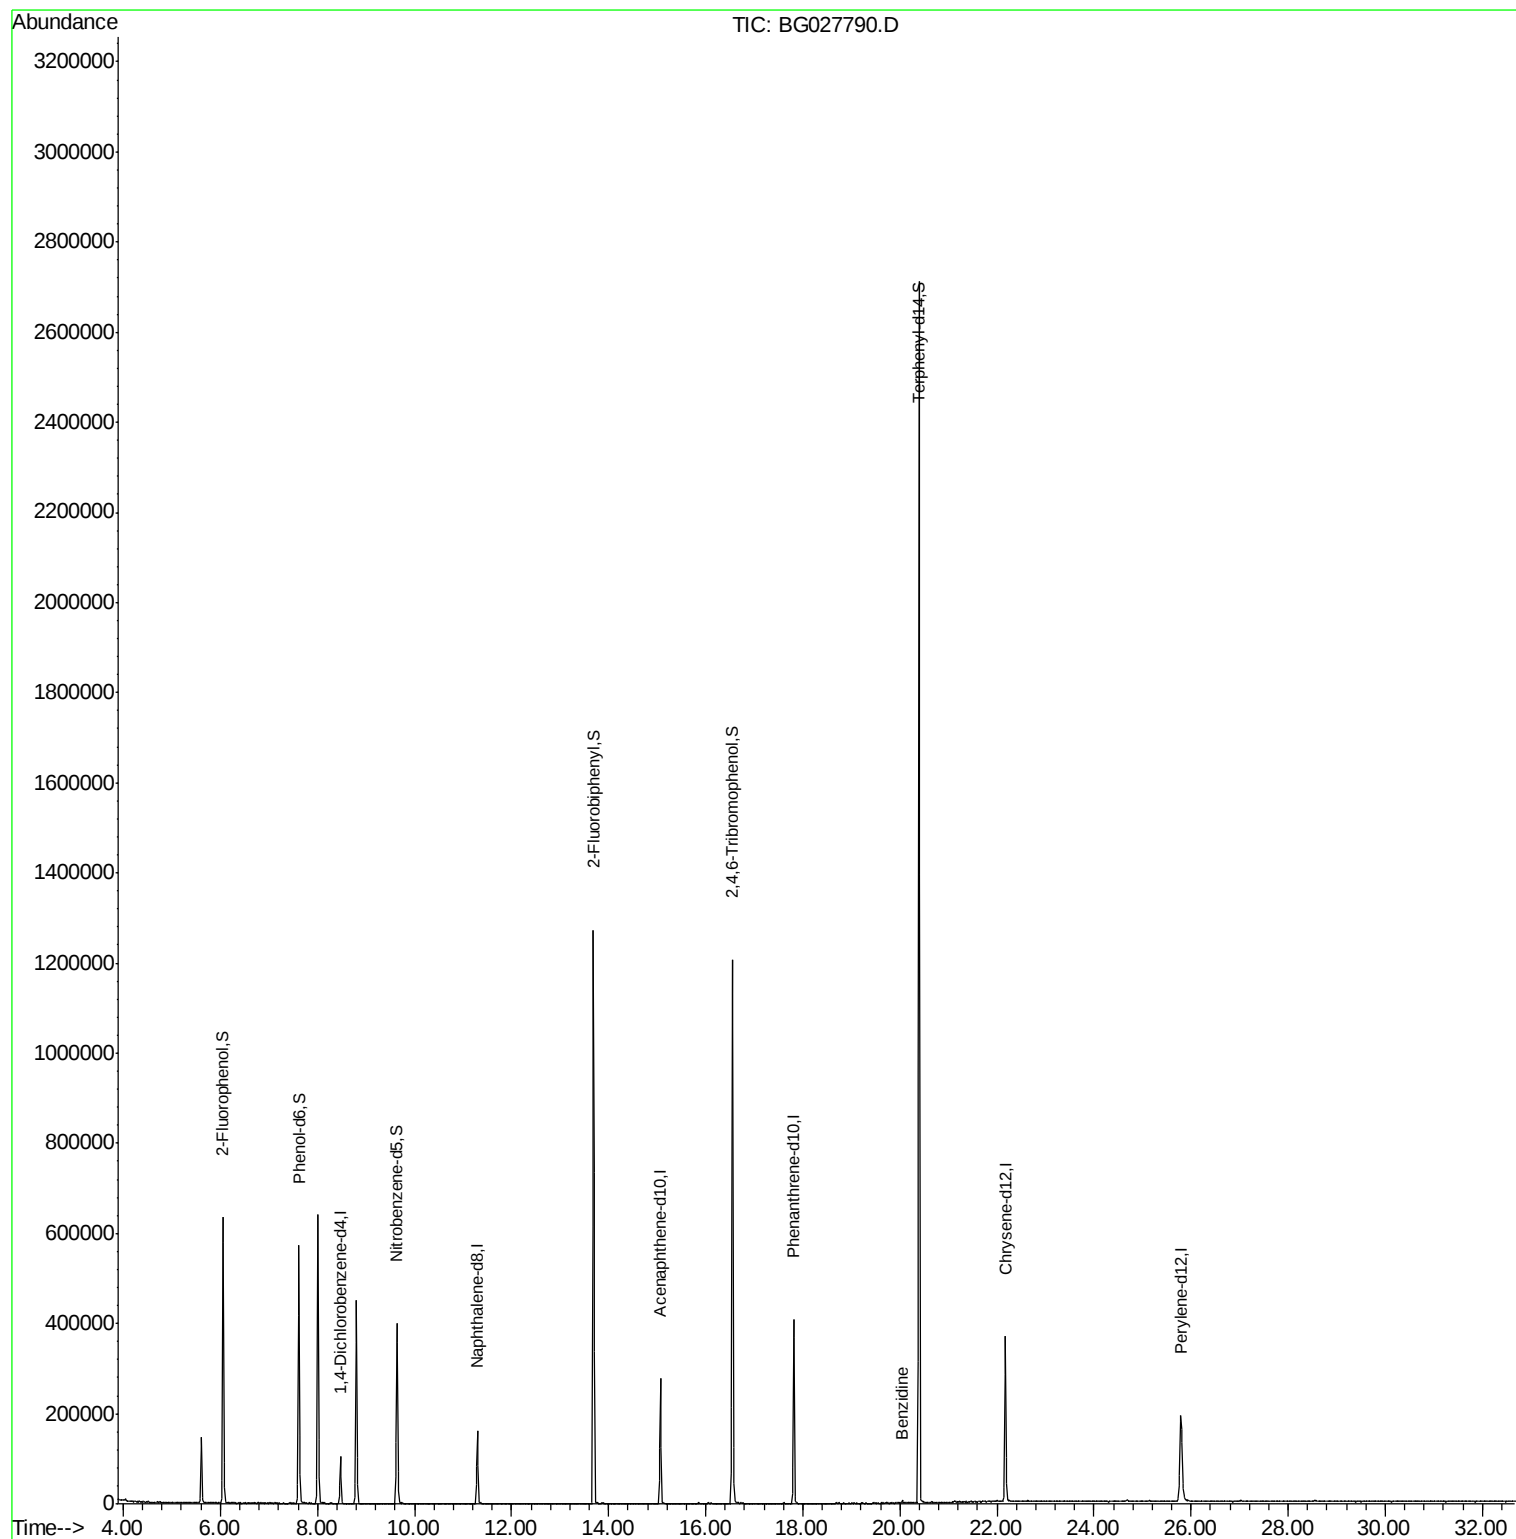

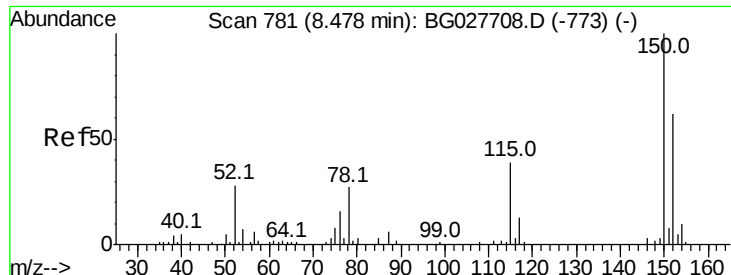


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.48 min Scan# 781
Delta R.T. -0.00 min
Lab File: BG027790.D
Acq: 1 Jul 2017 19:12

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 30362
Ion Ratio Lower Upper
152 100
150 163.0 114.0 171.0
115 64.9 48.1 72.1

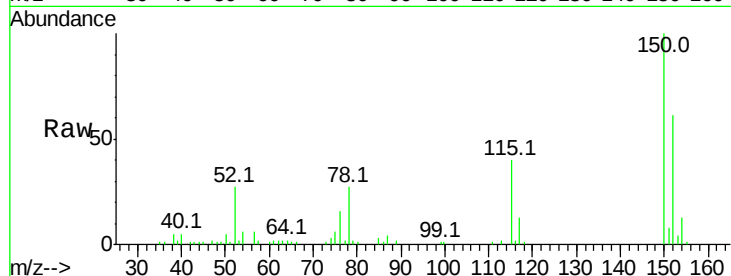


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

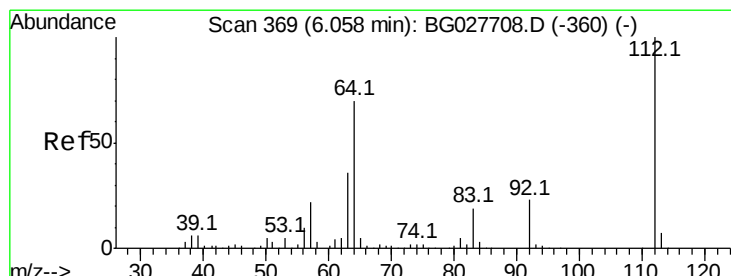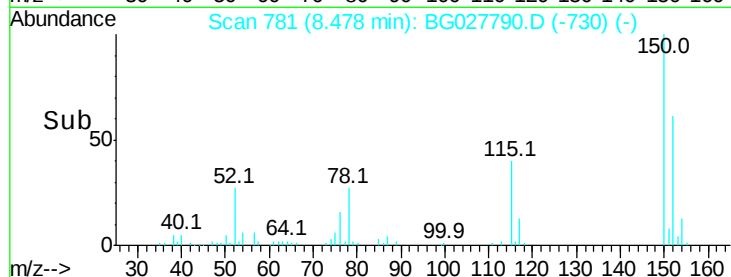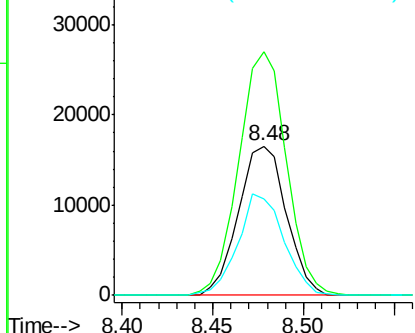



#5


2-Fluorophenol
Concen: 139.26 ng
RT: 6.06 min Scan# 369
Delta R.T. -0.00 min
Lab File: BG027790.D
Acq: 1 Jul 2017 19:12

Tgt Ion:112 Resp: 274583
Ion Ratio Lower Upper
112 100
64 71.3 61.8 92.6
63 37.0 37.2 55.8#

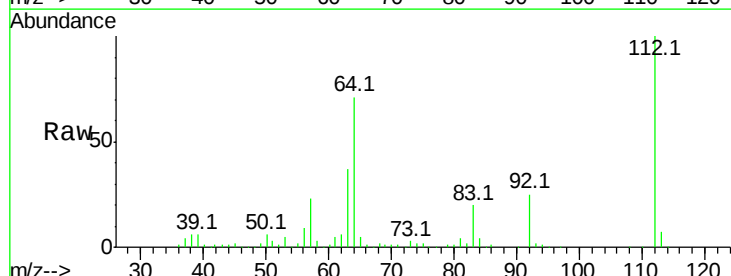

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

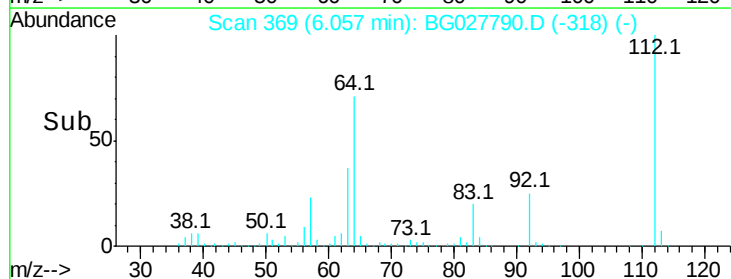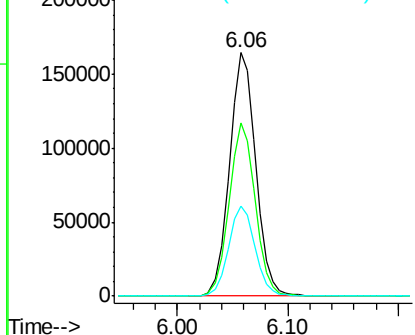

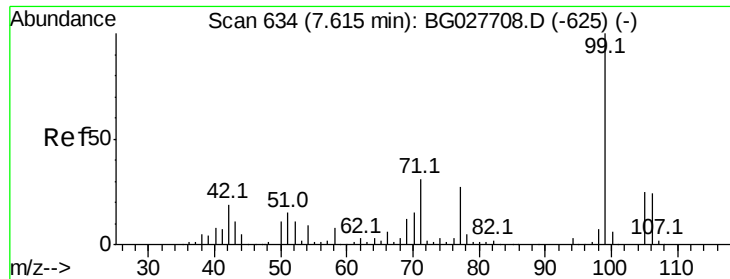

#7

Phenol-d6

Concen: 117.00 ng

RT: 7.62 min Scan# 635

Delta R.T. 0.01 min

Lab File: BG027790.D

Acq: 1 Jul 2017 19:12

Instrument :

BNA_G

ClientSampled :


Tot Ion: 99 Resp: 352430

Ion Ratio Lower Upper




99 100

42 19.3 20.5 30.7#

71 34.1 37.6 56.4#

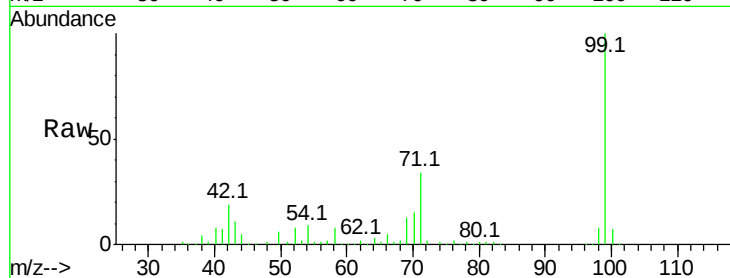

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

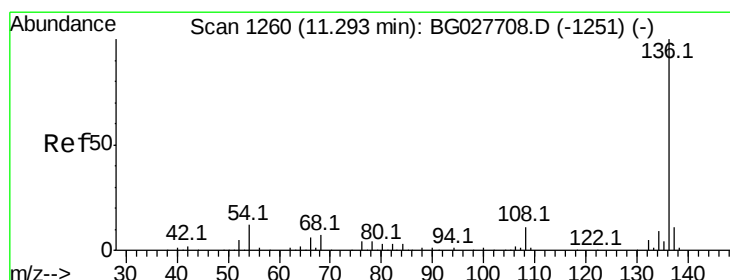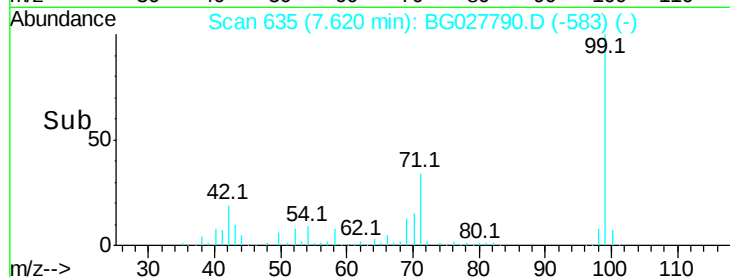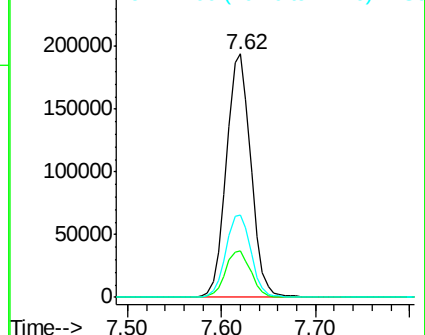

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.30 min Scan# 1261

Delta R.T. 0.01 min

Lab File: BG027790.D

Acq: 1 Jul 2017 19:12

Tgt Ion: 136 Resp: 148957


Ion Ratio Lower Upper

136 100



137 11.4 8.9 13.3


54 11.4 9.3 13.9

68 5.3 5.1 7.7

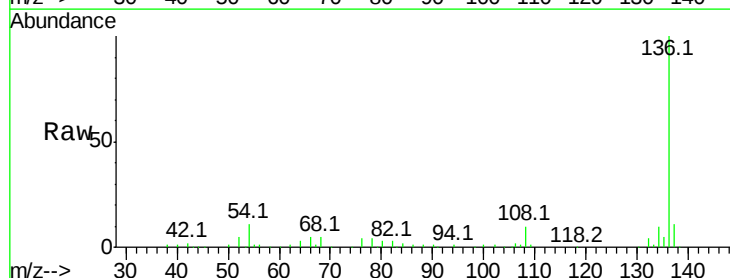

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



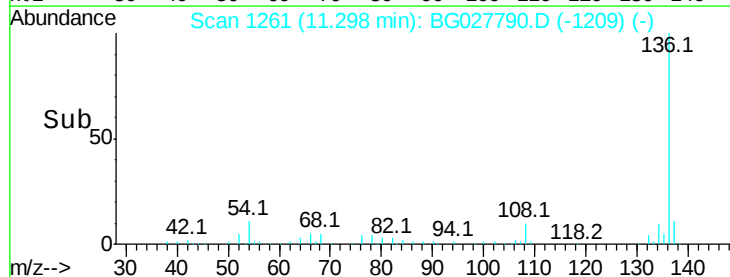
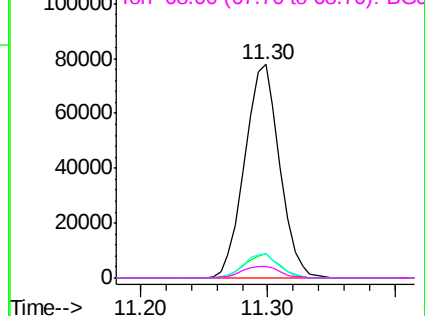


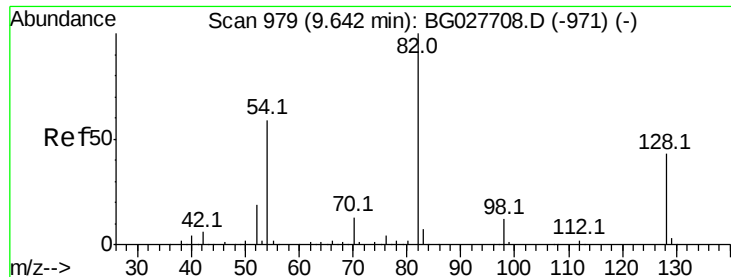

#23
 Nitrobenzene-d5
 Concen: 91.80 ng
 RT: 9.64 min Scan# 979
 Delta R.T. -0.00 min
 Lab File: BG027790.D
 Acq: 1 Jul 2017 19:12




Instrument :
 BNA_G
 ClientSampleID :


Tot Ion: 82 Resp: 245322
 Ion Ratio Lower Upper
 82 100
 128 42.8 26.4 39.6#
 54 61.4 49.4 74.2

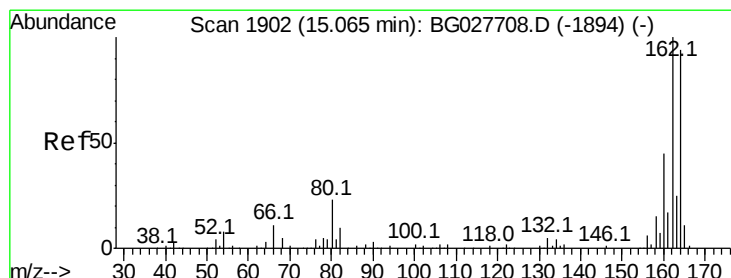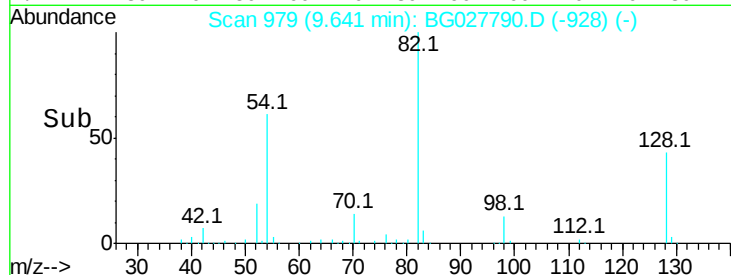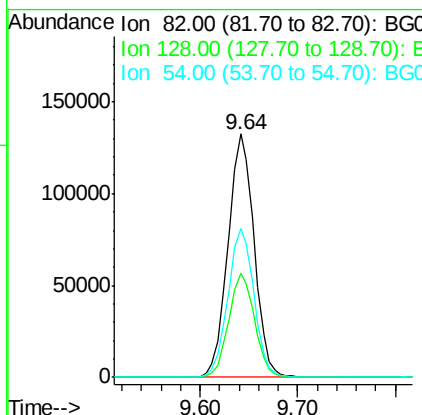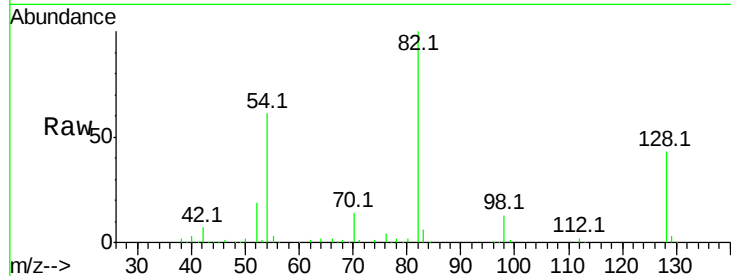

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 15.06 min Scan# 1902
 Delta R.T. -0.00 min
 Lab File: BG027790.D
 Acq: 1 Jul 2017 19:12

Tgt Ion:164 Resp: 99358
 Ion Ratio Lower Upper
 164 100
 162 102.7 85.1 127.7
 160 47.8 34.7 52.1

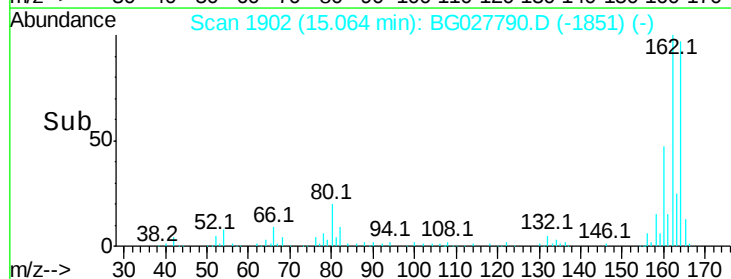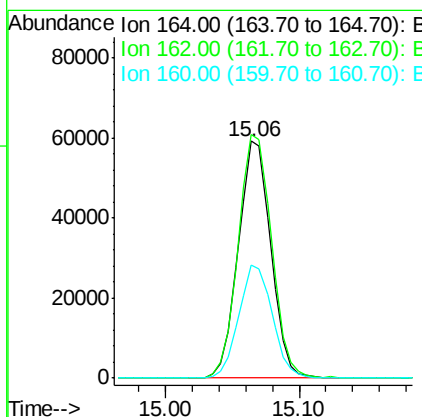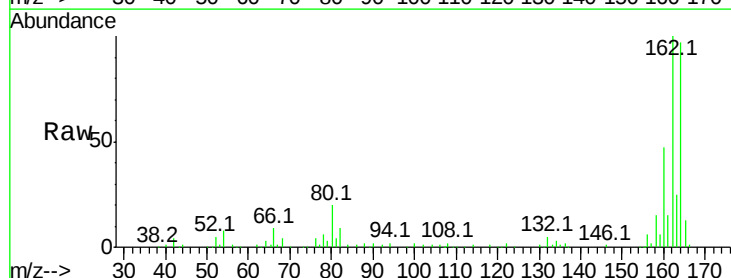


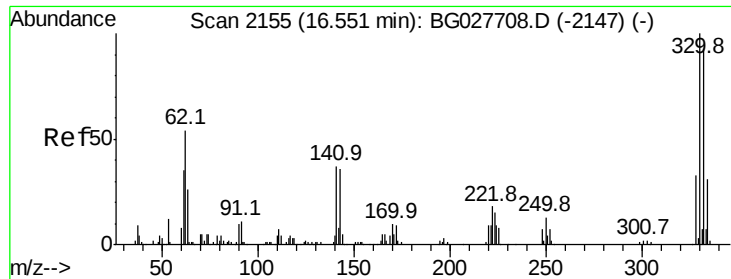




#41
 2,4,6-Tribromophenol
 Concen: 181.31 ng
 RT: 16.56 min Scan# 2156
 Delta R.T. 0.01 min
 Lab File: BG027790.D
 Acq: 1 Jul 2017 19:12

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.4	77.3	115.9
141	34.7	32.1	48.1

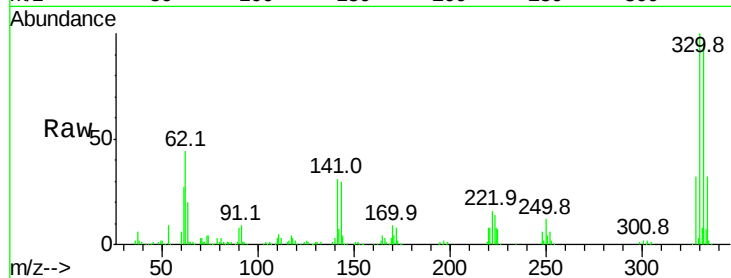


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

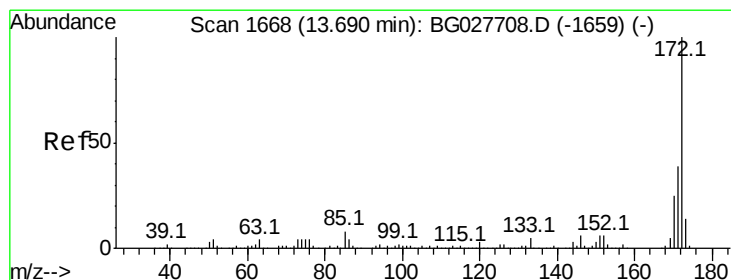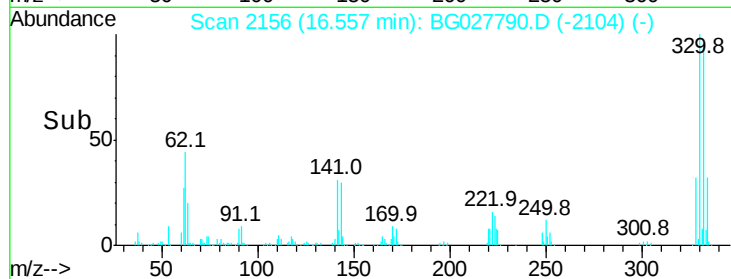
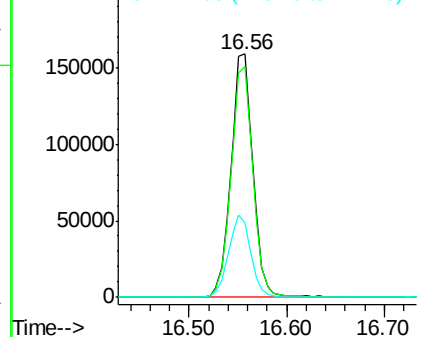



#44
 2-Fluorobiphenyl
 Concen: 96.59 ng
 RT: 13.69 min Scan# 1668
 Delta R.T. -0.00 min
 Lab File: BG027790.D
 Acq: 1 Jul 2017 19:12

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.8	32.2	48.2
170	24.4	21.8	32.6

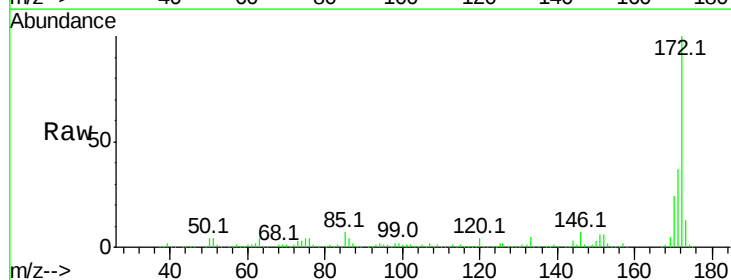

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

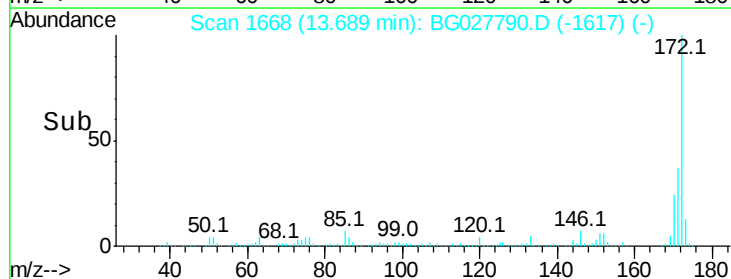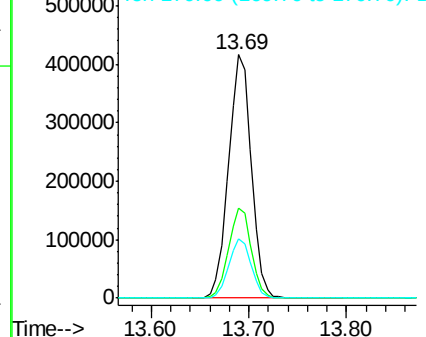


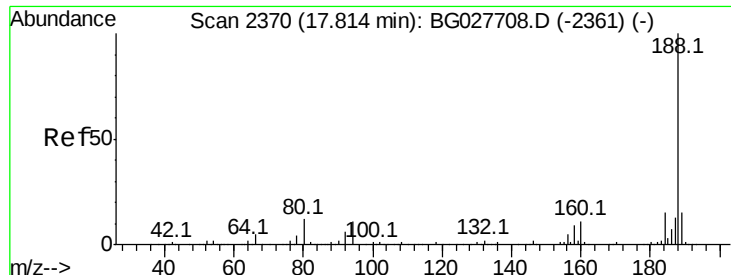




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.81 min Scan# 2370
Delta R.T. -0.00 min
Lab File: BG027790.D
Acq: 1 Jul 2017 19:12

Instrument :
BNA_G
ClientSampleId :

Tot Ion:188 Resp: 247793
Ion Ratio Lower Upper
188 100
94 9.7 5.8 8.8#
80 11.4 7.5 11.3#

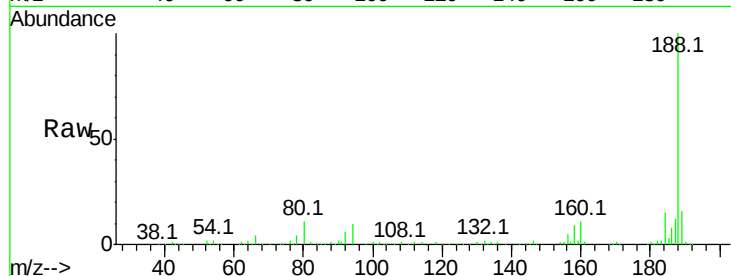


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

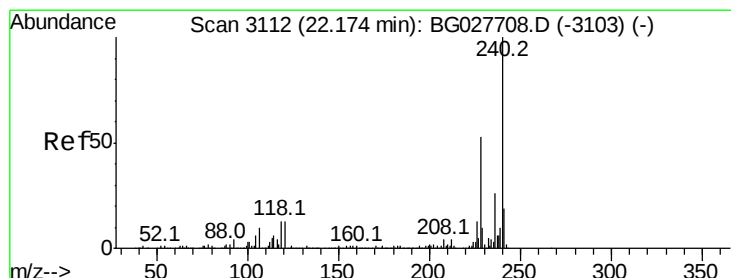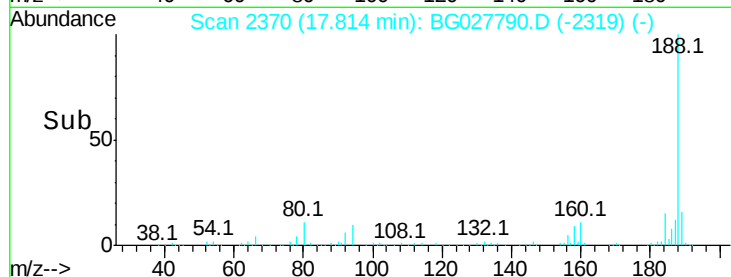
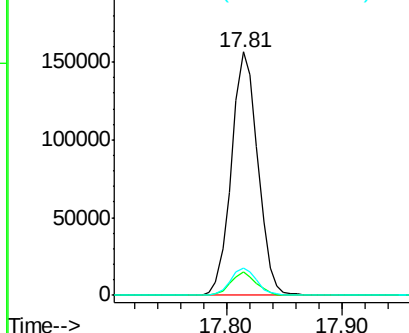



#75
Chrysene-d12
Concen: 20.00 ng
RT: 22.18 min Scan# 3113
Delta R.T. 0.01 min
Lab File: BG027790.D
Acq: 1 Jul 2017 19:12

Tgt Ion:240 Resp: 251555
Ion Ratio Lower Upper
240 100
120 10.8 5.7 8.5#
236 26.6 22.2 33.4

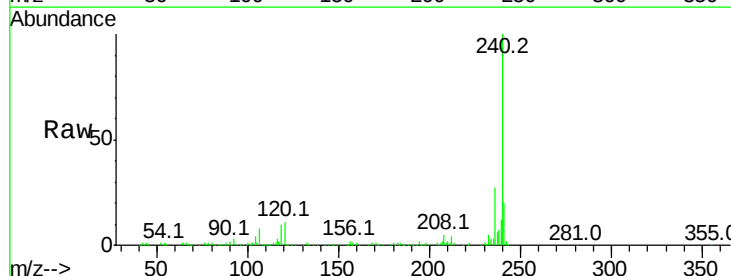

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

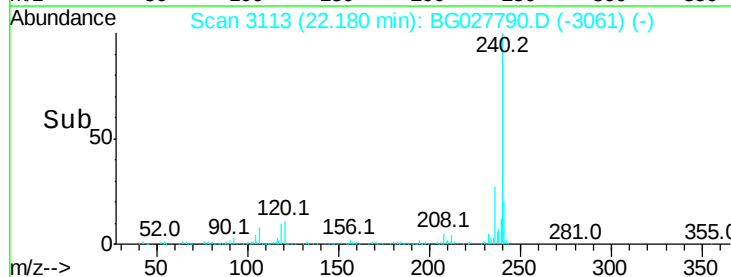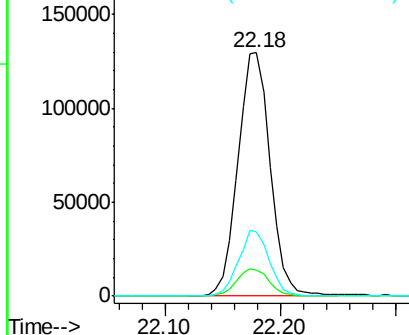

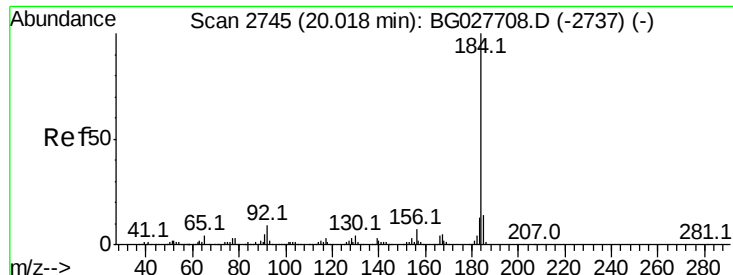

#76

Benzidine

Concen: 3.23 ng

RT: 20.04 min Scan# 2749

Delta R.T. 0.02 min

Lab File: BG027790.D

Acq: 1 Jul 2017 19:12

Instrument :

BNA_G

ClientSampleId :


Tot Ion:184 Resp: 57

Ion Ratio Lower Upper

184 100

185 0.0 13.0 19.6#




183 0.0 11.0 16.6#

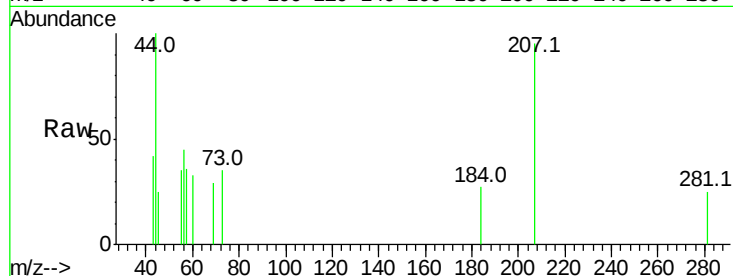

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

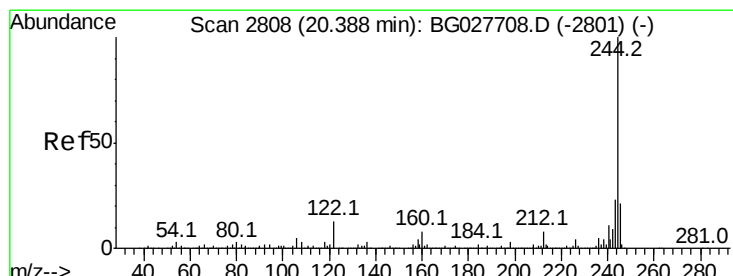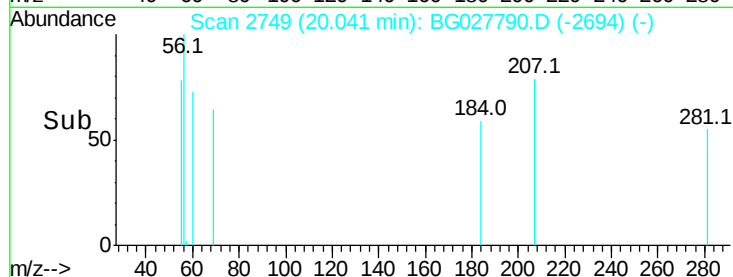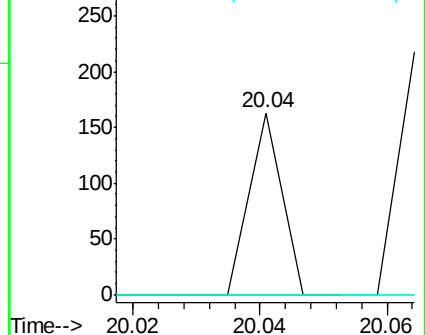

#78

Terphenyl-d14

Concen: 112.94 ng

RT: 20.39 min Scan# 2809

Delta R.T. 0.01 min

Lab File: BG027790.D

Acq: 1 Jul 2017 19:12


Tgt Ion:244 Resp: 1211863

Ion Ratio Lower Upper

244 100

212 7.6 10.0 15.0#



122 11.1 8.6 12.8

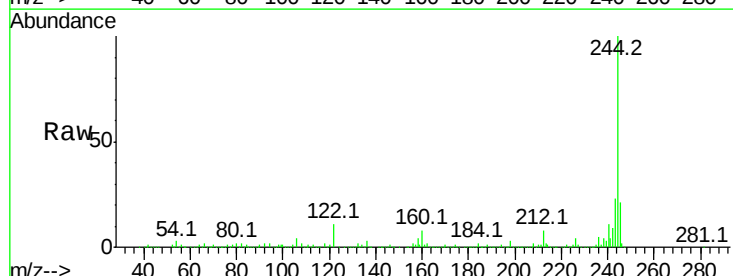


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

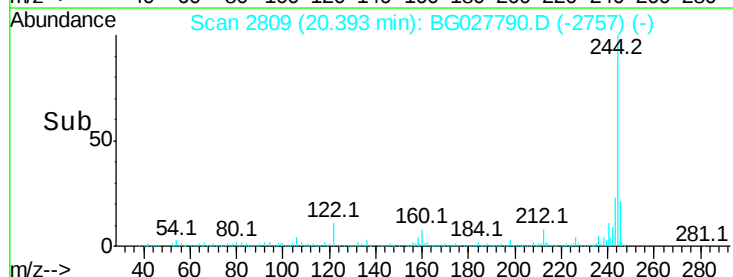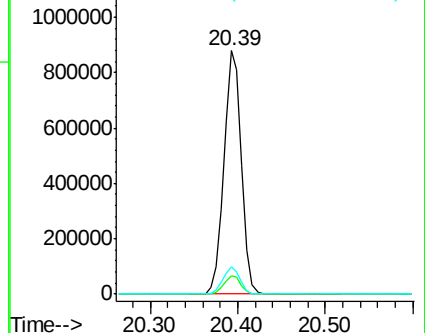

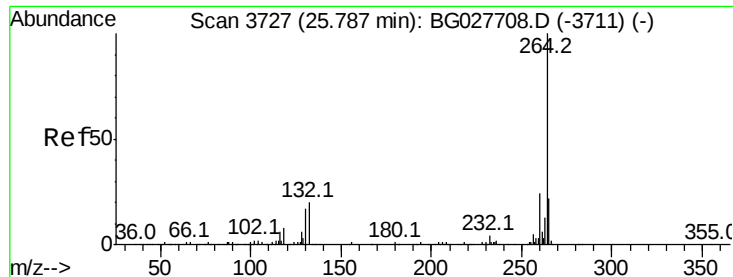

#86
Pervlene-d12
Concen: 20.00 ng
RT: 25.79 min Scan# 3728
Delta R.T. 0.01 min
Lab File: BG027790.D
Acq: 1 Jul 2017 19:12

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.2	21.8	32.8
265	20.9	18.2	27.4

