

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070117\
 Data File : BG027787.D
 Acq On : 1 Jul 2017 17:12
 Operator : SJ/JU
 Sample : I3980-12
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP-D-COMP

Quant Time: Jul 01 18:10:43 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 28 19:26:37 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.48	152	29379	20.00	ng	0.00
21) Naphthalene-d8	11.30	136	141284	20.00	ng	0.00
38) Acenaphthene-d10	15.06	164	92243	20.00	ng	0.00
63) Phenanthrene-d10	17.82	188	238457	20.00	ng	0.00
75) Chrysene-d12	22.18	240	243500	20.00	ng	0.00
86) Perylene-d12	25.80	264	239973	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.06	112	259645	136.09	ng	0.00
7) Phenol-d6	7.62	99	321952	110.46	ng	0.00
23) Nitrobenzene-d5	9.64	82	235290	92.83	ng	0.00
41) 2,4,6-Tribromophenol	16.56	330	235806	186.38	ng	0.00
44) 2-Fluorobiphenyl	13.69	172	626118	96.94	ng	0.00
78) Terphenyl-d14	20.40	244	1171482	112.79	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG070117\
Data File : BG027787.D
Acq On : 1 Jul 2017 17:12
Operator : SJ/JU
Sample : I3980-12
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-D-COMP

Quant Time: Jul 01 18:10:43 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 28 19:26:37 2017
Response via : Initial Calibration

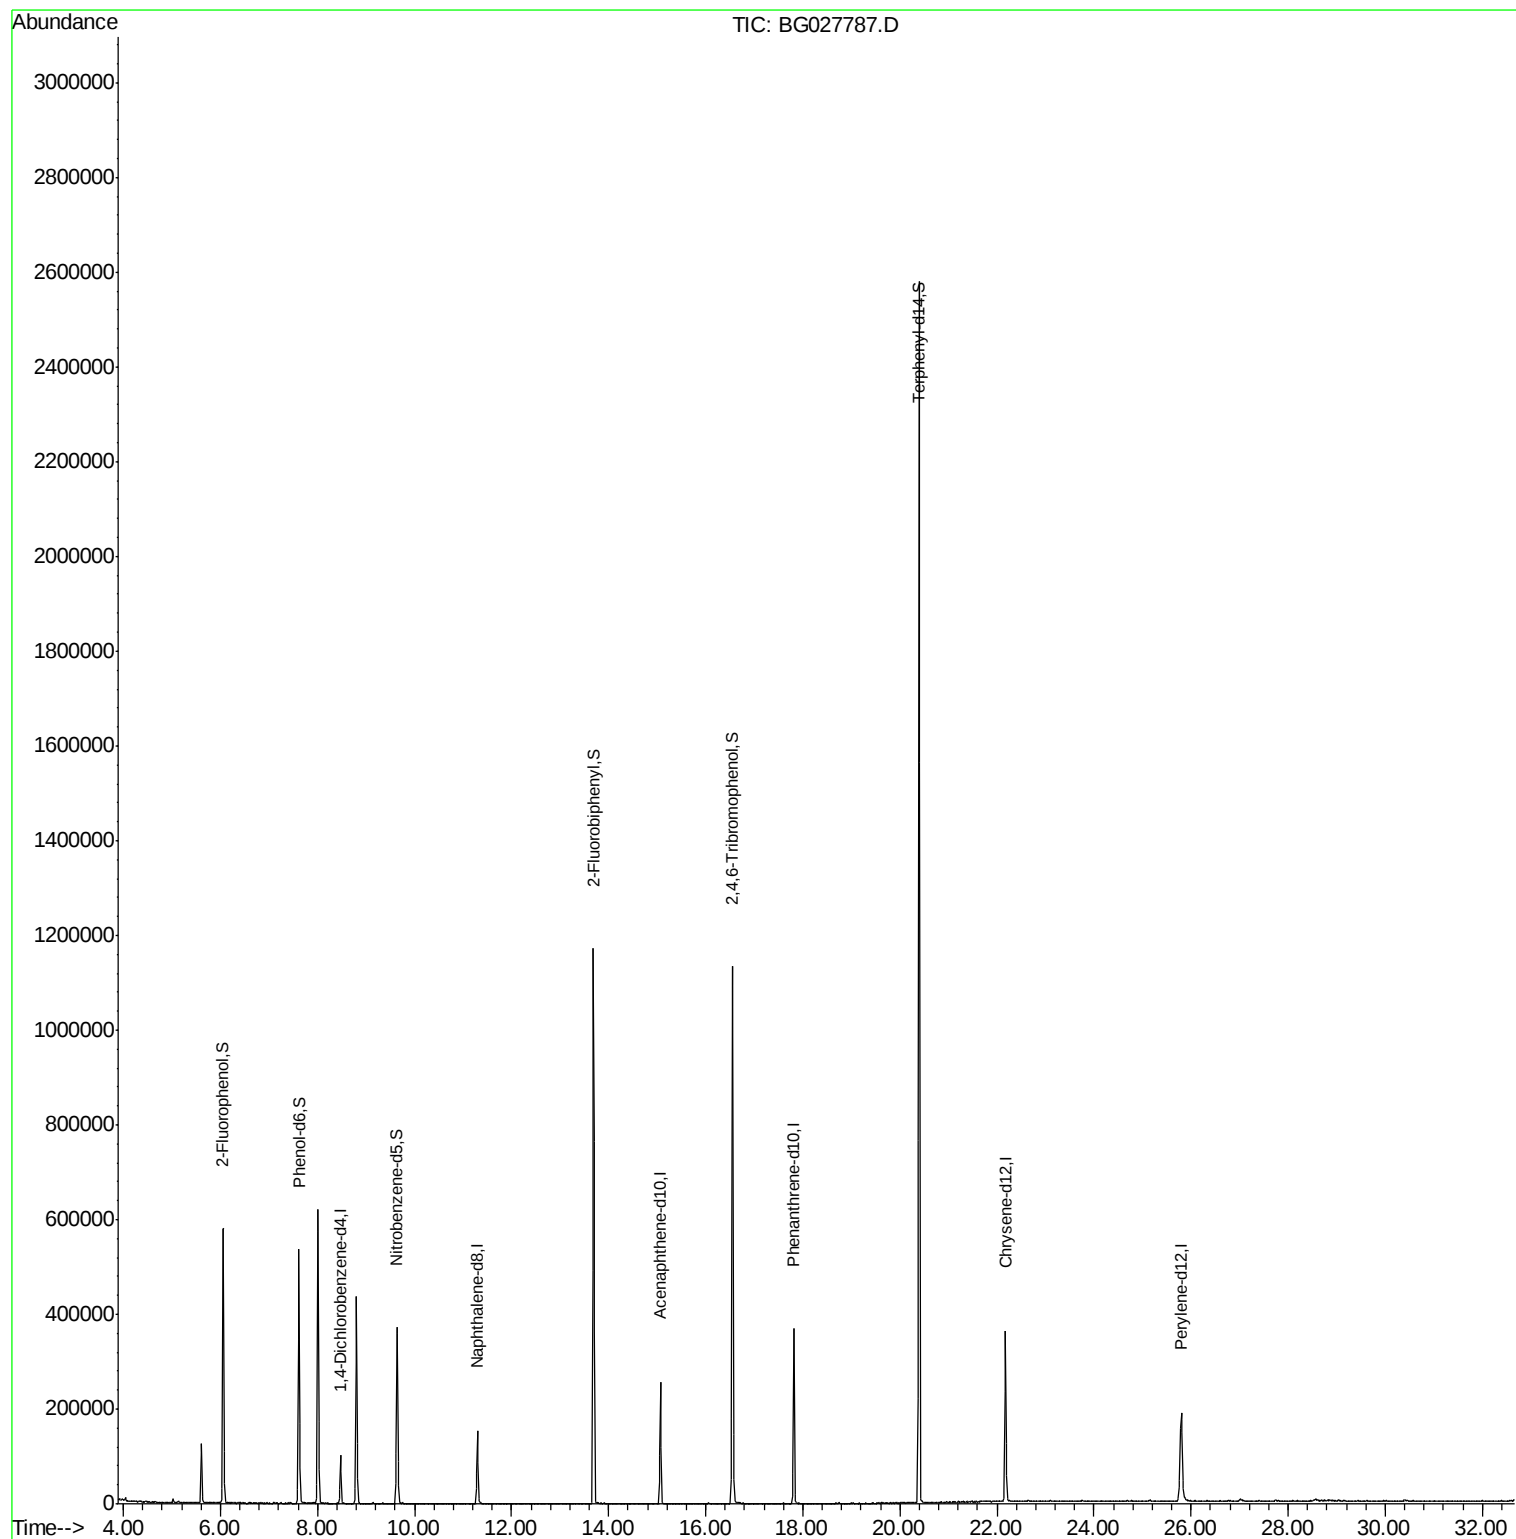


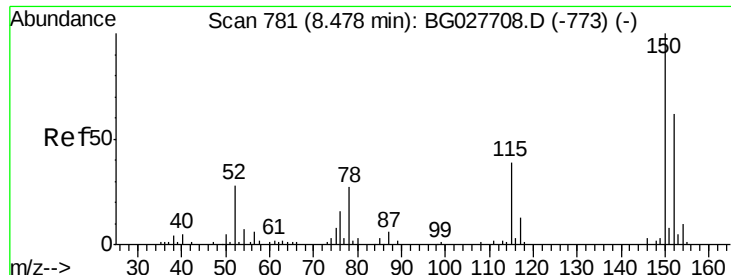




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.48 min Scan# 781
Delta R.T. -0.00 min
Lab File: BG027787.D
Acq: 1 Jul 2017 17:12

Instrument :
BNA_G
ClientSampleId :
SP-D-COMP

Tgt Ion:152 Resp: 29379
Ion Ratio Lower Upper
152 100
150 166.7 114.0 171.0
115 59.0 48.1 72.1

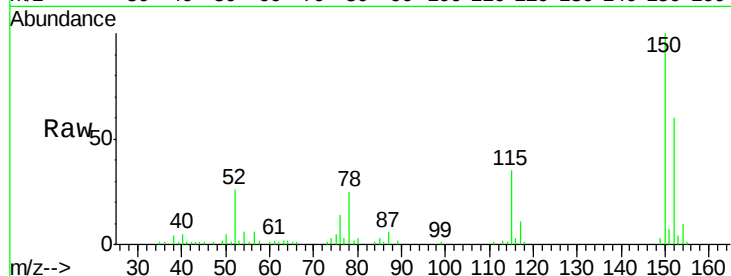


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

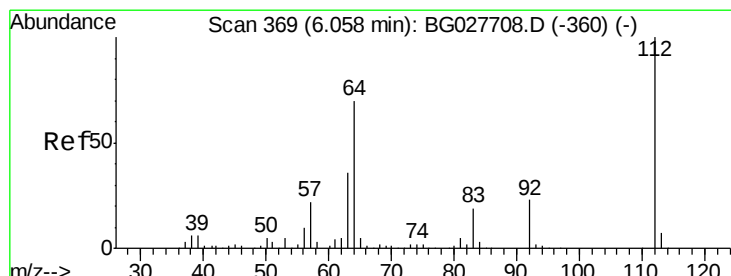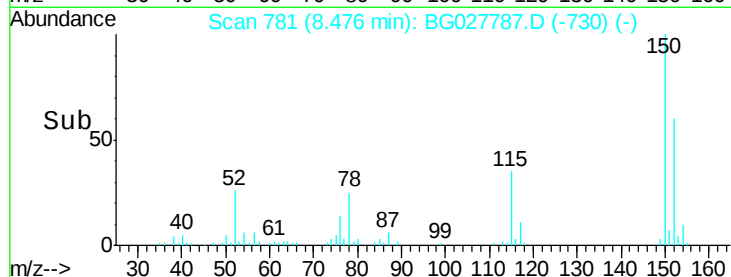
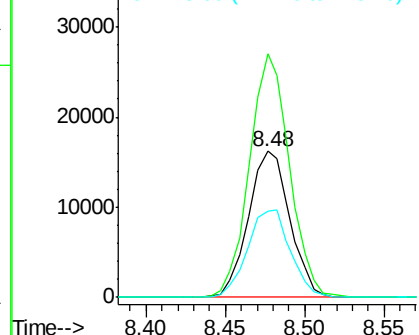



#5
2-Fluorophenol
Concen: 136.094 ng
RT: 6.06 min Scan# 370
Delta R.T. 0.00 min
Lab File: BG027787.D
Acq: 1 Jul 2017 17:12

Tgt Ion:112 Resp: 259645
Ion Ratio Lower Upper
112 100
64 71.1 61.8 92.6
63 36.8 37.2 55.8#

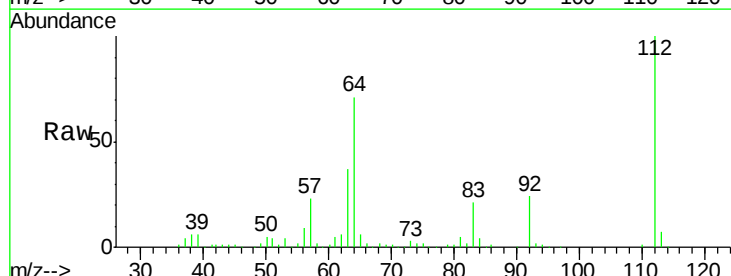

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

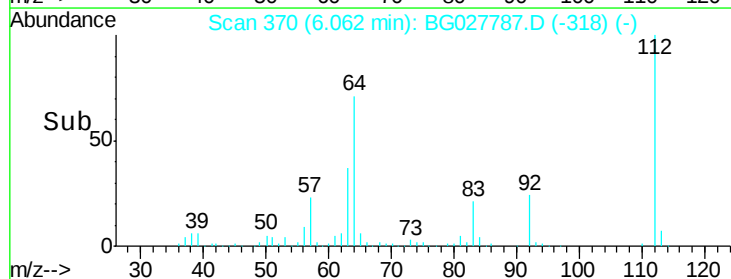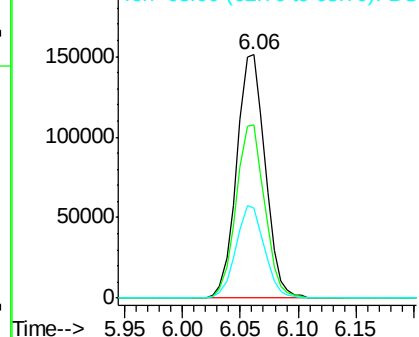

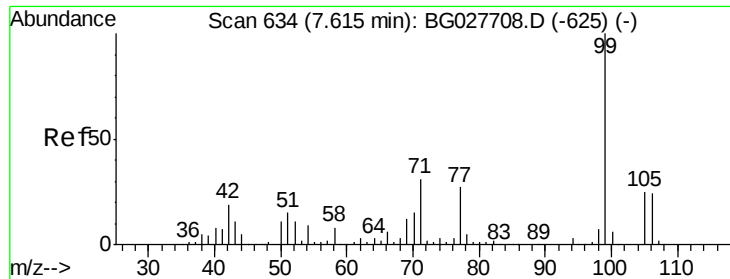

#7

Phenol-d6

Concen: 110.462 ng

RT: 7.62 min Scan# 635

Delta R.T. 0.00 min

Lab File: BG027787.D

Acq: 1 Jul 2017 17:12

Instrument :

BNA_G

ClientSampleId :

SP-D-COMP


Tgt Ion: 99 Resp: 321952

Ion Ratio Lower Upper




99 100

42 20.1 20.5 30.7#

71 35.9 37.6 56.4#

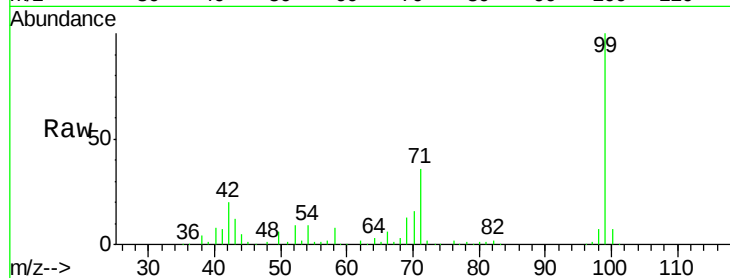

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

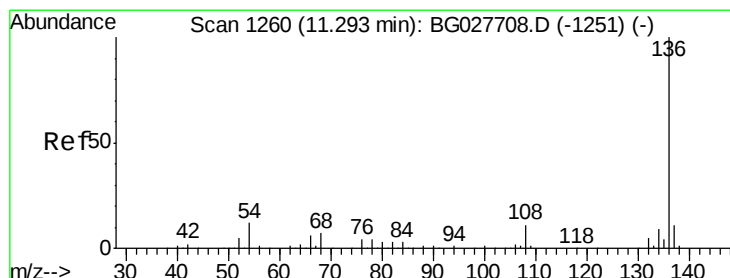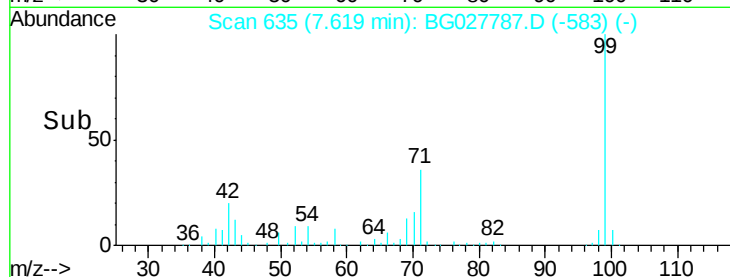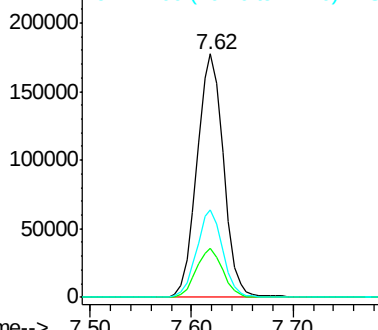

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.30 min Scan# 1261

Delta R.T. 0.00 min

Lab File: BG027787.D

Acq: 1 Jul 2017 17:12

Tgt Ion: 136 Resp: 141284


Ion Ratio Lower Upper

136 100



137 11.2 8.9 13.3


54 10.7 9.3 13.9

68 5.5 5.1 7.7

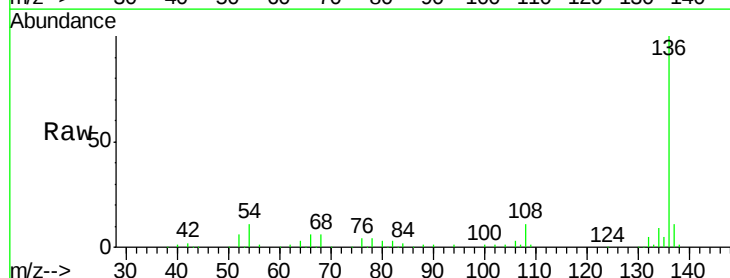

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



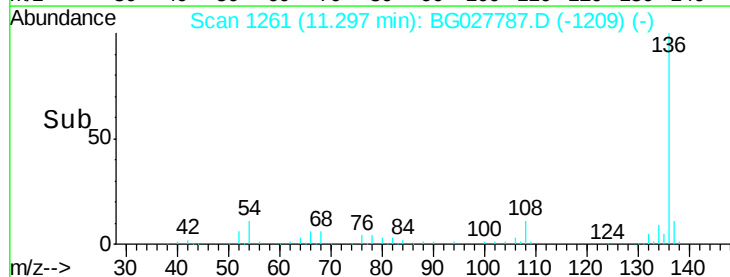
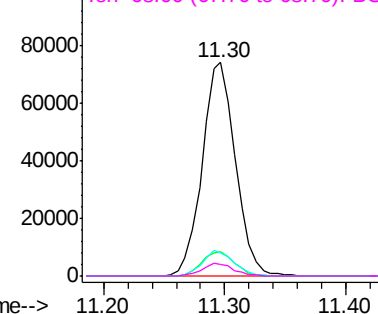


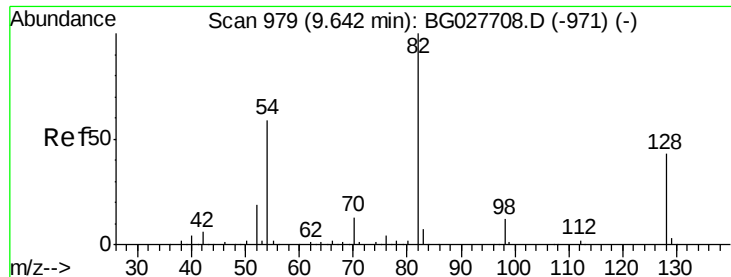

#23
 Nitrobenzene-d5
 Concen: 92.829 ng
 RT: 9.64 min Scan# 979
 Delta R.T. -0.00 min
 Lab File: BG027787.D
 Acq: 1 Jul 2017 17:12




Instrument :
 BNA_G
 ClientSampleId :
 SP-D-COMP


Tgt Ion: 82 Resp: 235290
 Ion Ratio Lower Upper
 82 100
 128 40.5 26.4 39.6#
 54 60.5 49.4 74.2

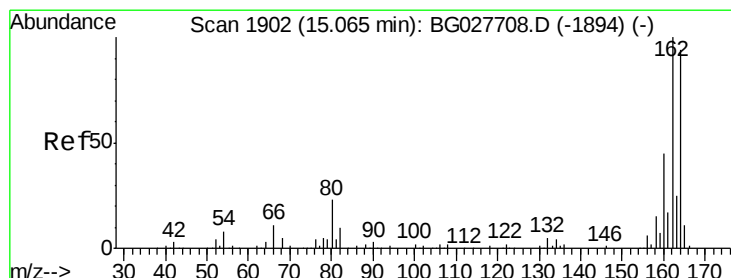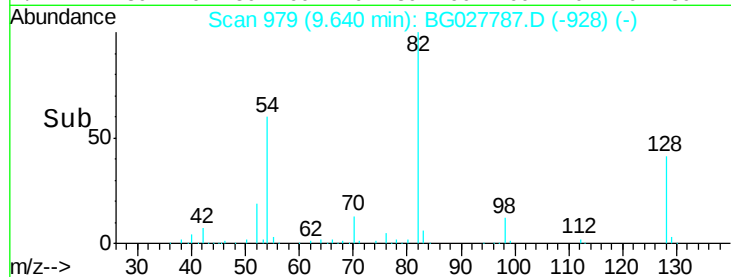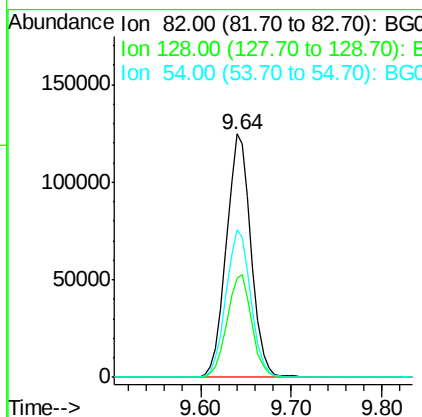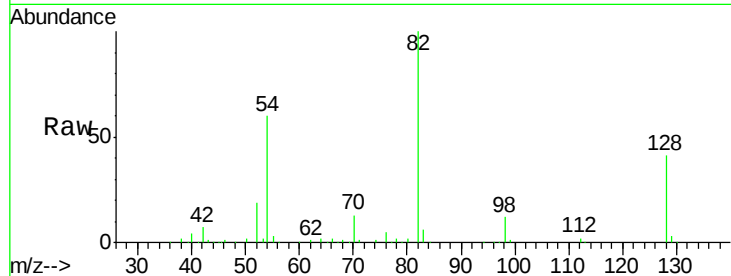

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.06 min Scan# 1902
 Delta R.T. -0.00 min
 Lab File: BG027787.D
 Acq: 1 Jul 2017 17:12

Tgt Ion: 164 Resp: 92243
 Ion Ratio Lower Upper
 164 100
 162 105.6 85.1 127.7
 160 48.6 34.7 52.1

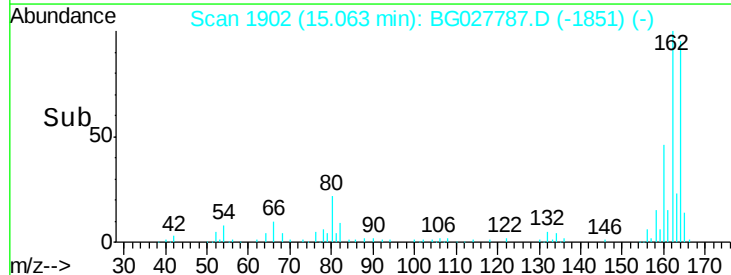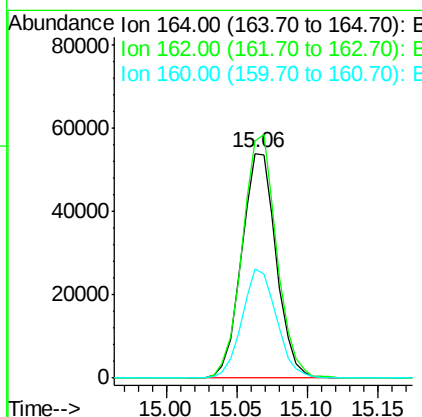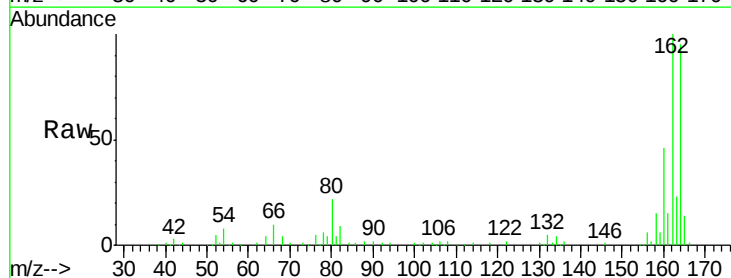


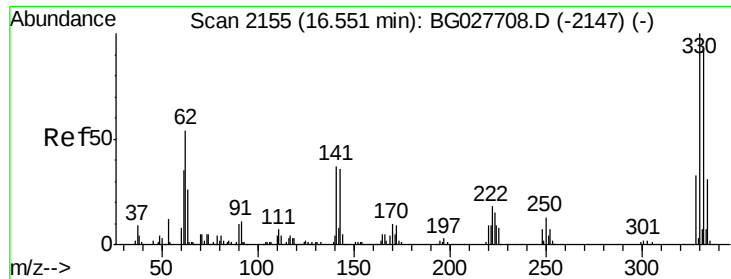




#41
 2,4,6-Tribromophenol
 Concen: 186.377 ng
 RT: 16.56 min Scan# 2156
 Delta R.T. 0.00 min
 Lab File: BG027787.D
 Acq: 1 Jul 2017 17:12

Instrument :
 BNA_G
 ClientSampleId :
 SP-D-COMP

Tgt Ion:330 Resp: 235806
 Ion Ratio Lower Upper
 330 100
 332 95.7 77.3 115.9
 141 35.2 32.1 48.1

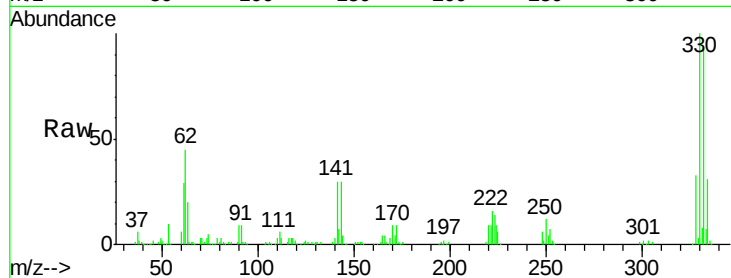


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

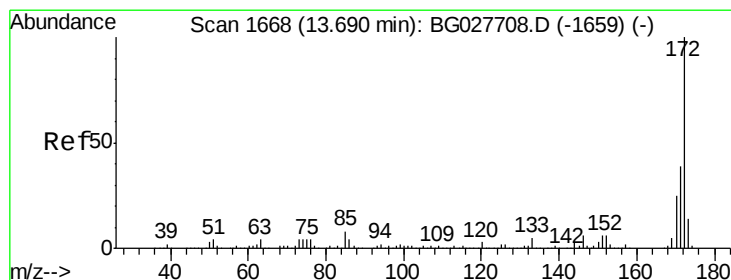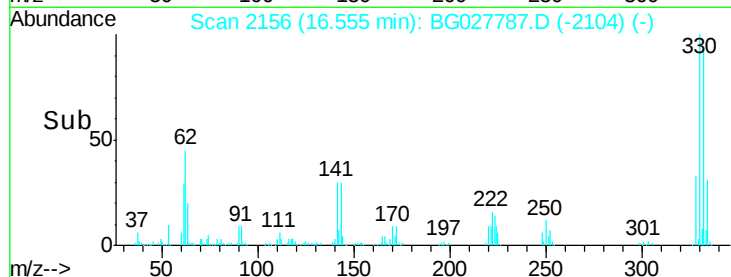
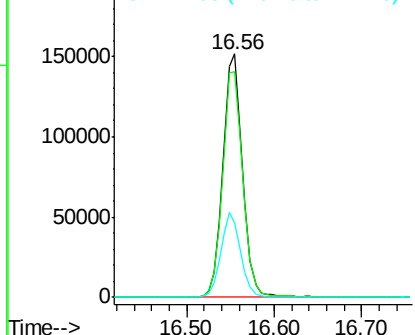



#44
 2-Fluorobiphenyl
 Concen: 96.940 ng
 RT: 13.69 min Scan# 1668
 Delta R.T. -0.00 min
 Lab File: BG027787.D
 Acq: 1 Jul 2017 17:12

Tgt Ion:172 Resp: 626118
 Ion Ratio Lower Upper
 172 100
 171 37.3 32.2 48.2
 170 23.8 21.8 32.6

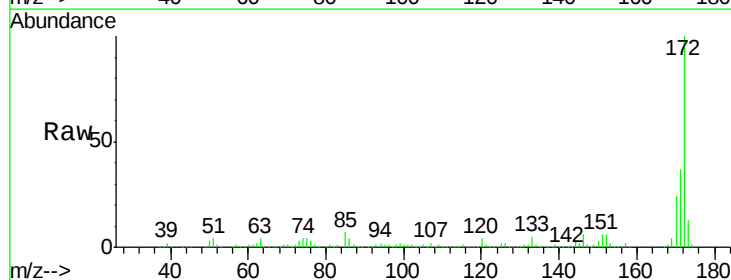

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

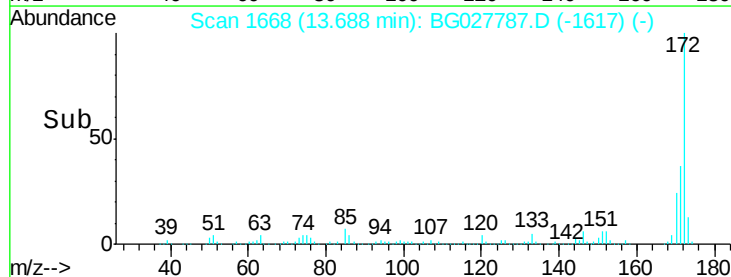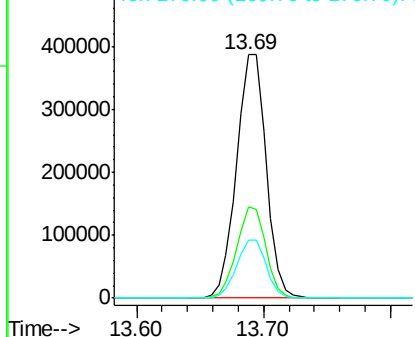


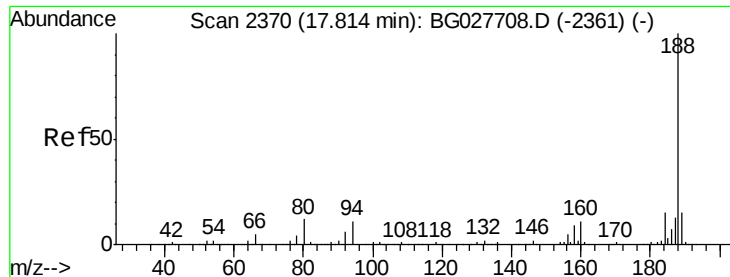




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.82 min Scan# 2371
Delta R.T. 0.00 min
Lab File: BG027787.D
Acq: 1 Jul 2017 17:12

Instrument :
BNA_G
ClientSampleId :
SP-D-COMP

Tgt Ion:188 Resp: 238457
Ion Ratio Lower Upper
188 100
94 8.9 5.8 8.8#
80 9.7 7.5 11.3

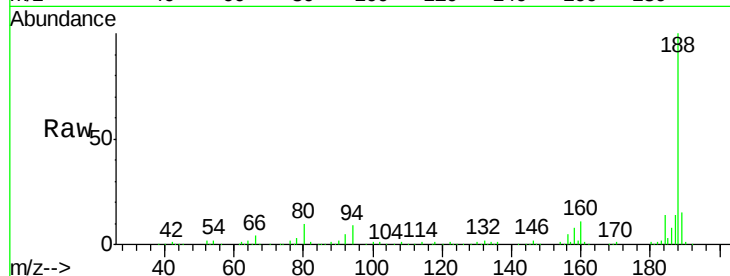


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

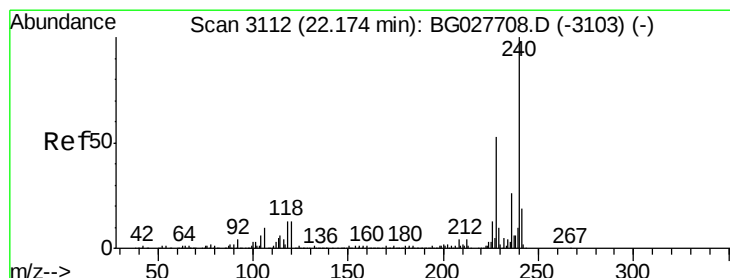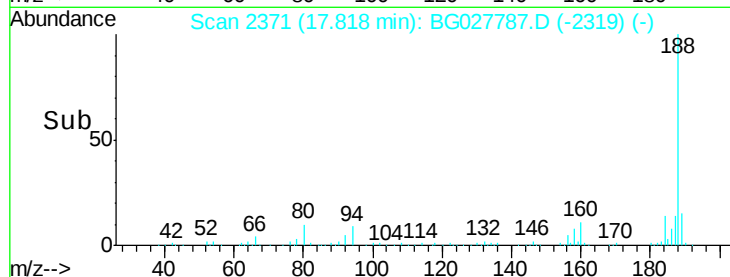
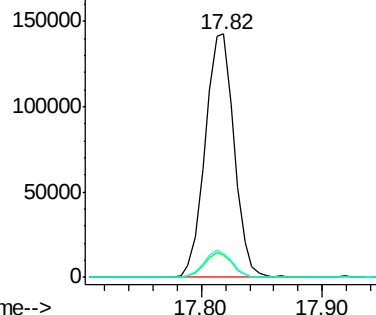



#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.18 min Scan# 3113
Delta R.T. 0.00 min
Lab File: BG027787.D
Acq: 1 Jul 2017 17:12

Tgt Ion:240 Resp: 243500
Ion Ratio Lower Upper
240 100
120 11.0 5.7 8.5#
236 25.9 22.2 33.4

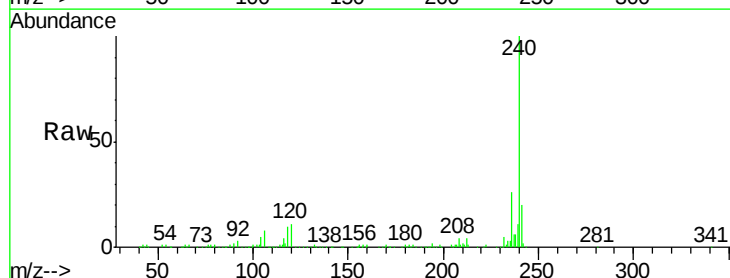

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

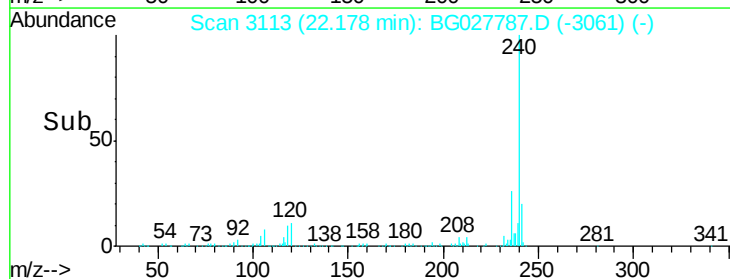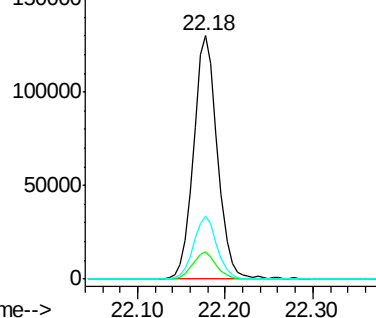

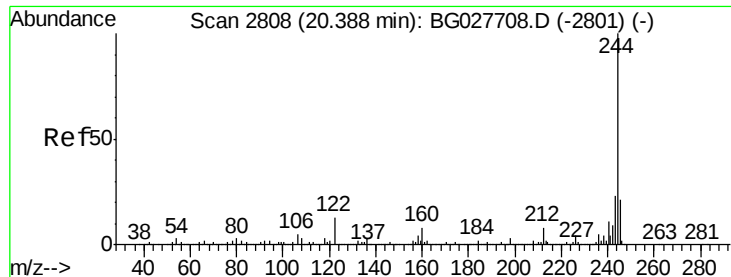

#78

Terphenyl-d14

Concen: 112.788 ng

RT: 20.40 min Scan# 2810

Delta R.T. 0.01 min

Lab File: BG027787.D

Acq: 1 Jul 2017 17:12

Instrument :

BNA_G

ClientSampled :

SP-D-COMP


Tgt Ion:244 Resp: 1171482

Ion Ratio Lower Upper

244 100

212 7.5 10.0 15.0#




122 10.2 8.6 12.8

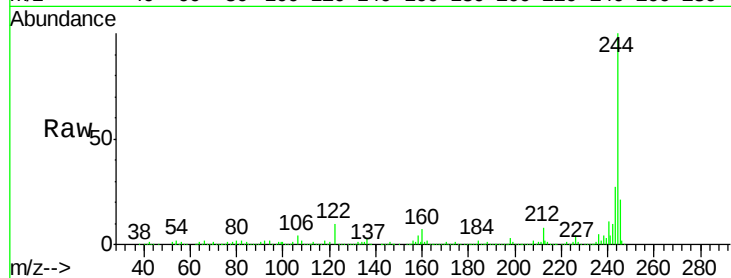

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

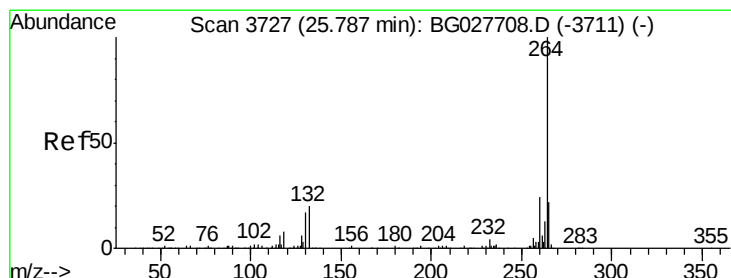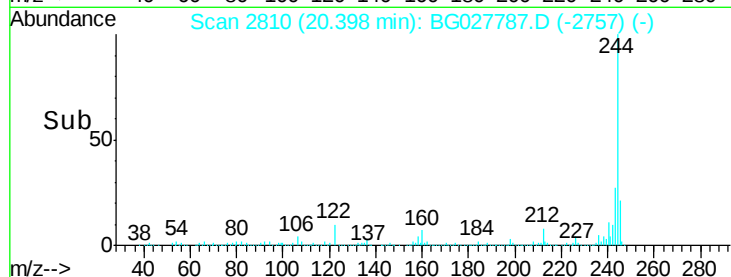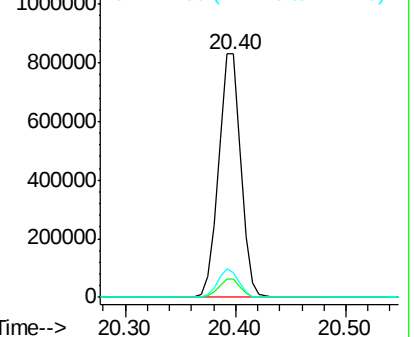

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.80 min Scan# 3729

Delta R.T. 0.01 min

Lab File: BG027787.D

Acq: 1 Jul 2017 17:12


Tgt Ion:264 Resp: 239973

Ion Ratio Lower Upper

264 100

260 22.1 21.8 32.8

265 19.7 18.2 27.4

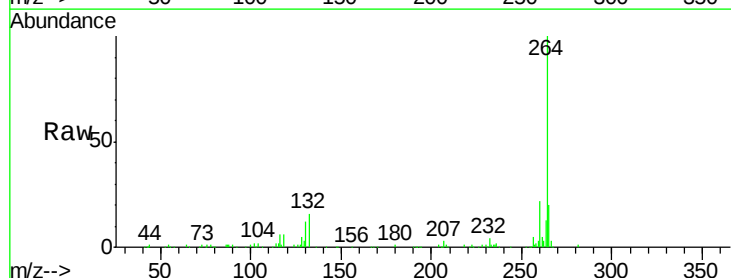

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

