


Data Path : Z:\HPCHEM1\BNA_G\Data\BG070117\
 Data File : BG027774.D
 Acq On : 1 Jul 2017 7:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 19:26:37 2017

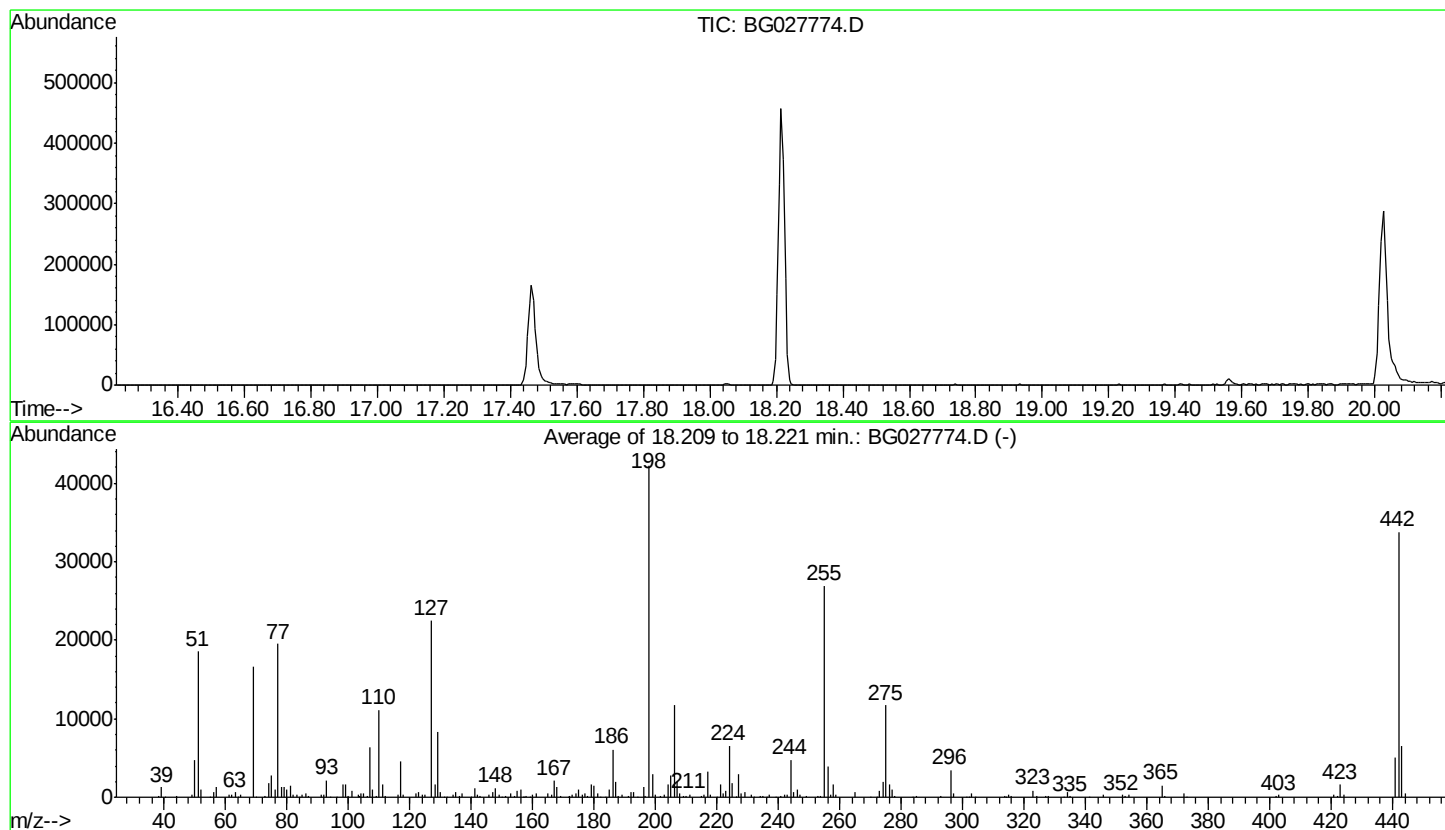

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	18534	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.5	16683	PASS
70	69	0.00	2	0.3	58	PASS
127	198	10	80	53.1	22434	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42240	PASS
199	198	5	9	7.0	2972	PASS
275	198	10	60	27.7	11709	PASS
365	198	1	100	3.5	1497	PASS
441	442	0.01	24	14.9	5020	PASS
442	198	50	100	79.9	33768	PASS
443	442	15	24	19.3	6503	PASS