


Data Path : Z:\HPCHEM1\BNA_G\Data\BG070117\
 Data File : BG027792.D
 Acq On : 1 Jul 2017 20:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG062817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 28 19:26:37 2017

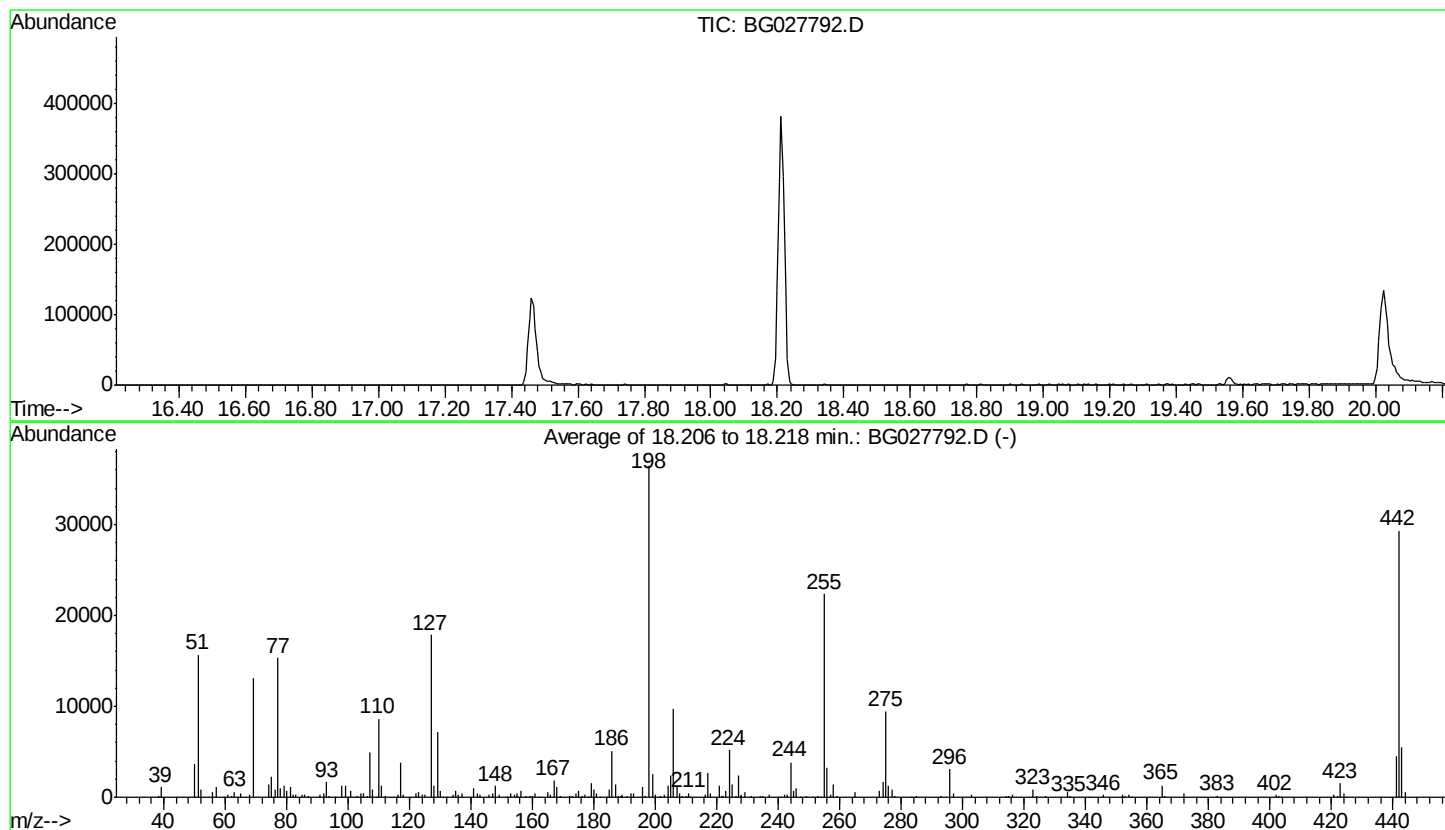

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	15702	PASS
68	69	0.00	2	1.7	225	PASS
69	198	0.00	100	36.0	13126	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	17868	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	36480	PASS
199	198	5	9	7.1	2581	PASS
275	198	10	60	25.8	9399	PASS
365	198	1	100	3.5	1289	PASS
441	442	0.01	24	15.2	4459	PASS
442	198	50	100	80.5	29354	PASS
443	442	15	24	19.0	5564	PASS